

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022122\
 Data File : BP009230.D
 Acq On : 21 Feb 2022 12:28
 Operator : CG/JU
 Sample : PB142358BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB142358BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009230.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.358	398	403	437	rBV	2503356	4740499	39.34%	9.287%
2	6.958	669	675	717	rBV	2197704	4905514	40.71%	9.610%
3	7.763	805	812	827	rBV	575237	1038297	8.62%	2.034%
4	8.928	1003	1010	1051	rBV	1426039	3202212	26.58%	6.273%
5	10.563	1279	1288	1316	rBV	562435	1442789	11.97%	2.827%
6	13.028	1699	1707	1742	rBV	4964443	8664578	71.91%	16.974%
7	14.416	1934	1943	1965	rBV	1048002	2108037	17.49%	4.130%
8	15.922	2192	2199	2255	rBV	2749029	6200614	51.46%	12.147%
9	17.175	2405	2412	2431	rBV	1223377	2512366	20.85%	4.922%
10	19.733	2841	2847	2864	rBV	8439565	12049570	100.00%	23.606%
11	21.280	3105	3110	3124	rBV	1418714	2331363	19.35%	4.567%
12	23.668	3510	3516	3532	rVB2	686717	1849105	15.35%	3.623%




Sum of corrected areas: 51044944

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022122\
Data File : BP009230.D
Acq On : 21 Feb 2022 12:28
Operator : CG/JU
Sample : PB142358BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142358BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

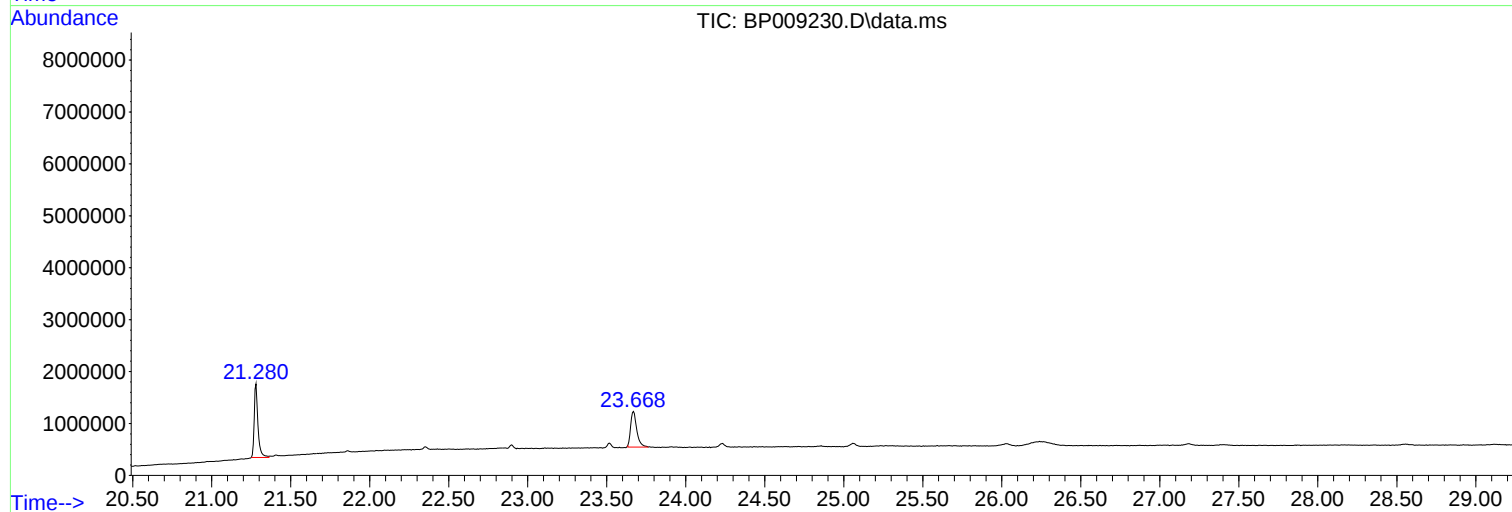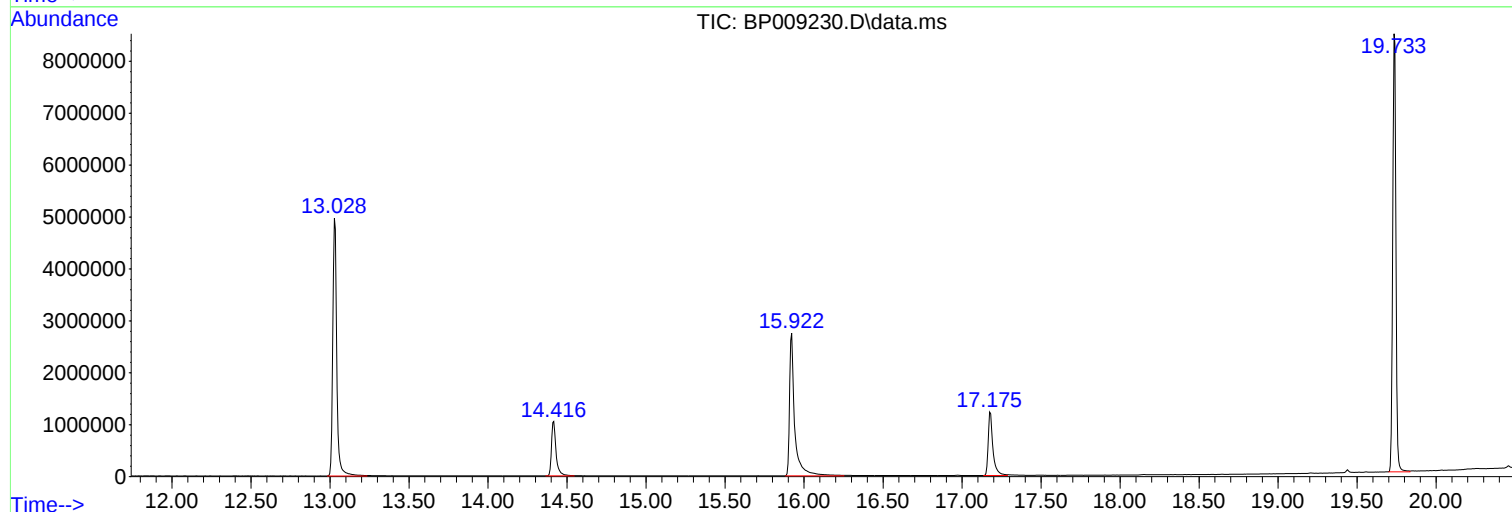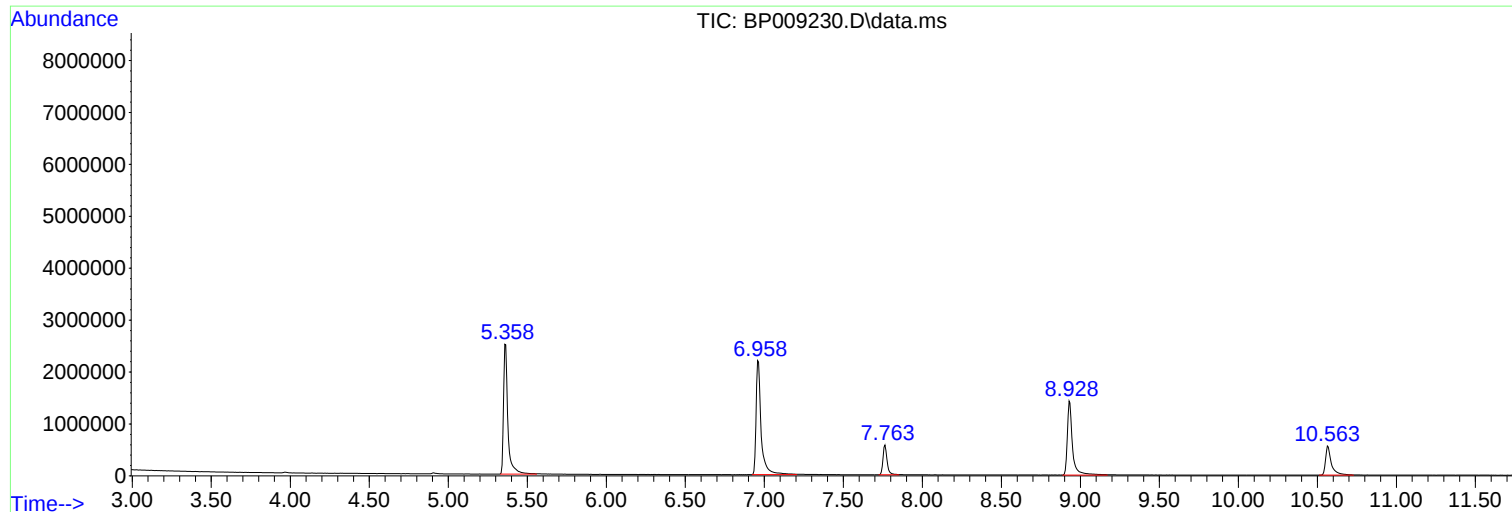

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022122\
Data File : BP009230.D
Acq On : 21 Feb 2022 12:28
Operator : CG/JU
Sample : PB142358BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142358BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022122\
Data File : BP009230.D
Acq On : 21 Feb 2022 12:28
Operator : CG/JU
Sample : PB142358BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142358BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------