
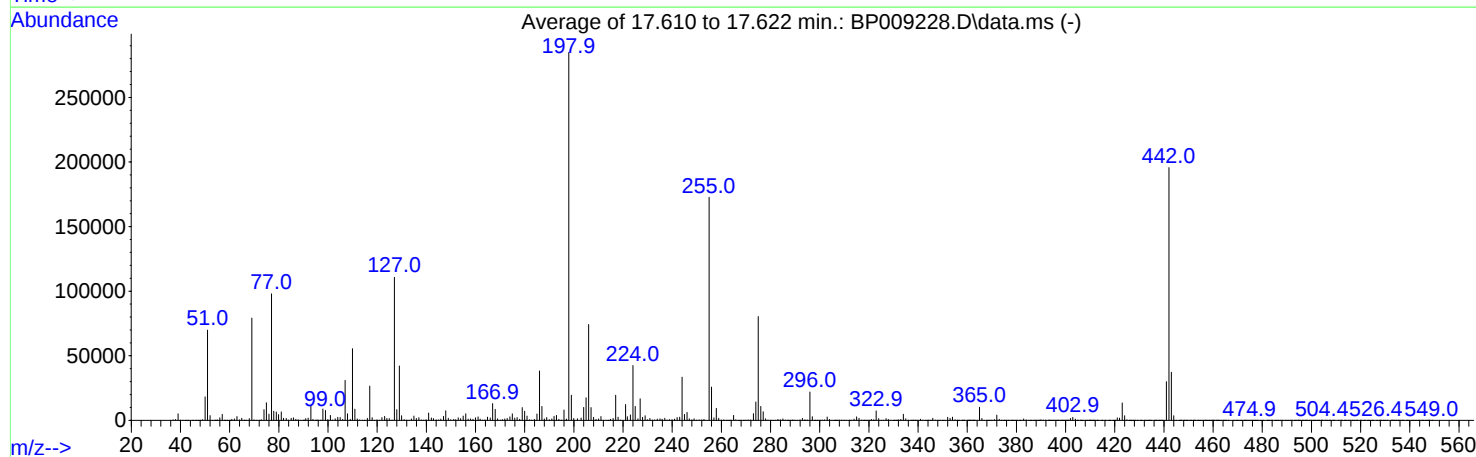


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022122\
 Data File : BP009228.D
 Acq On : 21 Feb 2022 11:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Feb 19 00:46:08 2022

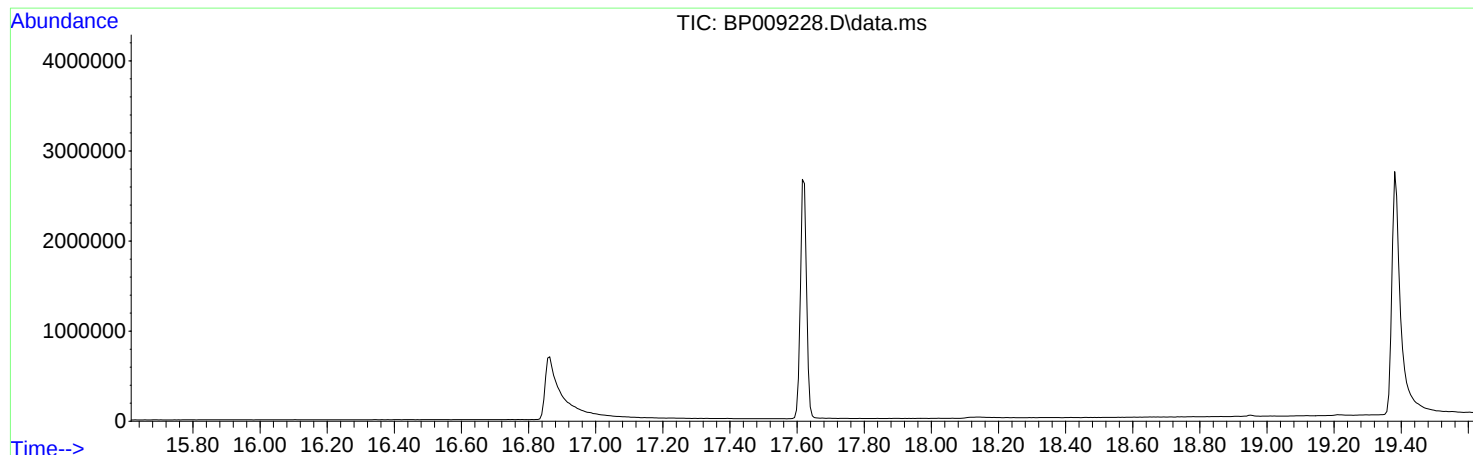




AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.5	69859	PASS
68	69	0.00	2	1.7	1346	PASS
69	198	0.00	100	27.8	79213	PASS
70	69	0.00	2	0.5	432	PASS
127	198	10	80	38.9	110745	PASS
197	198	0.00	2	0.3	983	PASS
198	198	100	100	100.0	284780	PASS
199	198	5	9	6.8	19478	PASS
275	198	10	60	28.2	80448	PASS
365	198	1	100	3.6	10176	PASS
441	198	0.01	100	10.5	29951	PASS
442	442	100	100	100.0	195661	PASS
443	442	15	24	19.1	37352	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022122\
Data File : BP009228.D
Acq On : 21 Feb 2022 11:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 22 02:36:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 19 00:46:08 2022
Response via : Initial Calibration

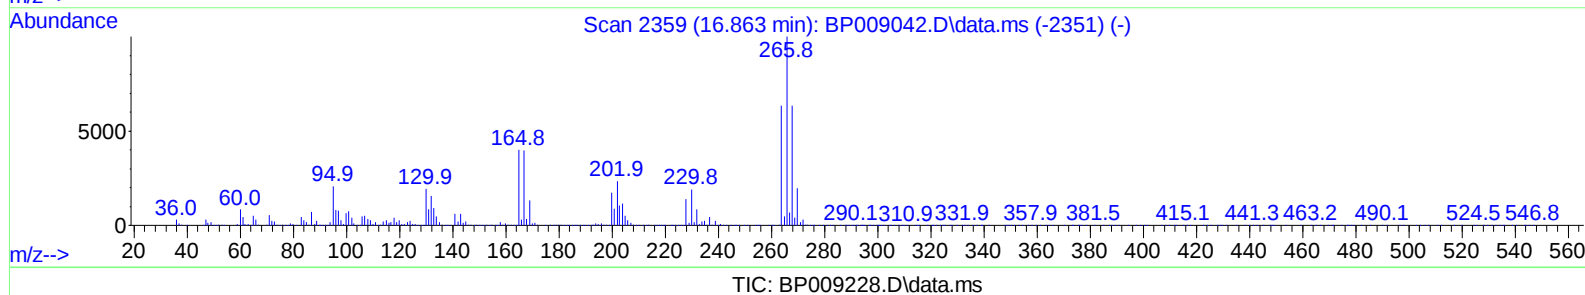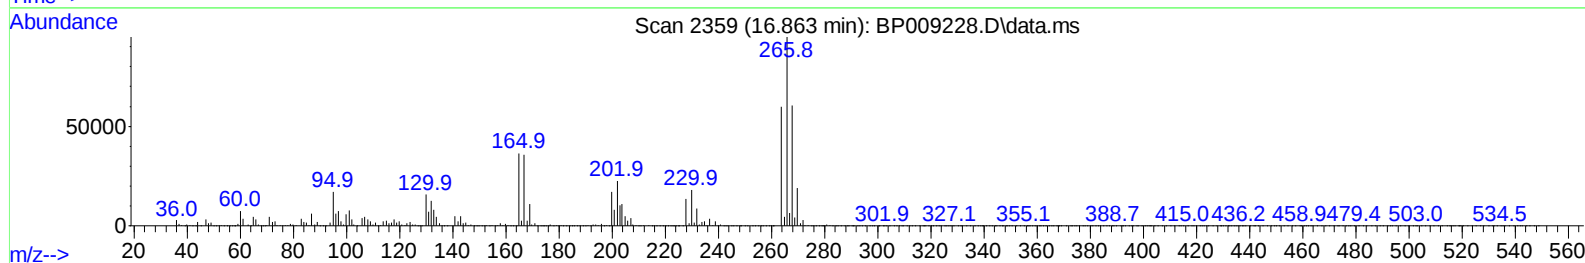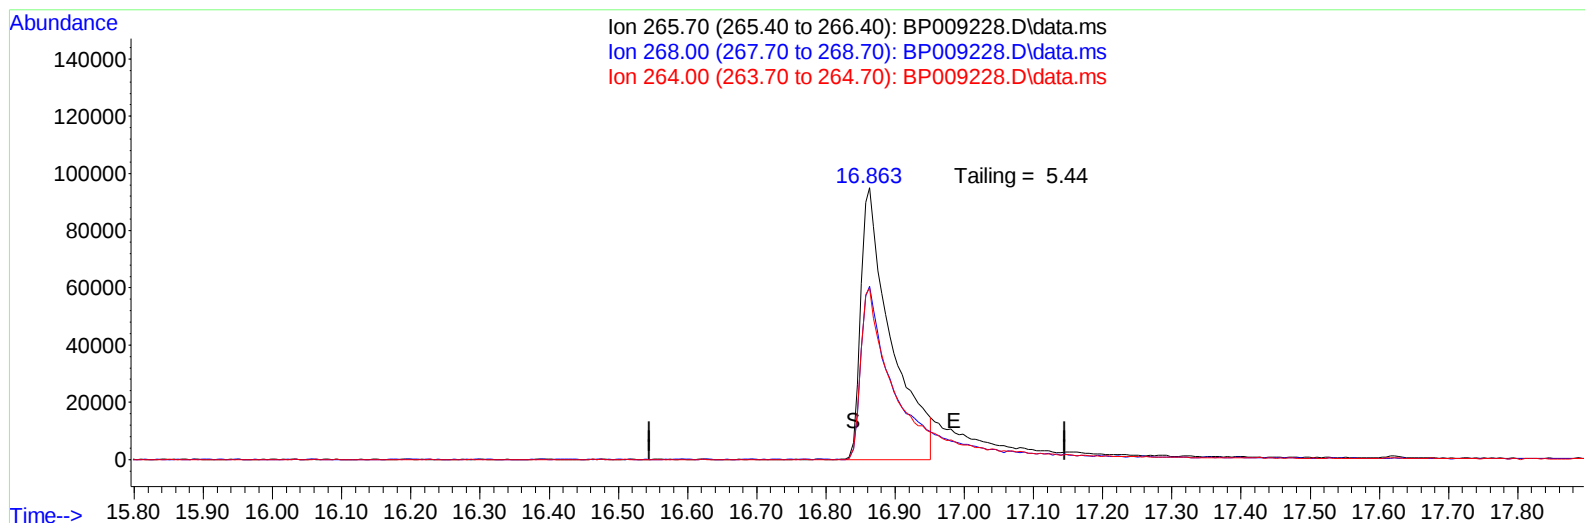

(70) Pentachlorophenol (C)

16.863min (+ 0.018) 430594.86 ng m




response 288421

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.71
264.00	62.90	63.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022122\
Data File : BP009228.D
Acq On : 21 Feb 2022 11:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 22 02:36:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 19 00:46:08 2022
Response via : Initial Calibration

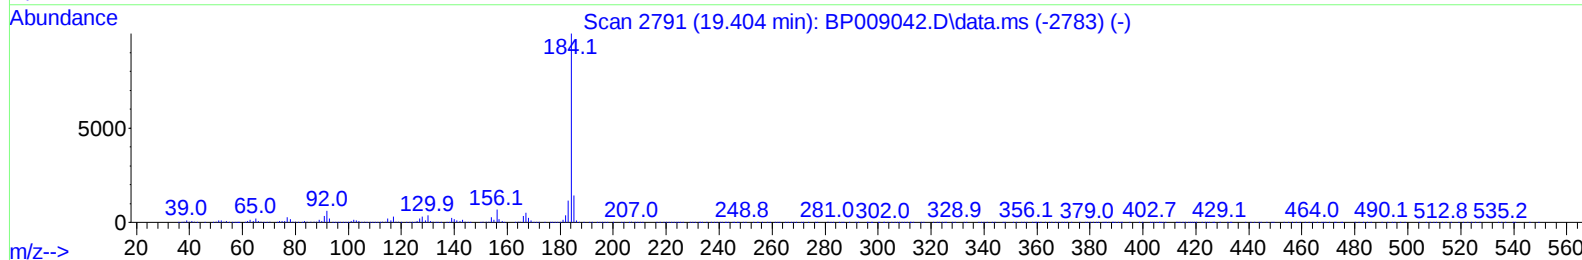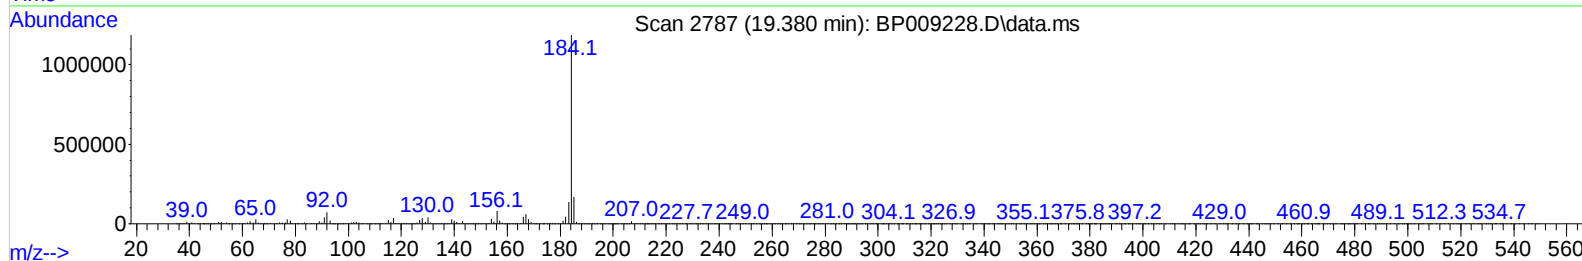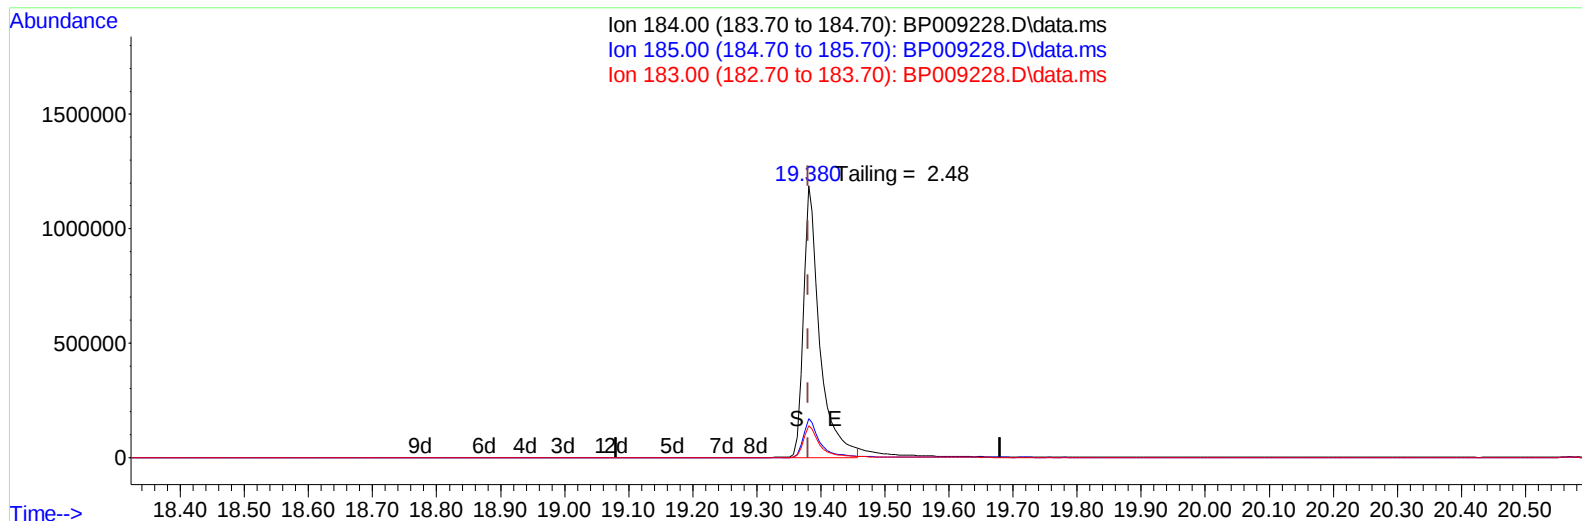

TIC: BP009228.D\data.ms

(77) Benzidine

19.380min (-0.000) 801854.06 ng m

response 2228489

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.39
183.00	11.90	11.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/21/2022	BNA_P	<u>BP009228.D</u>
Compound Name	Response	Retention Time
DDT	1011172	20.569
DDD	20329	20.151
DDE	5843	19.651
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26172	1037344	2.52

Instrument :
BNA_P
ClientSampleId :
DFTPP