
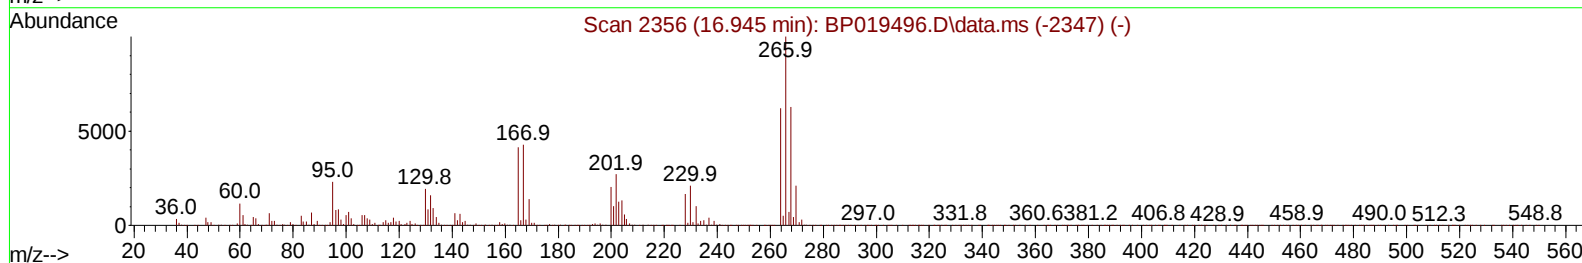
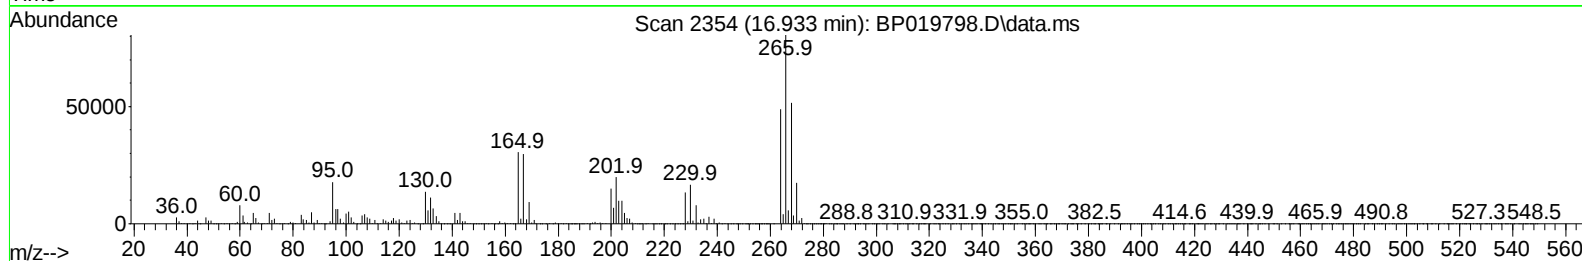


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022124\
Data File : BP019798.D
Acq On : 21 Feb 2024 09:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 01:09:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 19 23:35:42 2024
Response via : Initial Calibration

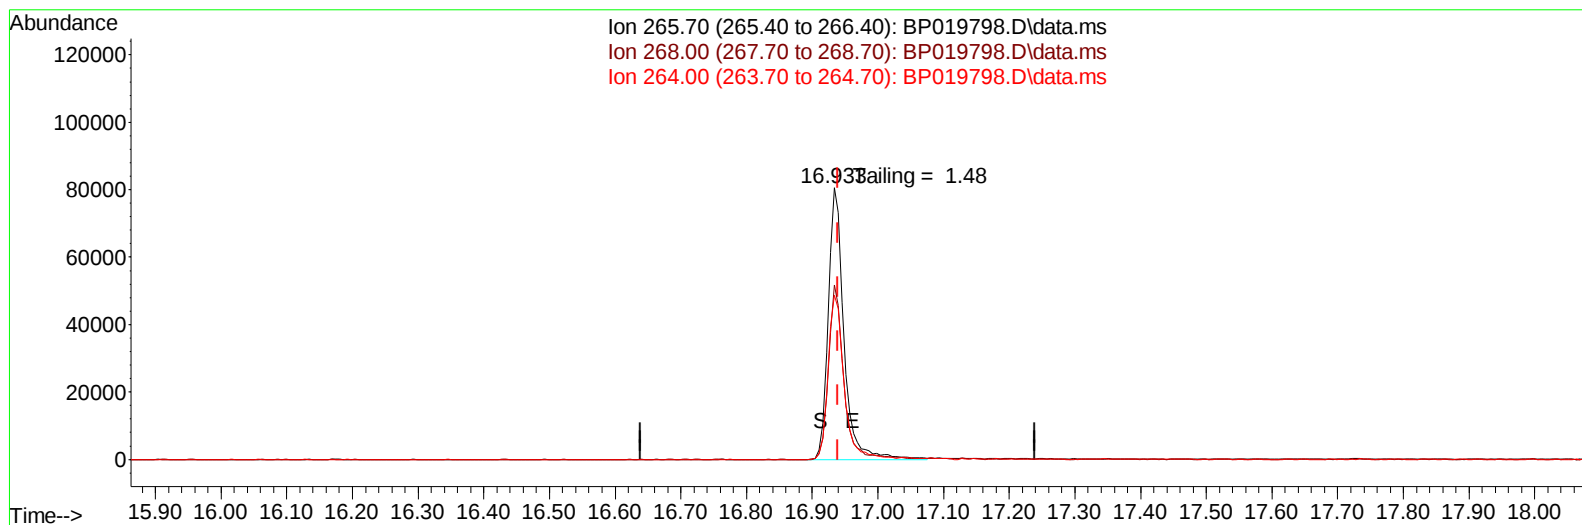

TIC: BP019798.D\data.ms

(70) Pentachlorophenol (C)




16.933min (-0.006) 591328.51 ng

response 134397

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	64.17
264.00	62.10	60.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022124\
Data File : BP019798.D
Acq On : 21 Feb 2024 09:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 01:09:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 19 23:35:42 2024
Response via : Initial Calibration

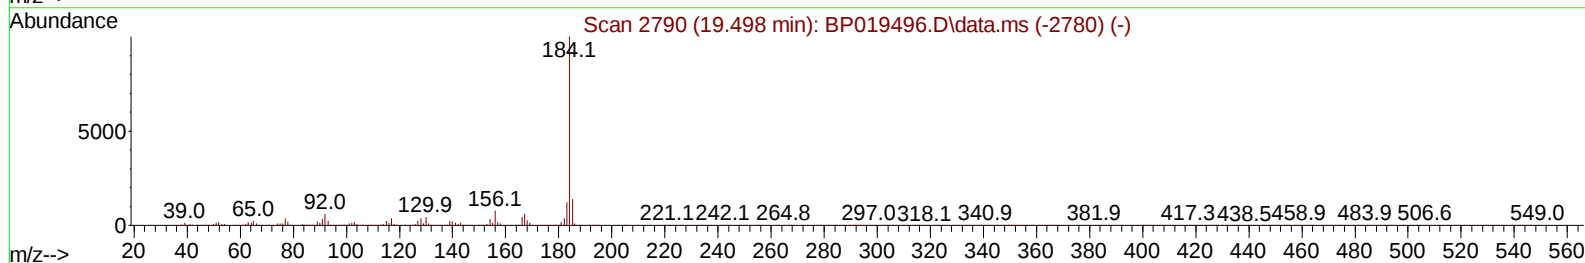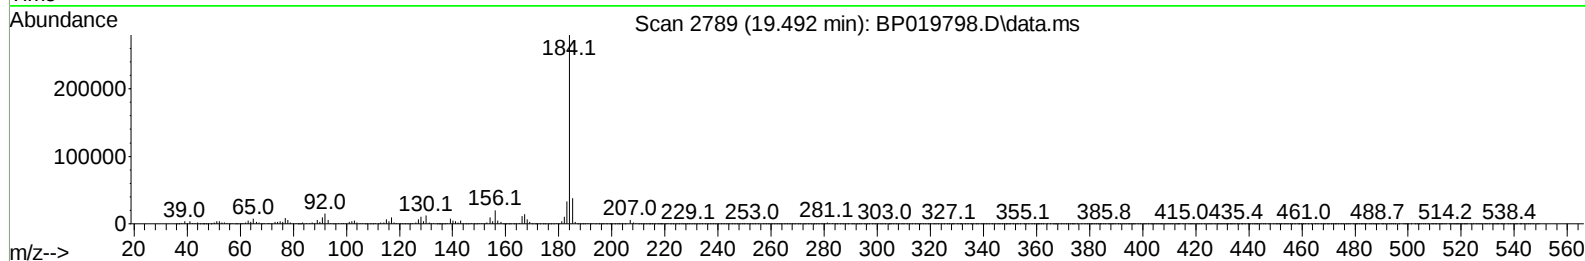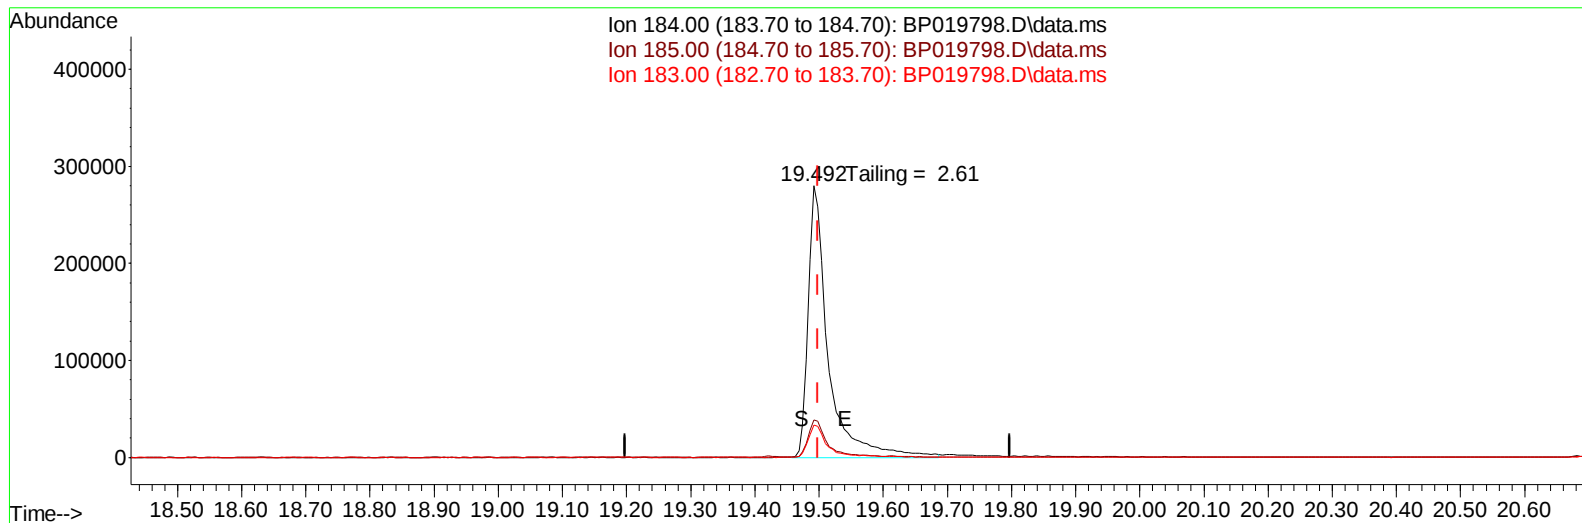

TIC: BP019798.D\data.ms

(77) Benzidine

19.492min (-0.006) 301154.31 ng

response 604429

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.72
183.00	12.10	11.90
0.00	0.00	0.00