

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022124\
 Data File : BP019802.D
 Acq On : 21 Feb 2024 11:43
 Operator : MA/JU
 Sample : PB159144BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB159144BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP019802.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.017	323	328	335	rBV	41442	60863	1.14%	0.289%
2	5.469	398	405	415	rBV	1295057	1949096	36.40%	9.263%
3	7.069	669	677	690	rBV	1120902	1883962	35.18%	8.953%
4	7.893	811	817	827	rBV	263145	429511	8.02%	2.041%
5	9.063	1008	1016	1033	rBV	715384	1283167	23.96%	6.098%
6	10.693	1286	1293	1308	rBV	296315	537133	10.03%	2.553%
7	13.157	1704	1712	1735	rBV	1886770	2969370	55.46%	14.111%
8	14.534	1938	1946	1960	rBV	404031	706477	13.19%	3.357%
9	16.028	2192	2200	2229	rBV	1478070	2616260	48.86%	12.433%
10	17.286	2407	2414	2426	rBV	538802	898850	16.79%	4.272%
11	19.569	2798	2802	2806	rBV	58725	68782	1.28%	0.327%
12	19.857	2844	2851	2862	rBV	4130237	5354515	100.00%	25.446%
13	20.586	2972	2975	2980	rBV3	50240	59802	1.12%	0.284%
14	21.380	3105	3110	3124	rBV2	754380	1156537	21.60%	5.496%
15	23.798	3515	3521	3532	rVB	465470	1068471	19.95%	5.078%




Sum of corrected areas: 21042796

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022124\
Data File : BP019802.D
Acq On : 21 Feb 2024 11:43
Operator : MA/JU
Sample : PB159144BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159144BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

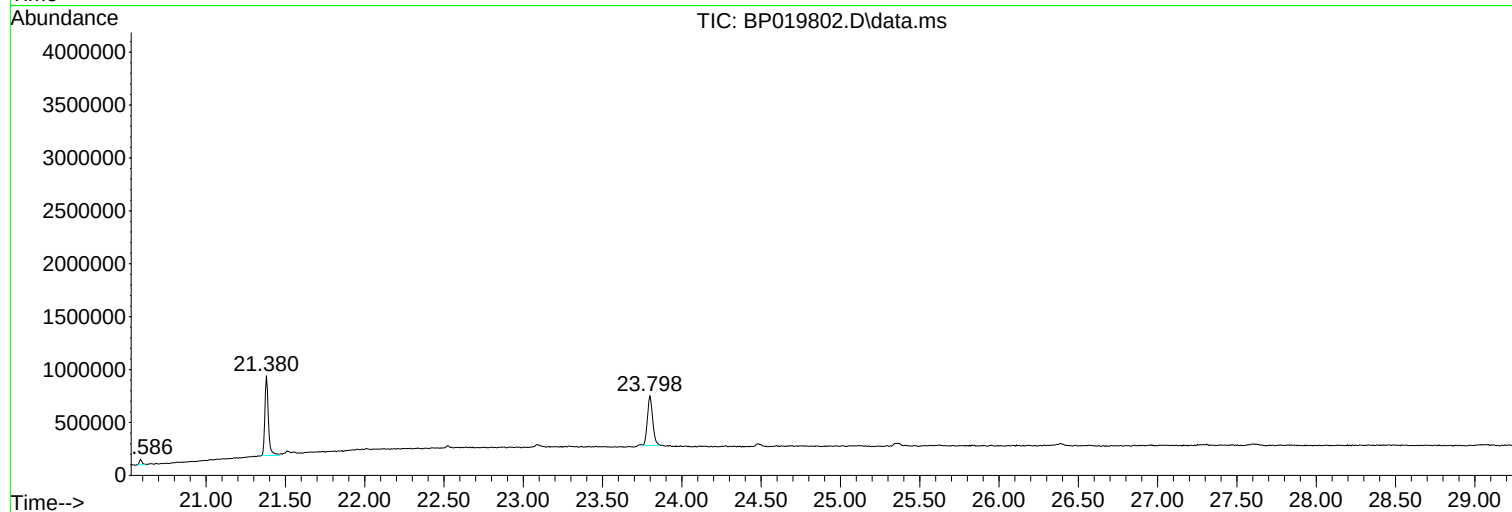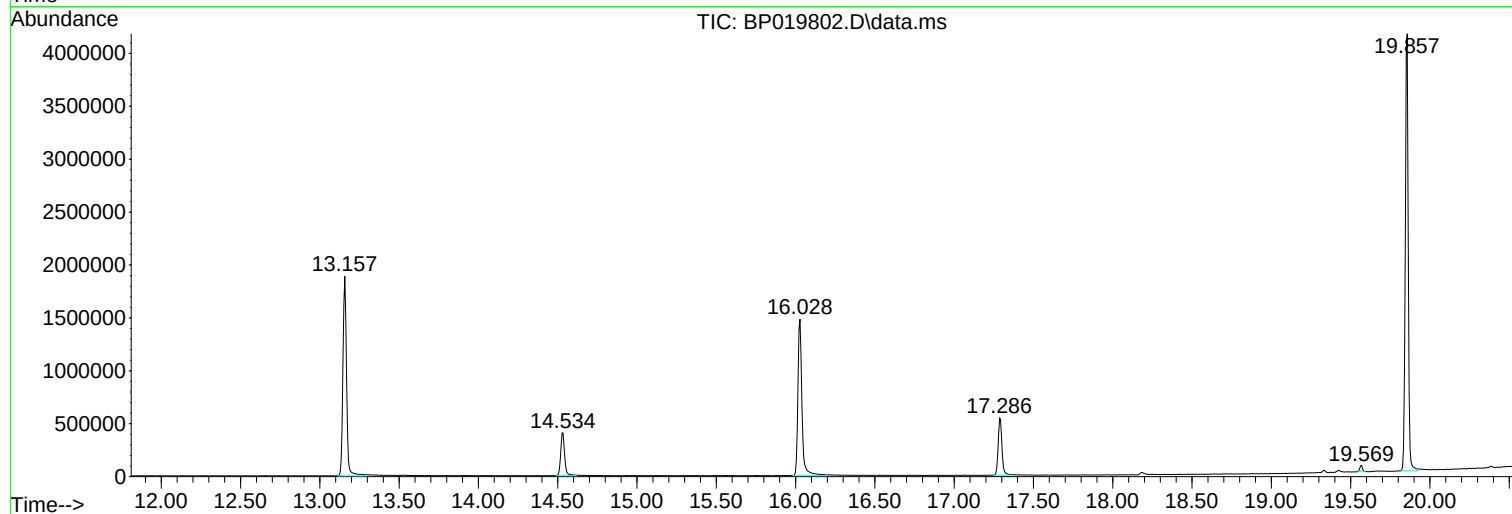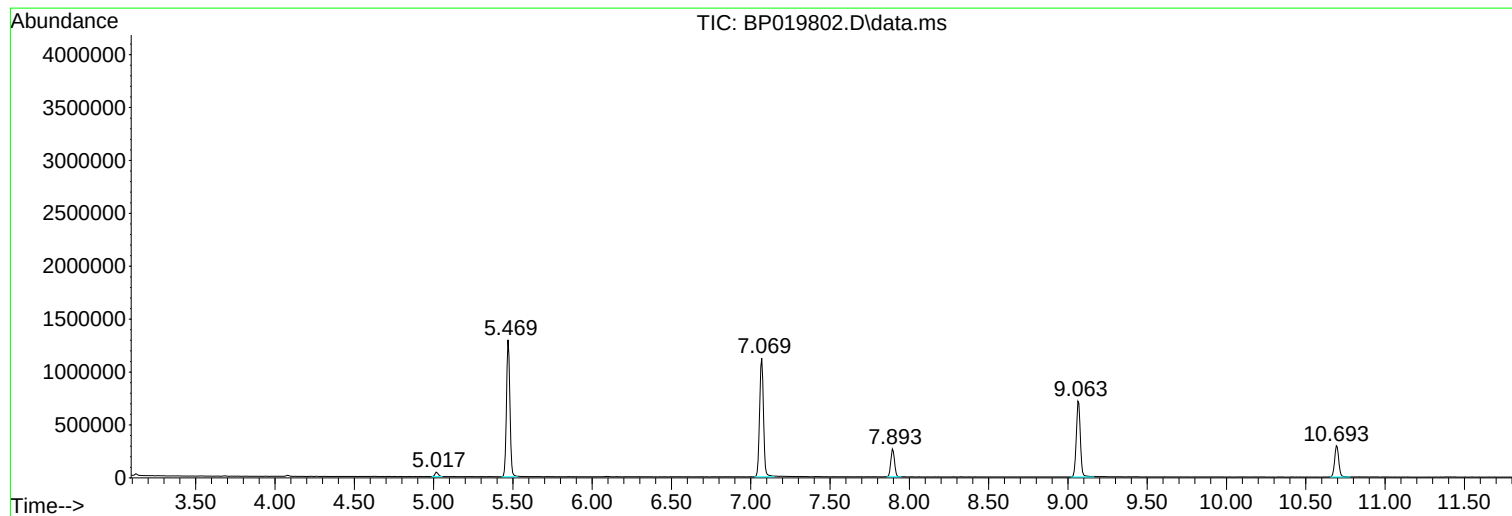

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022124\
Data File : BP019802.D
Acq On : 21 Feb 2024 11:43
Operator : MA/JU
Sample : PB159144BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159144BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.016	2.83 ng	60863	1,4-Dichlorobenzene-d4	7.893

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50		
2	4-Methoxy-1-pentene	100	C6H12O	098386-09-5	43		
3	3-Hydroxy-3-methyl-2-butanone	102	C5H10O2	000115-22-0	43		
4	Propane, 1,1-dipropoxy-	160	C9H20O2	004744-11-0	39		
5	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	37		

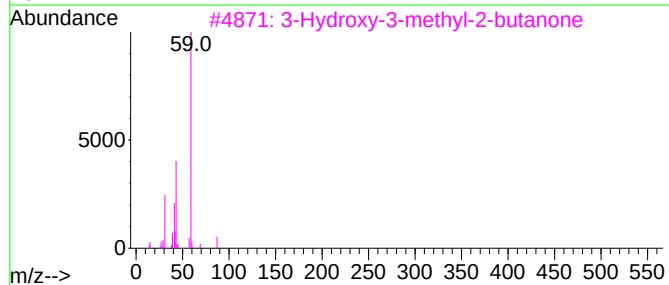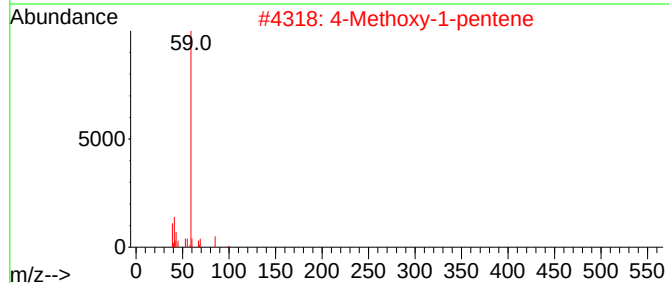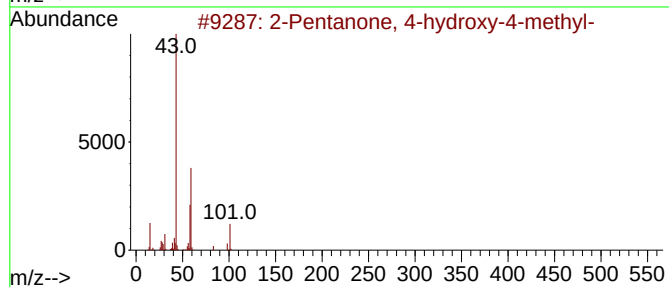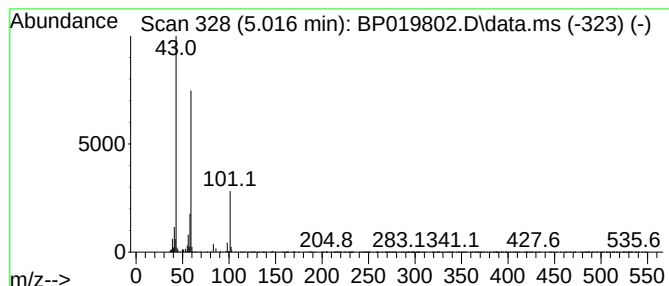

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022124\
Data File : BP019802.D
Acq On : 21 Feb 2024 11:43
Operator : MA/JU
Sample : PB159144BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159144BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.016	2.8	ng	60863	1	7.893	429511	20.0