


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022124\
Data File : BP019798.D
Acq On : 21 Feb 2024 09:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Feb 19 23:35:42 2024

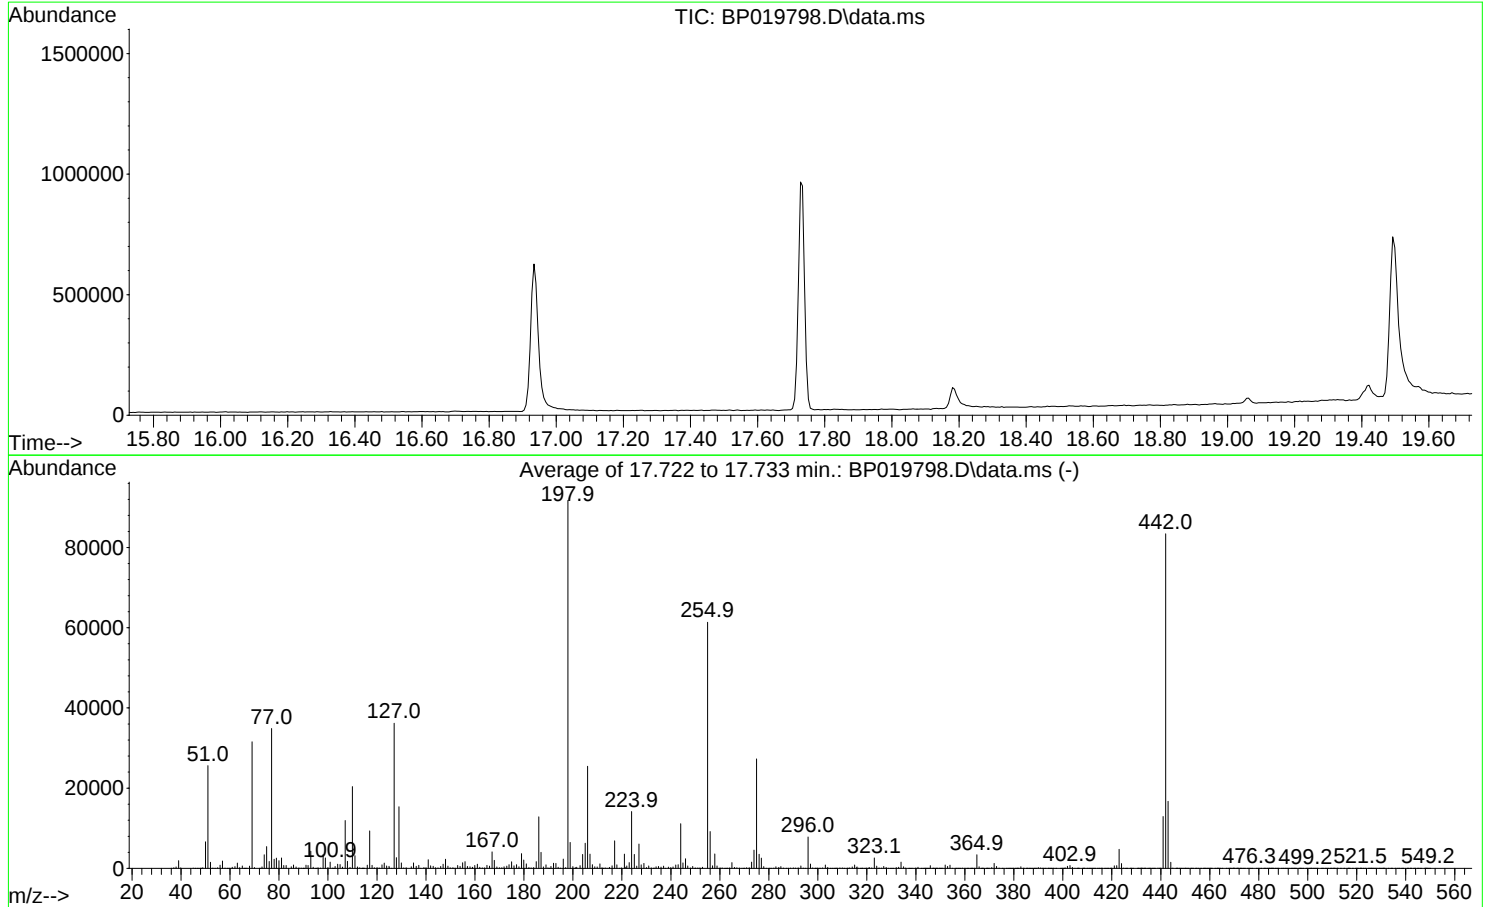




AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	27.9	25602	PASS
68	69	0.00	2	1.8	555	PASS
69	198	0.00	100	34.4	31578	PASS
70	69	0.00	2	0.7	213	PASS
127	198	10	80	39.5	36186	PASS
197	198	0.00	2	0.2	200	PASS
198	198	100	100	100.0	91724	PASS
199	198	5	9	7.1	6482	PASS
275	198	10	60	29.8	27298	PASS
365	198	1	100	3.7	3414	PASS
441	198	0.01	100	14.1	12924	PASS
442	442	100	100	100.0	83443	PASS
443	442	15	24	20.0	16722	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022124\
Data File : BP019798.D
Acq On : 21 Feb 2024 09:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 22 01:09:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 19 23:35:42 2024
Response via : Initial Calibration

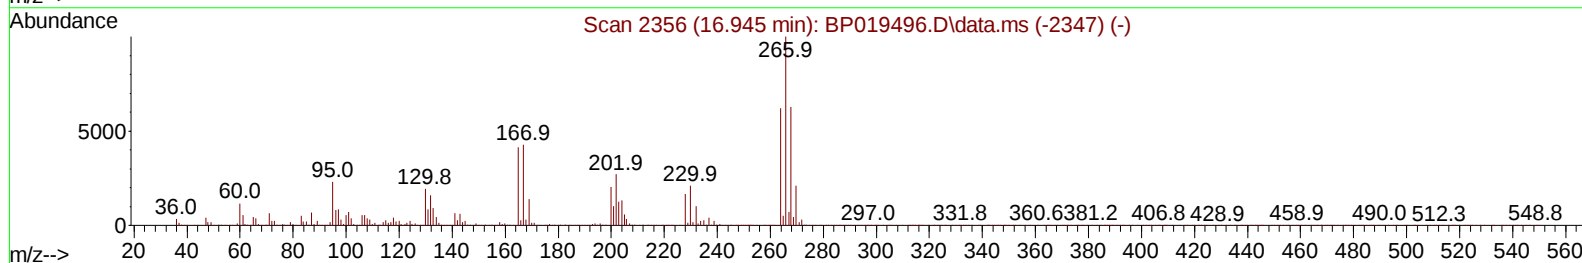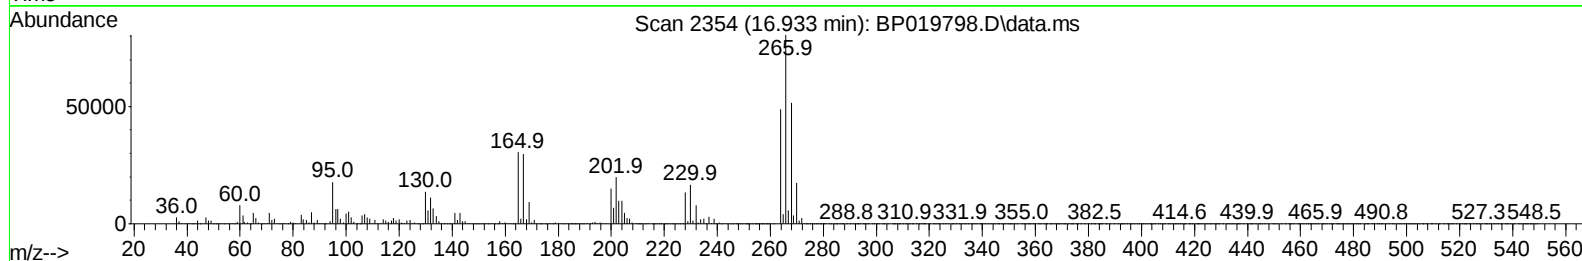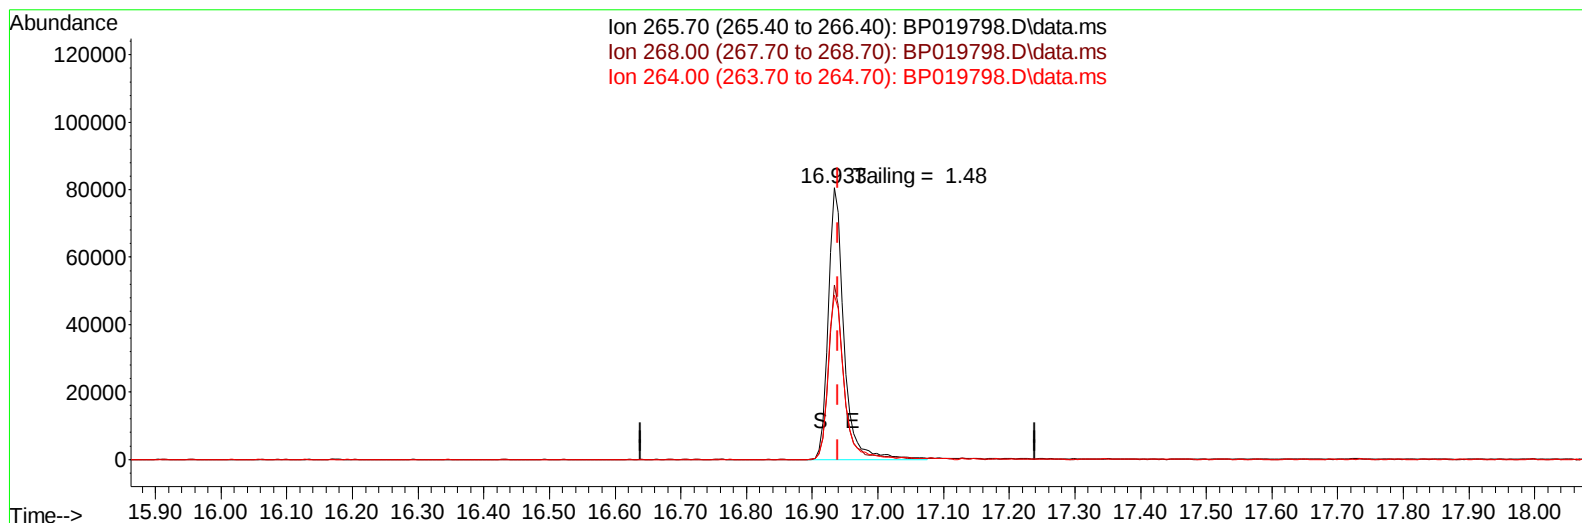

TIC: BP019798.D\data.ms

(70) Pentachlorophenol (C)

16.933min (-0.006) 591328.51 ng




response 134397

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	64.17
264.00	62.10	60.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022124\
Data File : BP019798.D
Acq On : 21 Feb 2024 09:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 22 01:09:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 19 23:35:42 2024
Response via : Initial Calibration

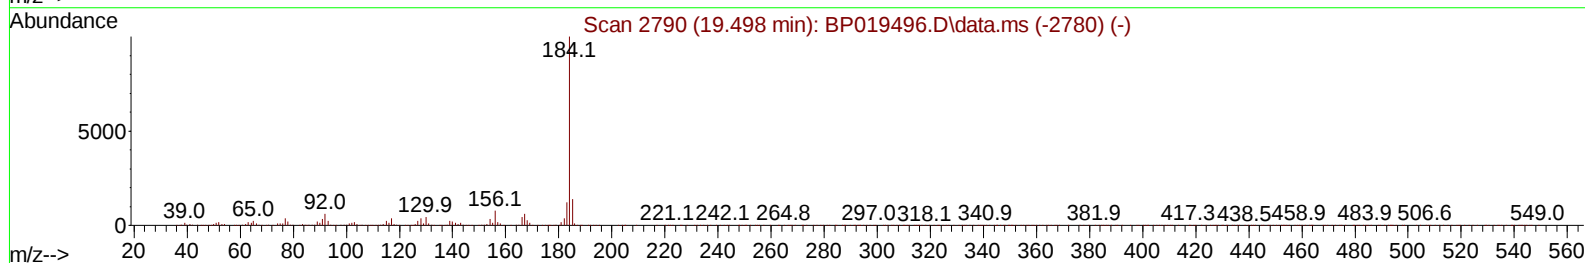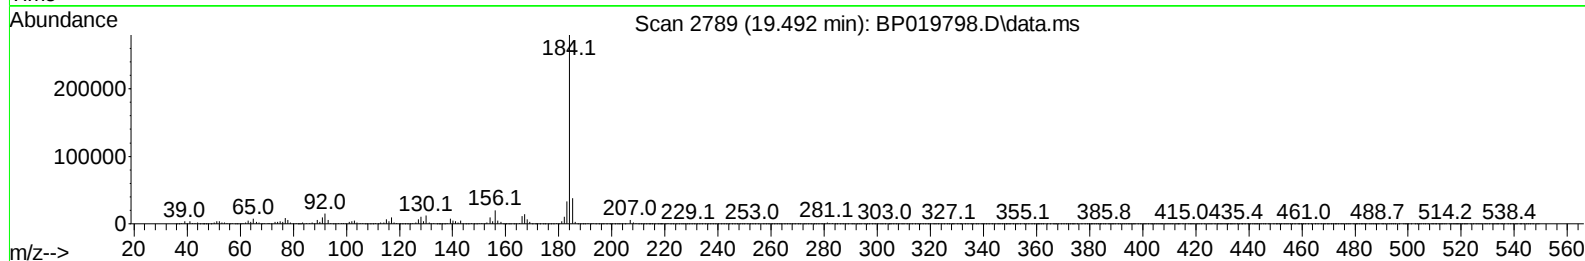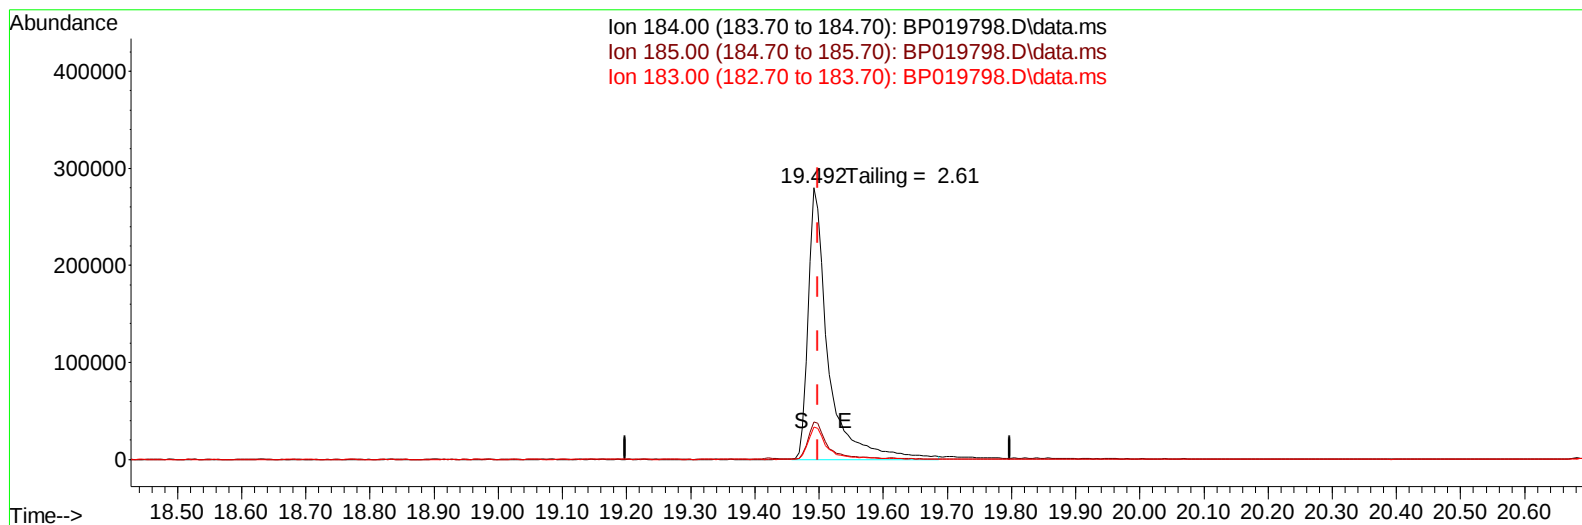

TIC: BP019798.D\data.ms

(77) Benzidine

19.492min (-0.006) 301154.31 ng

response 604429

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.72
183.00	12.10	11.90
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/21/2024	BNA_P	<u>BP019798.D</u>
Compound Name	Response	Retention Time
DDT	343608	20.686
DDD	11063	20.263
DDE	1240	19.757
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12303	355911	3.46

Instrument :
BNA_P
ClientSampleId :
DFTPP