

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022223\
 Data File : BP013869.D
 Acq On : 22 Feb 2023 10:07
 Operator : CG/JU
 Sample : PB150979BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK979

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013869.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.452	41	45	55	rVB	41832	59545	1.24%	0.126%
2	3.887	115	119	141	rBV	490599	822045	17.10%	1.743%
3	4.222	172	176	183	rVB2	11323	18481	0.38%	0.039%
4	4.699	252	257	259	rBV6	3171	5490	0.11%	0.012%
5	7.252	684	691	706	rVB	651563	1030978	21.44%	2.186%
6	7.422	713	720	734	rBV	517556	823435	17.12%	1.746%
7	7.628	747	755	765	rBV	647063	1069254	22.24%	2.267%
8	8.104	829	836	849	rBV	525621	845084	17.57%	1.792%
9	8.810	947	956	966	rBV	853169	1388812	28.88%	2.945%
10	9.281	1028	1036	1048	rBV	642610	1087631	22.62%	2.306%
11	10.004	1152	1159	1173	rBV	568739	956731	19.90%	2.029%
12	10.546	1243	1251	1262	rBV	836380	1473913	30.65%	3.125%
13	10.934	1309	1317	1325	rBV	738653	1247115	25.93%	2.644%
14	11.063	1332	1339	1355	rBV	822206	1475103	30.68%	3.128%
15	12.510	1580	1585	1592	rBV3	13168	24571	0.51%	0.052%
16	13.628	1769	1775	1780	rVB9	4249	7148	0.15%	0.015%
17	14.145	1856	1863	1875	rBV	1824201	2525025	52.51%	5.354%
18	14.263	1880	1883	1890	rVB9	3992	6991	0.15%	0.015%
19	14.439	1905	1913	1926	rBV	1901437	2881644	59.93%	6.110%
20	14.739	1957	1964	1973	rBV	1221316	1869187	38.87%	3.963%
21	14.928	1988	1996	2013	rBV	688432	1125508	23.41%	2.387%
22	15.145	2030	2033	2038	rVB7	4925	7872	0.16%	0.017%
23	15.733	2122	2133	2145	rBV	2618368	3687893	76.69%	7.820%
24	15.845	2145	2152	2169	rVV	866232	1183350	24.61%	2.509%
25	15.975	2170	2174	2178	rVB2	12929	19604	0.41%	0.042%
26	17.175	2372	2378	2382	rBV8	4012	8206	0.17%	0.017%
27	17.498	2426	2433	2443	rBV	1717846	2385799	49.61%	5.059%
28	17.598	2443	2450	2463	rVV	2806368	4103223	85.33%	8.701%
29	19.392	2751	2755	2760	rBV3	40380	53918	1.12%	0.114%
30	19.463	2762	2767	2773	rVV	38348	57686	1.20%	0.122%
31	19.816	2821	2827	2836	rBV	3681927	4808633	100.00%	10.196%
32	21.568	3120	3125	3134	rBV	1893896	2679840	55.73%	5.682%
33	23.957	3524	3531	3544	rVB2	2282710	4758669	98.96%	10.090%
34	24.121	3552	3559	3571	rVB2	1279419	2662373	55.37%	5.645%

Sum of corrected areas: 47160757




Instrument :
BNA_P
ClientSampleId :
SBLK979

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022223\
Data File : BP013869.D
Acq On : 22 Feb 2023 10:07
Operator : CG/JU
Sample : PB150979BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK979

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

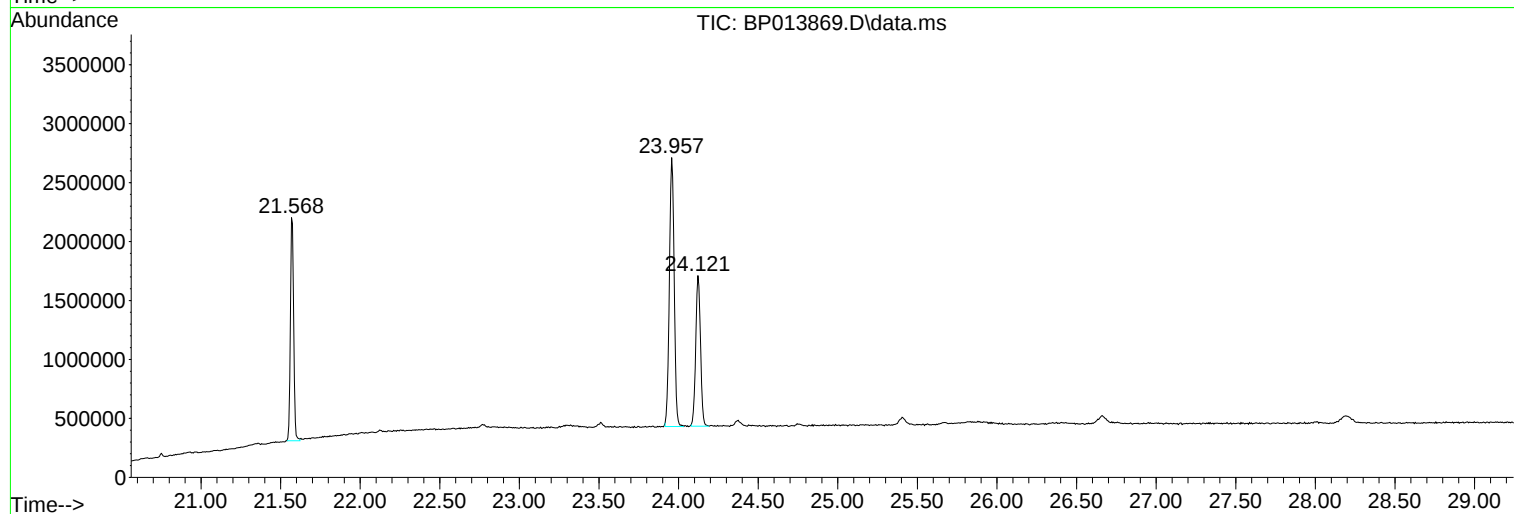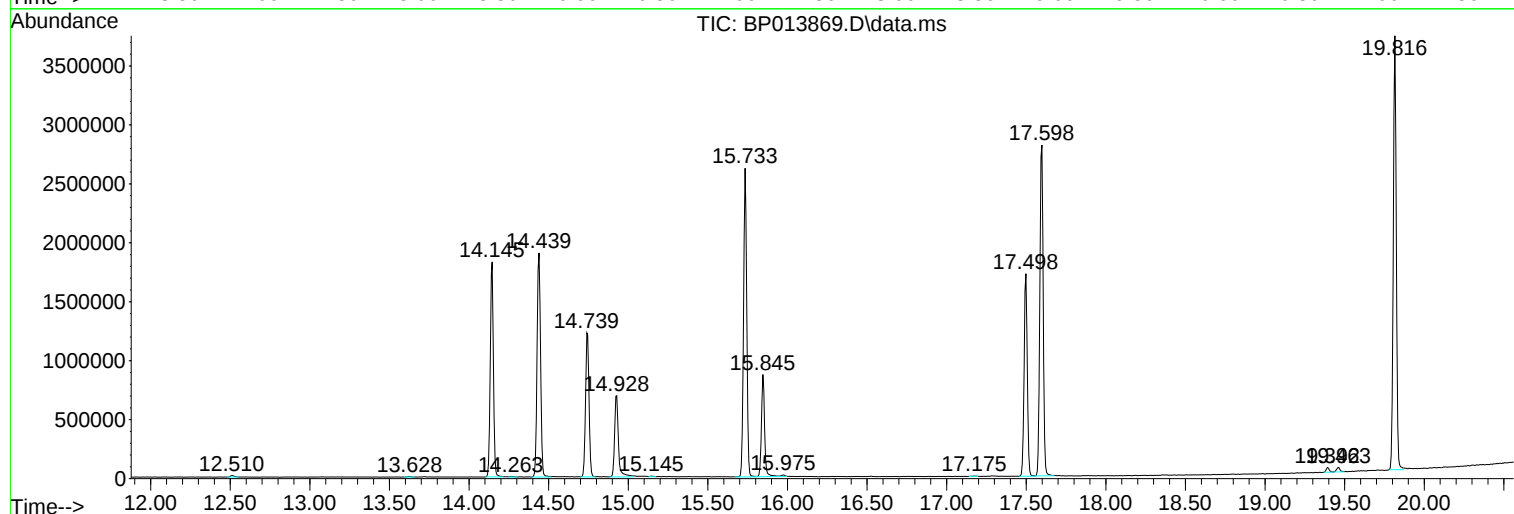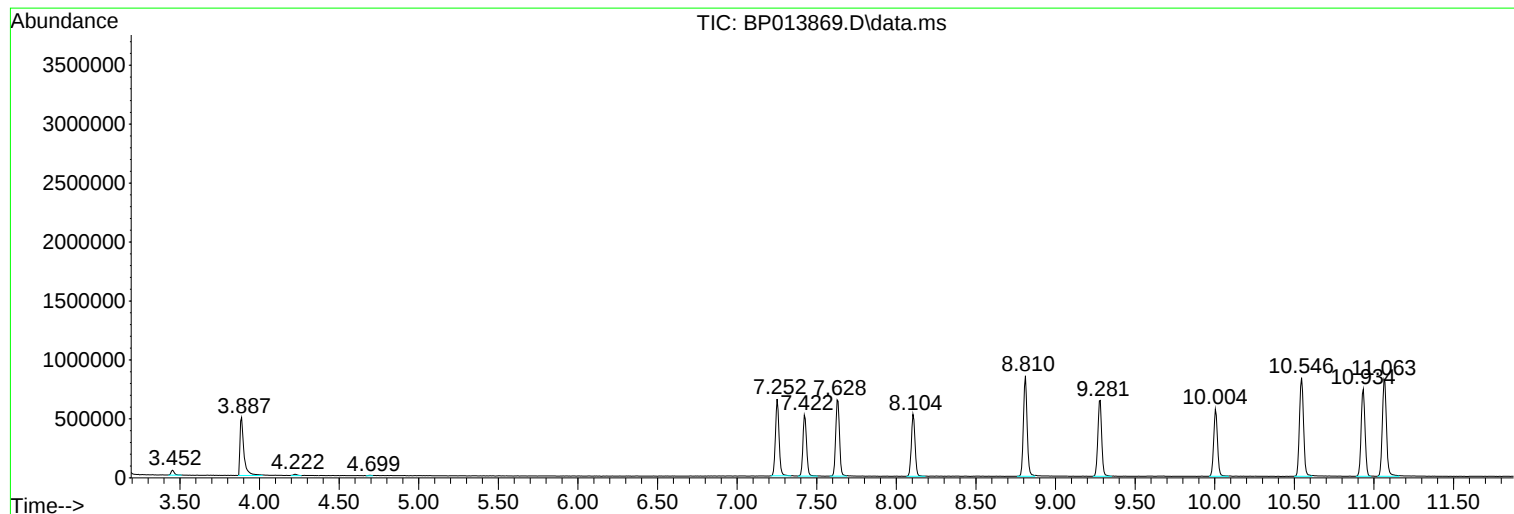

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022223\
Data File : BP013869.D
Acq On : 22 Feb 2023 10:07
Operator : CG/JU
Sample : PB150979BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK979

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022223\
Data File : BP013869.D
Acq On : 22 Feb 2023 10:07
Operator : CG/JU
Sample : PB150979BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK979

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc