

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022223\
 Data File : BP013874.D
 Acq On : 22 Feb 2023 14:59
 Operator : CG/JU
 Sample : PB150982BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK982

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013874.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.458	41	46	53	rVB	50202	69352	1.70%	0.159%
2	3.887	116	119	137	rBV	602294	889812	21.84%	2.035%
3	4.228	172	177	181	rBV	15944	22049	0.54%	0.050%
4	5.740	431	434	444	rVB	2116	4682	0.11%	0.011%
5	7.257	685	692	707	rBV	689241	1100635	27.02%	2.517%
6	7.428	714	721	734	rBV	558995	871136	21.39%	1.992%
7	7.634	749	756	772	rVB	720048	1142967	28.06%	2.614%
8	8.110	828	837	855	rBV	728133	1153290	28.31%	2.638%
9	8.816	949	957	972	rBV	853365	1381312	33.91%	3.159%
10	9.281	1029	1036	1051	rBV	633882	1078849	26.48%	2.467%
11	10.010	1152	1160	1174	rBV	564228	935526	22.97%	2.140%
12	10.551	1244	1252	1265	rBV	876246	1442947	35.42%	3.300%
13	10.940	1310	1318	1329	rVB	921780	1545031	37.93%	3.534%
14	11.069	1333	1340	1360	rBV	785217	1392270	34.18%	3.184%
15	12.516	1581	1586	1592	rBV3	13681	24853	0.61%	0.057%
16	13.634	1770	1776	1782	rBV8	5403	10602	0.26%	0.024%
17	14.151	1854	1864	1878	rBV	1605805	2240301	55.00%	5.124%
18	14.257	1881	1882	1887	rVB5	2794	4197	0.10%	0.010%
19	14.445	1906	1914	1929	rBV	1751898	2567332	63.03%	5.872%
20	14.751	1957	1966	1978	rBV	1468798	2163845	53.12%	4.949%
21	14.934	1990	1997	2015	rBV	594530	974441	23.92%	2.229%
22	15.151	2031	2034	2040	rVB8	4754	7373	0.18%	0.017%
23	15.504	2090	2094	2099	rVB7	2683	4530	0.11%	0.010%
24	15.698	2123	2127	2128	rBV4	4386	4676	0.11%	0.011%
25	15.739	2128	2134	2143	rVV	2322952	3274182	80.38%	7.489%
26	15.851	2147	2153	2165	rBV	722881	1016596	24.96%	2.325%
27	15.981	2171	2175	2180	rVB3	10988	16427	0.40%	0.038%
28	16.098	2191	2195	2202	rBV9	4617	10901	0.27%	0.025%
29	16.763	2304	2308	2314	rBV9	3121	6157	0.15%	0.014%
30	16.951	2336	2340	2344	rVB6	3956	6493	0.16%	0.015%
31	17.181	2376	2379	2384	rVB7	3540	4084	0.10%	0.009%
32	17.310	2394	2401	2405	rVB7	3905	10875	0.27%	0.025%
33	17.504	2426	2434	2443	rBV	1881484	2667446	65.48%	6.101%
34	17.604	2444	2451	2465	rVV	2408538	3521603	86.45%	8.054%
35	18.369	2577	2581	2584	rBV5	5193	9320	0.23%	0.021%
36	19.398	2752	2756	2761	rVB2	32400	42051	1.03%	0.096%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022223\
Data File : BP013874.D
Acq On : 22 Feb 2023 14:59
Operator : CG/JU
Sample : PB150982BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK982

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Title : SVOA CALIBRATION

37	19.469	2764	2768	2773	rVV	29443	41403	1.02%	0.095%
38	19.822	2822	2828	2844	rBV	3067111	4073509	100.00%	9.317%
39	21.580	3122	3127	3137	rVB	1806469	2504092	61.47%	5.727%
40	23.962	3525	3532	3541	rBV2	1491224	3189969	78.31%	7.296%
41	24.133	3554	3561	3573	rVB2	1071697	2295346	56.35%	5.250%




Sum of corrected areas: 43722462

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022223\
Data File : BP013874.D
Acq On : 22 Feb 2023 14:59
Operator : CG/JU
Sample : PB150982BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK982

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

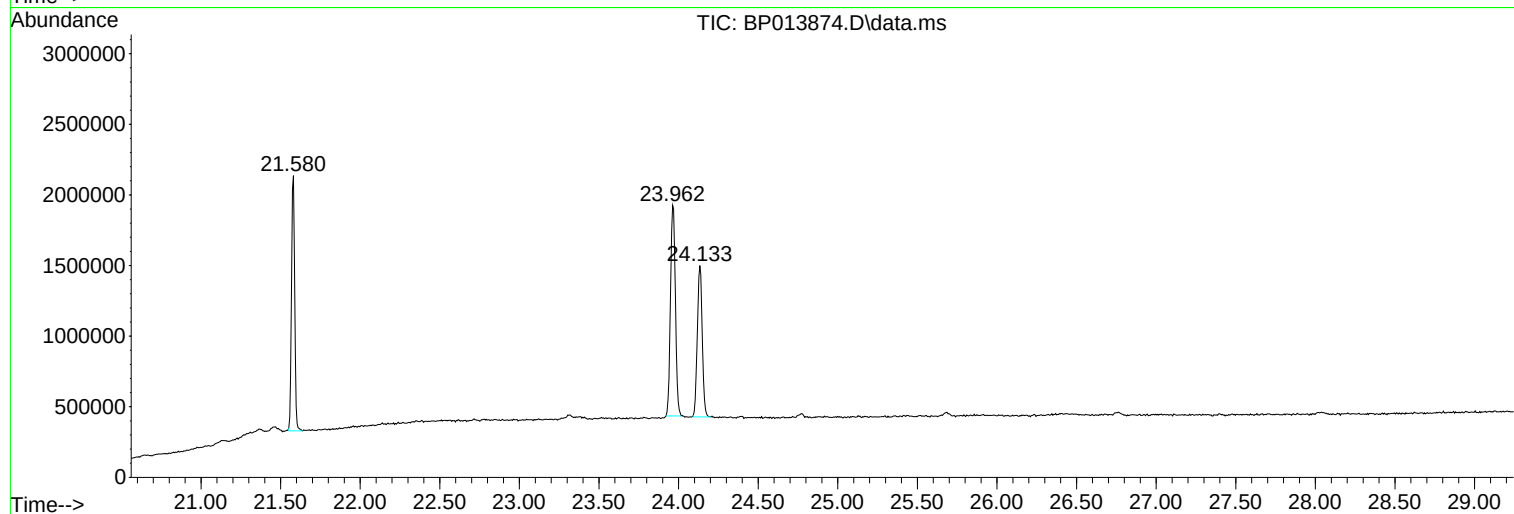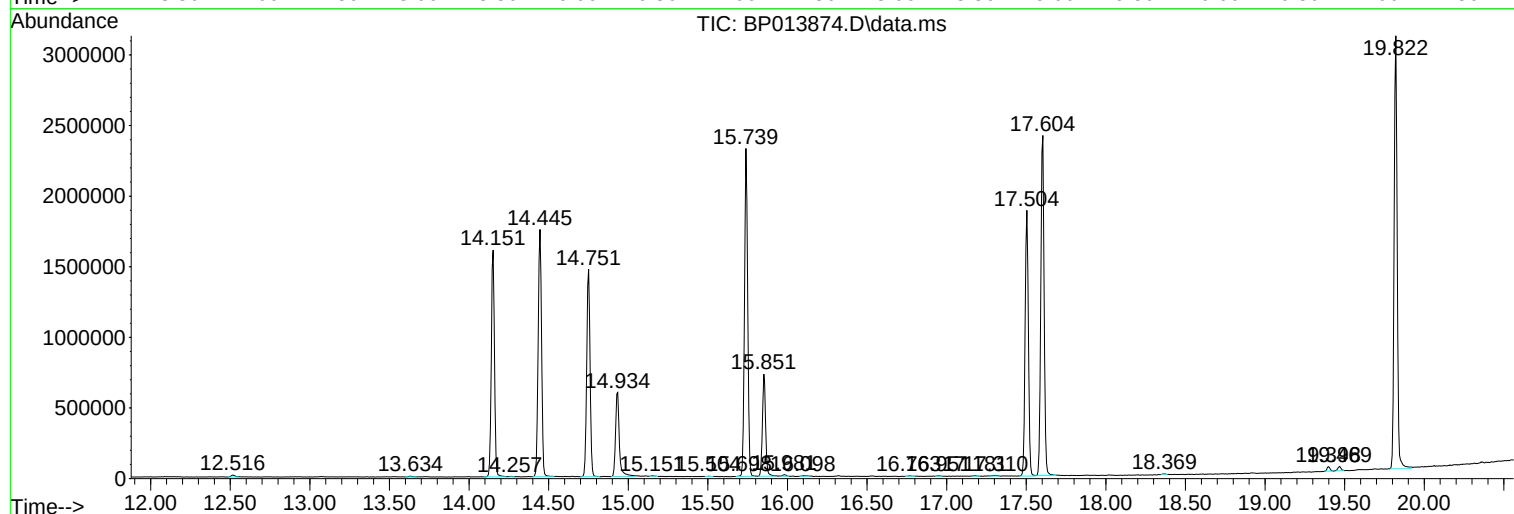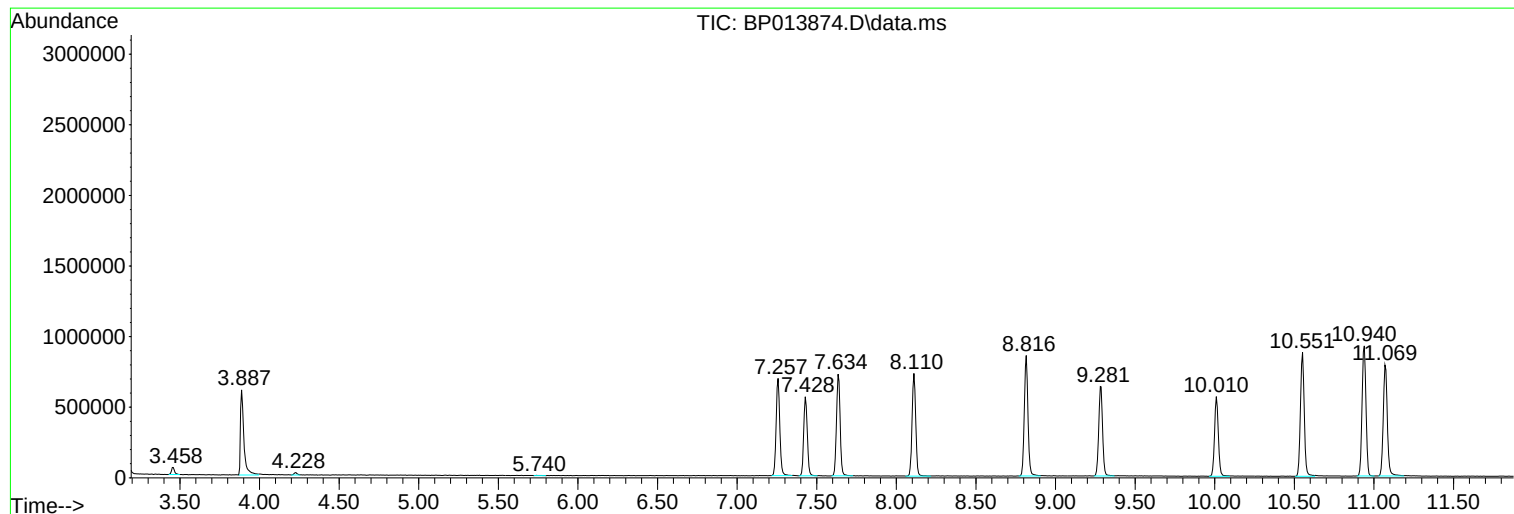

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022223\
Data File : BP013874.D
Acq On : 22 Feb 2023 14:59
Operator : CG/JU
Sample : PB150982BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK982

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022223\
Data File : BP013874.D
Acq On : 22 Feb 2023 14:59
Operator : CG/JU
Sample : PB150982BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK982

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc