
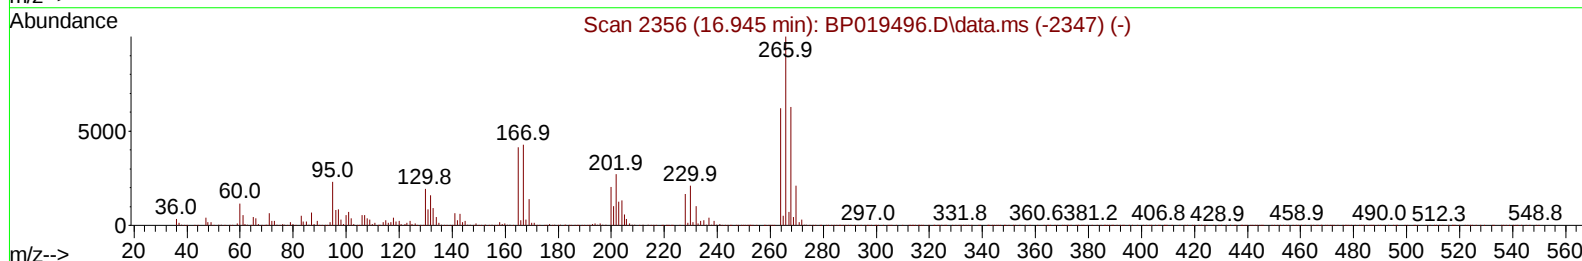
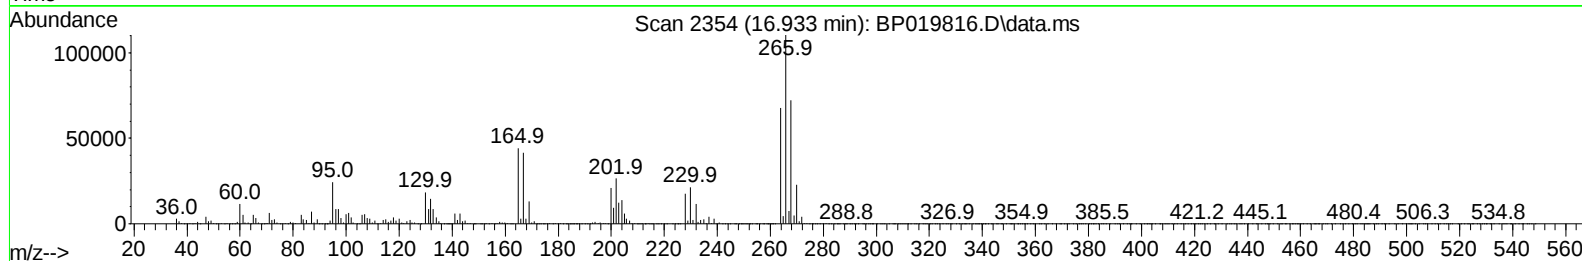


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022224\
Data File : BP019816.D
Acq On : 22 Feb 2024 10:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 11:18:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 19 23:35:42 2024
Response via : Initial Calibration

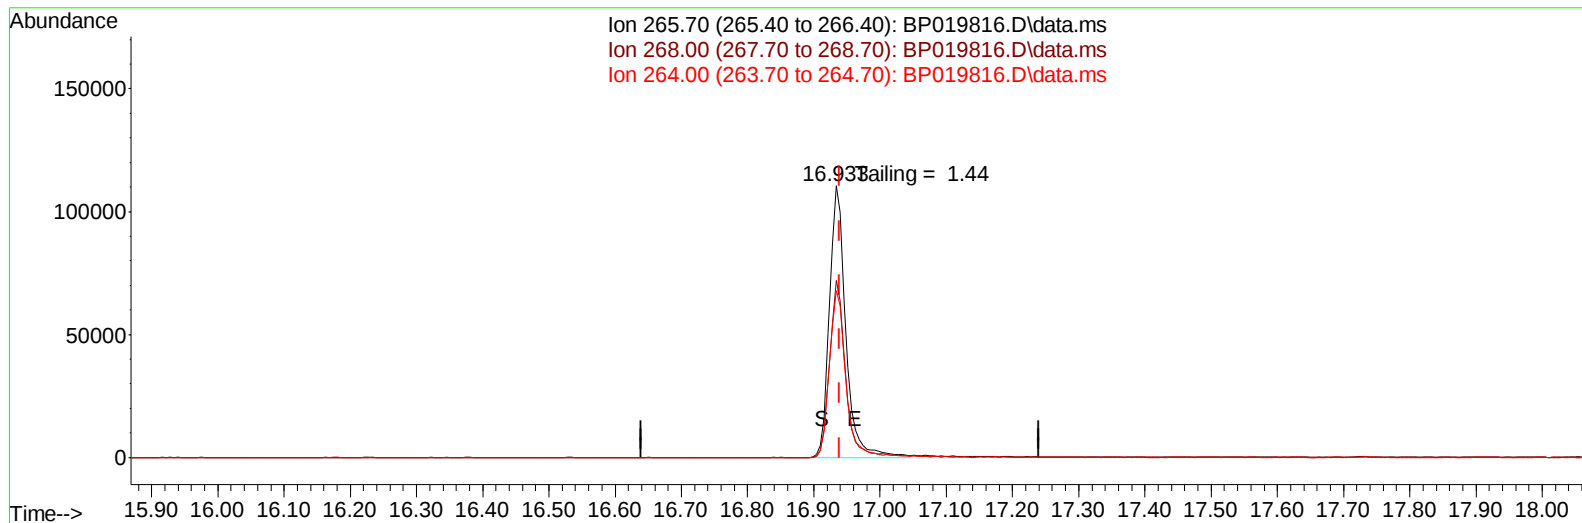

TIC: BP019816.D\data.ms

(70) Pentachlorophenol (C)




16.933min (-0.006) 597290.96 ng

response 190053

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	65.28
264.00	62.10	61.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022224\
Data File : BP019816.D
Acq On : 22 Feb 2024 10:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 11:18:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 19 23:35:42 2024
Response via : Initial Calibration

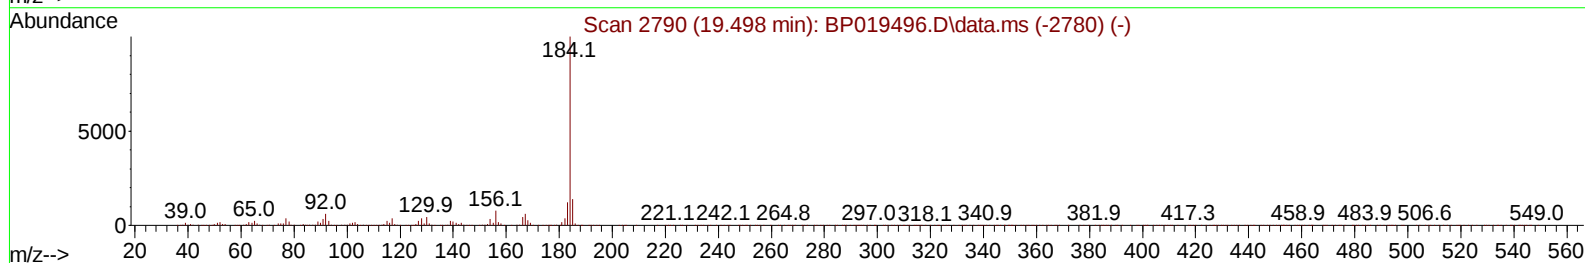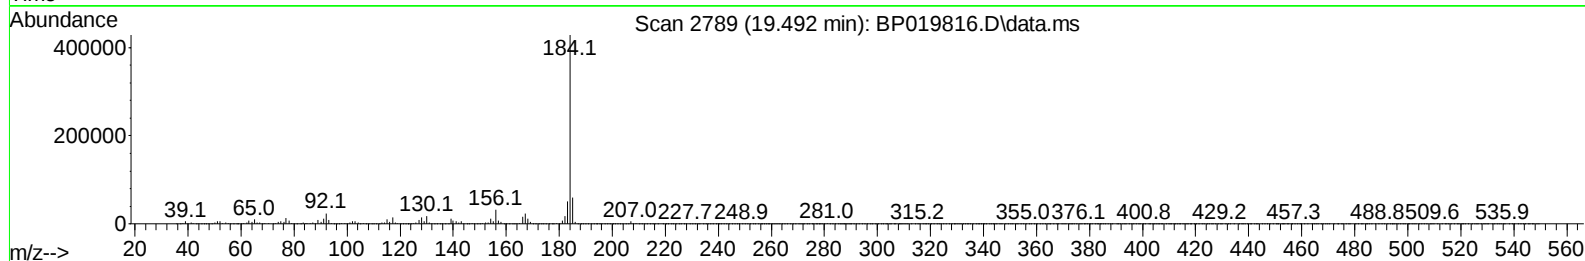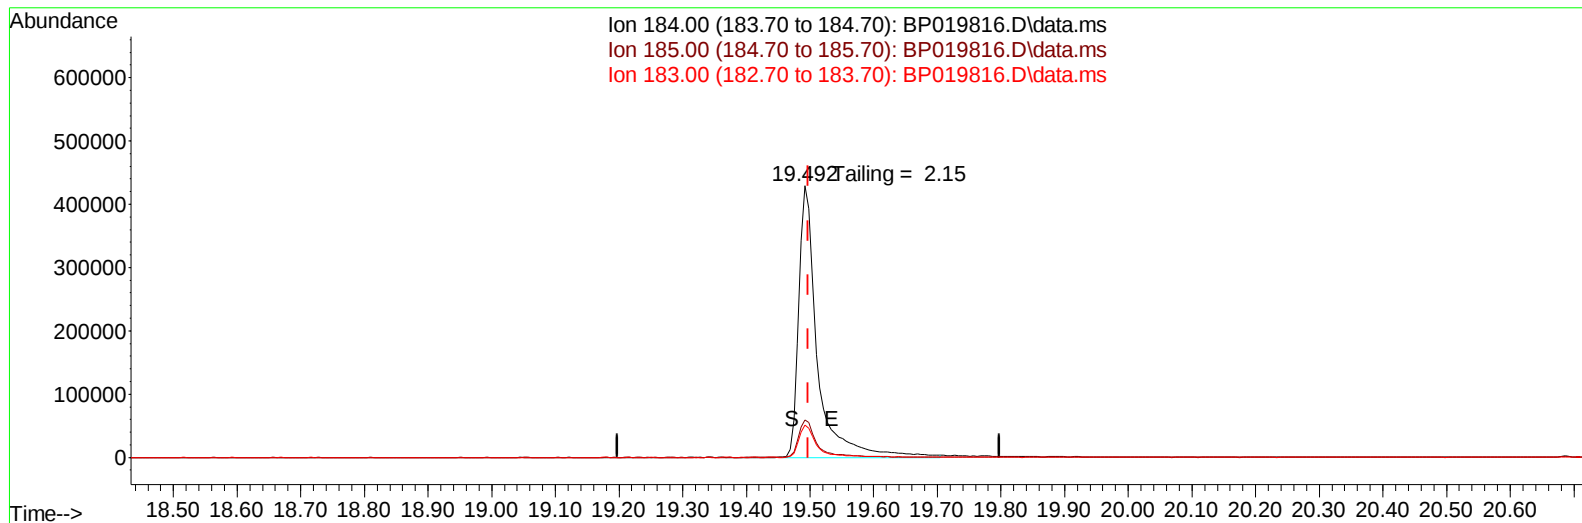

TIC: BP019816.D\data.ms

(77) Benzidine**19.492min (-0.006) 284587.10 ng****response 880566**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.90
183.00	12.10	11.86
0.00	0.00	0.00