
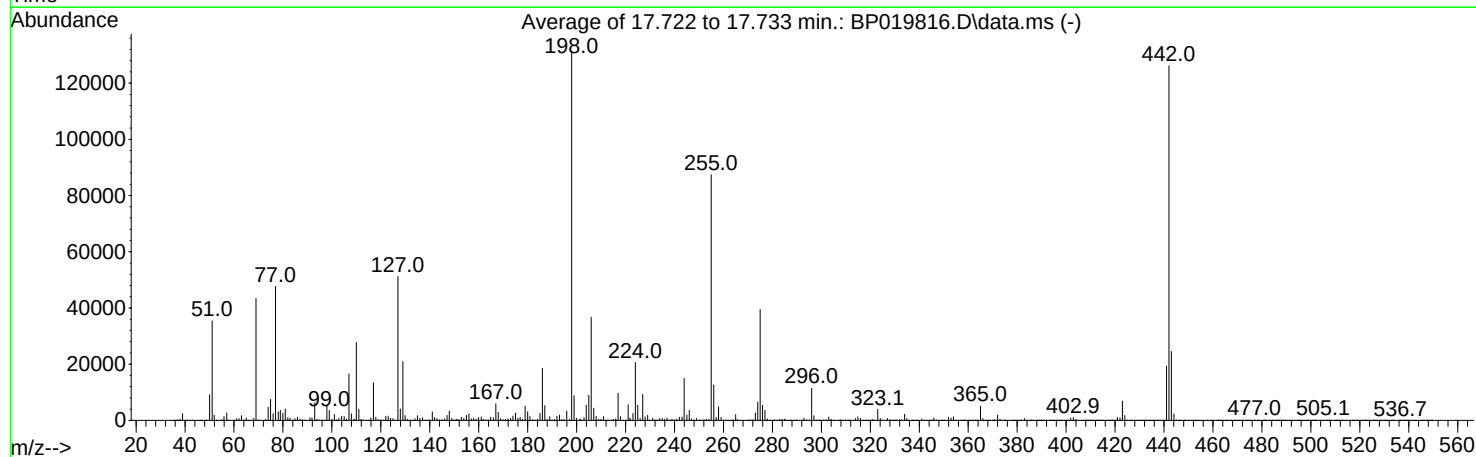


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022224\
Data File : BP019816.D
Acq On : 22 Feb 2024 10:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 23 13:10:49 2024

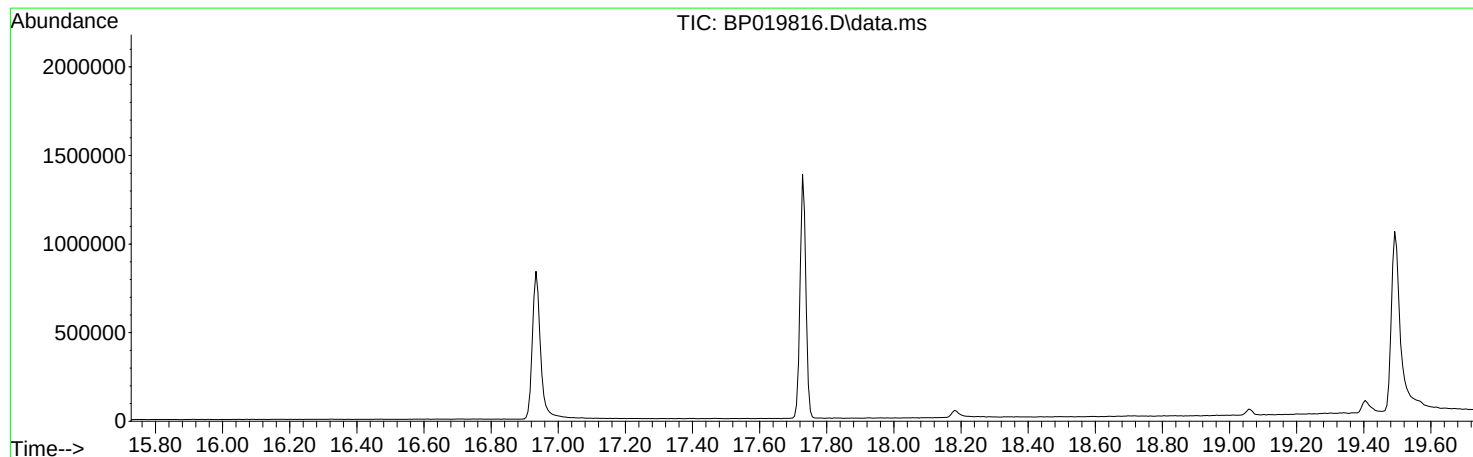




AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.1	35432	PASS
68	69	0.00	2	1.6	703	PASS
69	198	0.00	100	33.1	43379	PASS
70	69	0.00	2	0.4	174	PASS
127	198	10	80	39.1	51211	PASS
197	198	0.00	2	0.3	337	PASS
198	198	100	100	100.0	130909	PASS
199	198	5	9	6.7	8796	PASS
275	198	10	60	30.1	39447	PASS
365	198	1	100	3.8	5008	PASS
441	198	0.01	100	14.7	19303	PASS
442	442	100	100	100.0	126173	PASS
443	442	15	24	19.4	24473	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022224\
Data File : BP019816.D
Acq On : 22 Feb 2024 10:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 22 11:18:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 19 23:35:42 2024
Response via : Initial Calibration

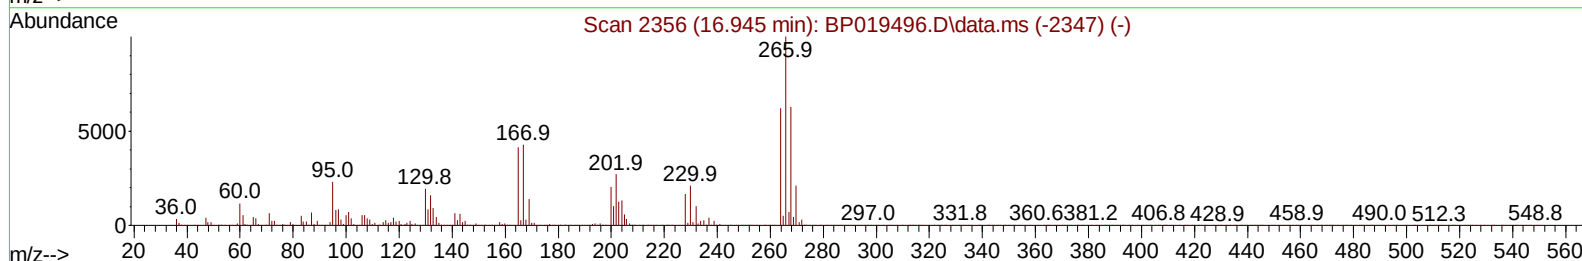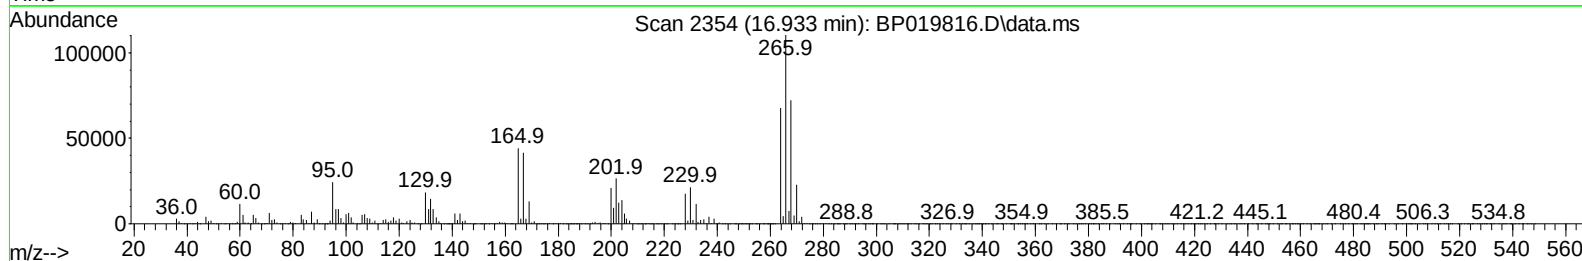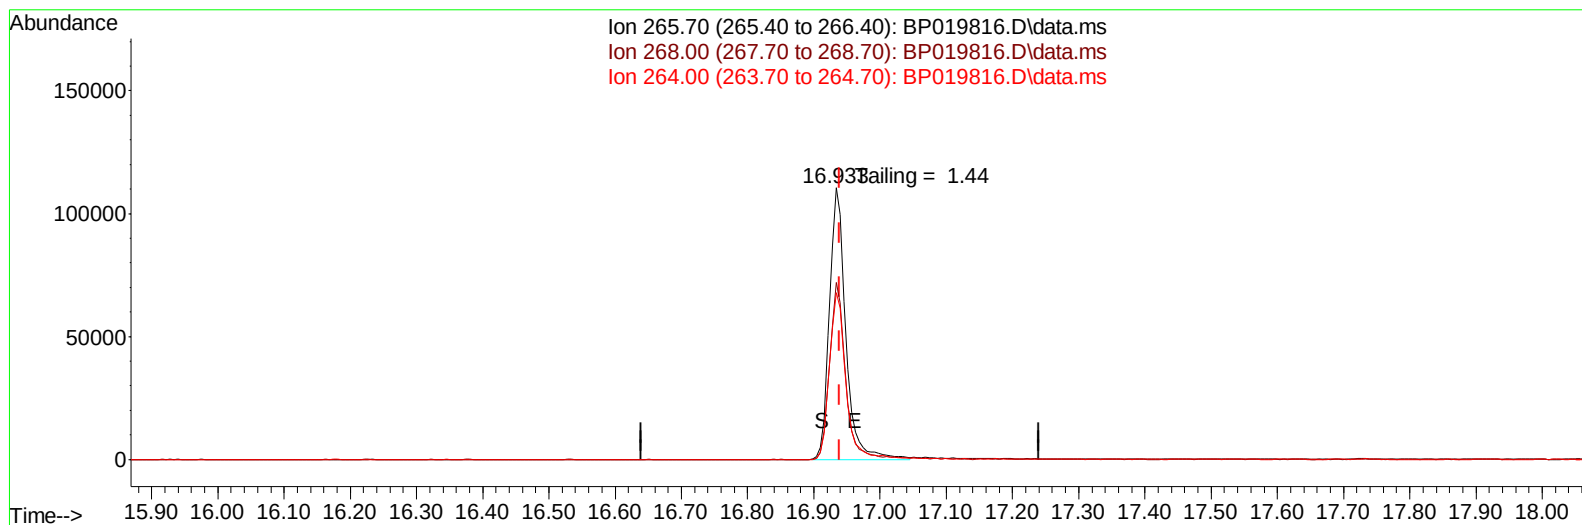

TIC: BP019816.D\data.ms

(70) Pentachlorophenol (C)

16.933min (-0.006) 597290.96 ng




response 190053

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	65.28
264.00	62.10	61.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022224\
Data File : BP019816.D
Acq On : 22 Feb 2024 10:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 22 11:18:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 19 23:35:42 2024
Response via : Initial Calibration

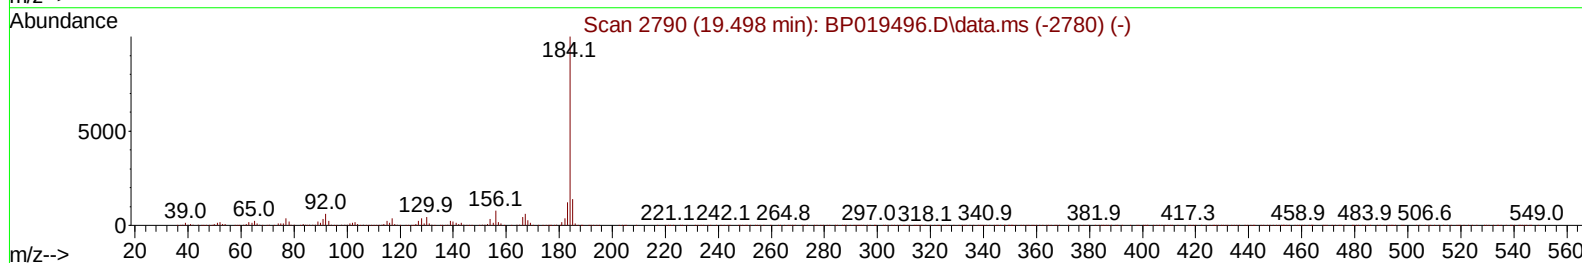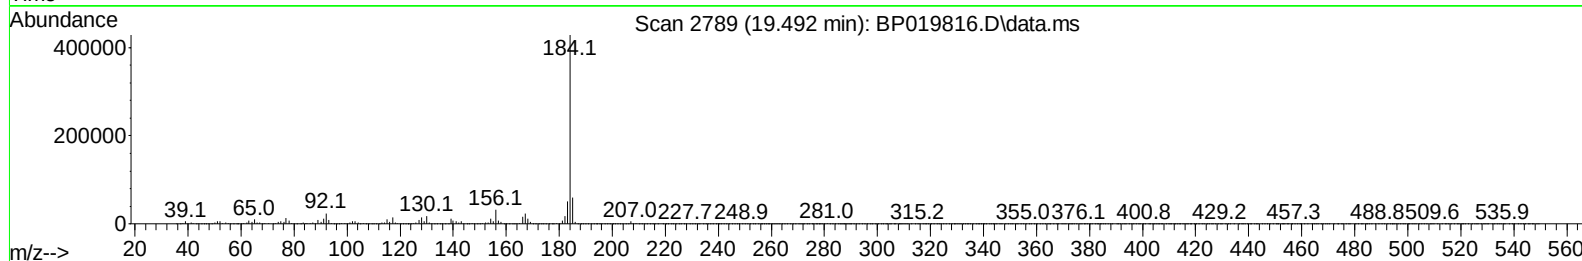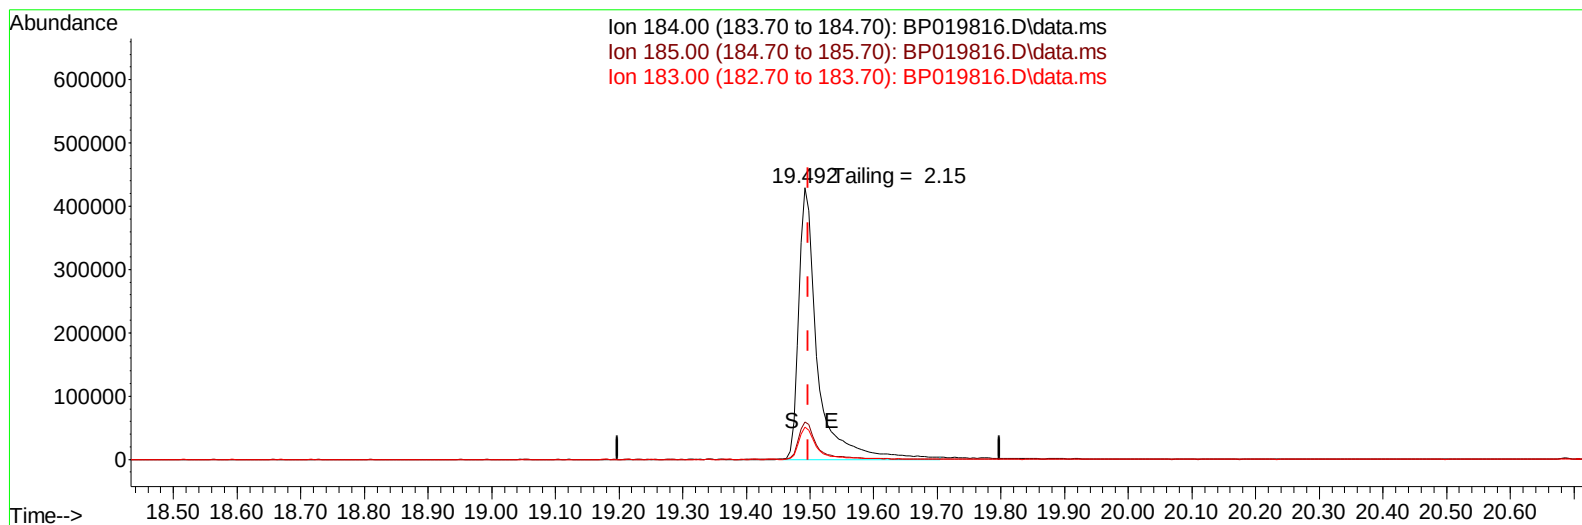

TIC: BP019816.D\data.ms

(77) Benzidine

19.492min (-0.006) 284587.10 ng

response 880566

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.90
183.00	12.10	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/22/2024	BNA_P	<u>BP019816.D</u>
Compound Name	Response	Retention Time
DDT	505494	20.686
DDD	18183	20.257
DDE	1460	19.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19643	525137	3.74

Instrument :
BNA_P
ClientSampleId :
DFTPP