

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022321\
 Data File : BP004856.D
 Acq On : 23 Feb 2021 15:05
 Operator : CG/JU
 Sample : PB134680BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK680

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP022221.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	8	12	20	rVB	13308	23660	1.68%	0.155%
2	3.670	79	82	106	rBV	148671	309737	22.02%	2.023%
3	3.975	131	134	142	rVB5	3058	5597	0.40%	0.037%
4	4.181	167	169	172	rVB3	1225	1444	0.10%	0.009%
5	4.228	175	177	182	rBV6	1060	1725	0.12%	0.011%
6	4.587	236	238	241	rVB4	1682	1581	0.11%	0.010%
7	4.628	241	245	248	rBV6	1185	2016	0.14%	0.013%
8	4.681	253	254	258	rVB4	1183	1458	0.10%	0.010%
9	6.934	630	637	649	rVB	275983	452504	32.17%	2.956%
10	7.093	656	664	673	rBV	205157	320856	22.81%	2.096%
11	7.293	688	698	708	rBV	315458	503689	35.81%	3.291%
12	7.363	708	710	715	rVB6	1313	1743	0.12%	0.011%
13	7.758	770	777	784	rBV	226472	363540	25.84%	2.375%
14	8.469	891	898	909	rVV	347039	553011	39.31%	3.613%
15	8.916	964	974	983	rBV	262787	429335	30.52%	2.805%
16	9.634	1089	1096	1107	rBV	246262	393524	27.97%	2.571%
17	10.175	1180	1188	1201	rBV	348996	587023	41.73%	3.835%
18	10.546	1243	1251	1260	rBV	276018	466200	33.14%	3.046%
19	10.687	1268	1275	1288	rBV	307329	540482	38.42%	3.531%
20	10.799	1292	1294	1299	rVB6	1079	1534	0.11%	0.010%
21	12.146	1517	1523	1528	rBV3	5020	8601	0.61%	0.056%
22	13.816	1800	1807	1820	rBV	561071	777964	55.30%	5.082%
23	14.098	1846	1855	1867	rBV	648995	925346	65.78%	6.045%
24	14.404	1901	1907	1917	rVB	392621	583778	41.50%	3.814%
25	14.622	1938	1944	1958	rBV	242030	366285	26.04%	2.393%
26	15.239	2045	2049	2052	rVB6	912	1513	0.11%	0.010%
27	15.404	2070	2077	2090	rVB	794584	1088488	77.38%	7.111%
28	15.522	2090	2097	2107	rBV	269396	379200	26.96%	2.477%
29	15.645	2111	2118	2124	rVB2	9618	14383	1.02%	0.094%
30	16.092	2190	2194	2198	rBV7	921	1824	0.13%	0.012%
31	16.186	2205	2210	2216	rBV6	2590	5020	0.36%	0.033%
32	16.951	2337	2340	2345	rBV3	2022	2266	0.16%	0.015%
33	17.163	2370	2376	2385	rVB	463509	658715	46.83%	4.303%
34	17.263	2386	2393	2403	rBV	829235	1181322	83.98%	7.718%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022321\
 Data File : BP004856.D
 Acq On : 23 Feb 2021 15:05
 Operator : CG/JU
 Sample : PB134680BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK680

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP022221.M
 Title : SVOA CALIBRATION

35	18.063	2526	2529	2532	rBV5	1847	2455	0.17%	0.016%
36	18.133	2536	2541	2544	rVV6	1149	2417	0.17%	0.016%
37	18.404	2585	2587	2591	rBV4	1239	2063	0.15%	0.013%
38	18.516	2605	2606	2608	rBV2	1487	1447	0.10%	0.009%
39	18.628	2624	2625	2628	rBV3	2123	1490	0.11%	0.010%
40	19.151	2709	2714	2719	rBV	9754	14565	1.04%	0.095%
41	19.392	2752	2755	2761	rVB2	8555	10080	0.72%	0.066%
42	19.504	2768	2774	2782	rBV	1079203	1383955	98.38%	9.041%
43	21.033	3032	3034	3041	rVB2	14865	19221	1.37%	0.126%
44	21.251	3066	3071	3077	rBV	606650	753119	53.54%	4.920%
45	21.369	3088	3091	3093	rBV2	19838	19721	1.40%	0.129%
46	23.410	3431	3438	3450	rVB	724339	1406746	100.00%	9.190%
47	23.557	3457	3463	3473	rVB	378792	734371	52.20%	4.798%


Sum of corrected areas: 15307014

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022321\
Data File : BP004856.D
Acq On : 23 Feb 2021 15:05
Operator : CG/JU
Sample : PB134680BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK680

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP022221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

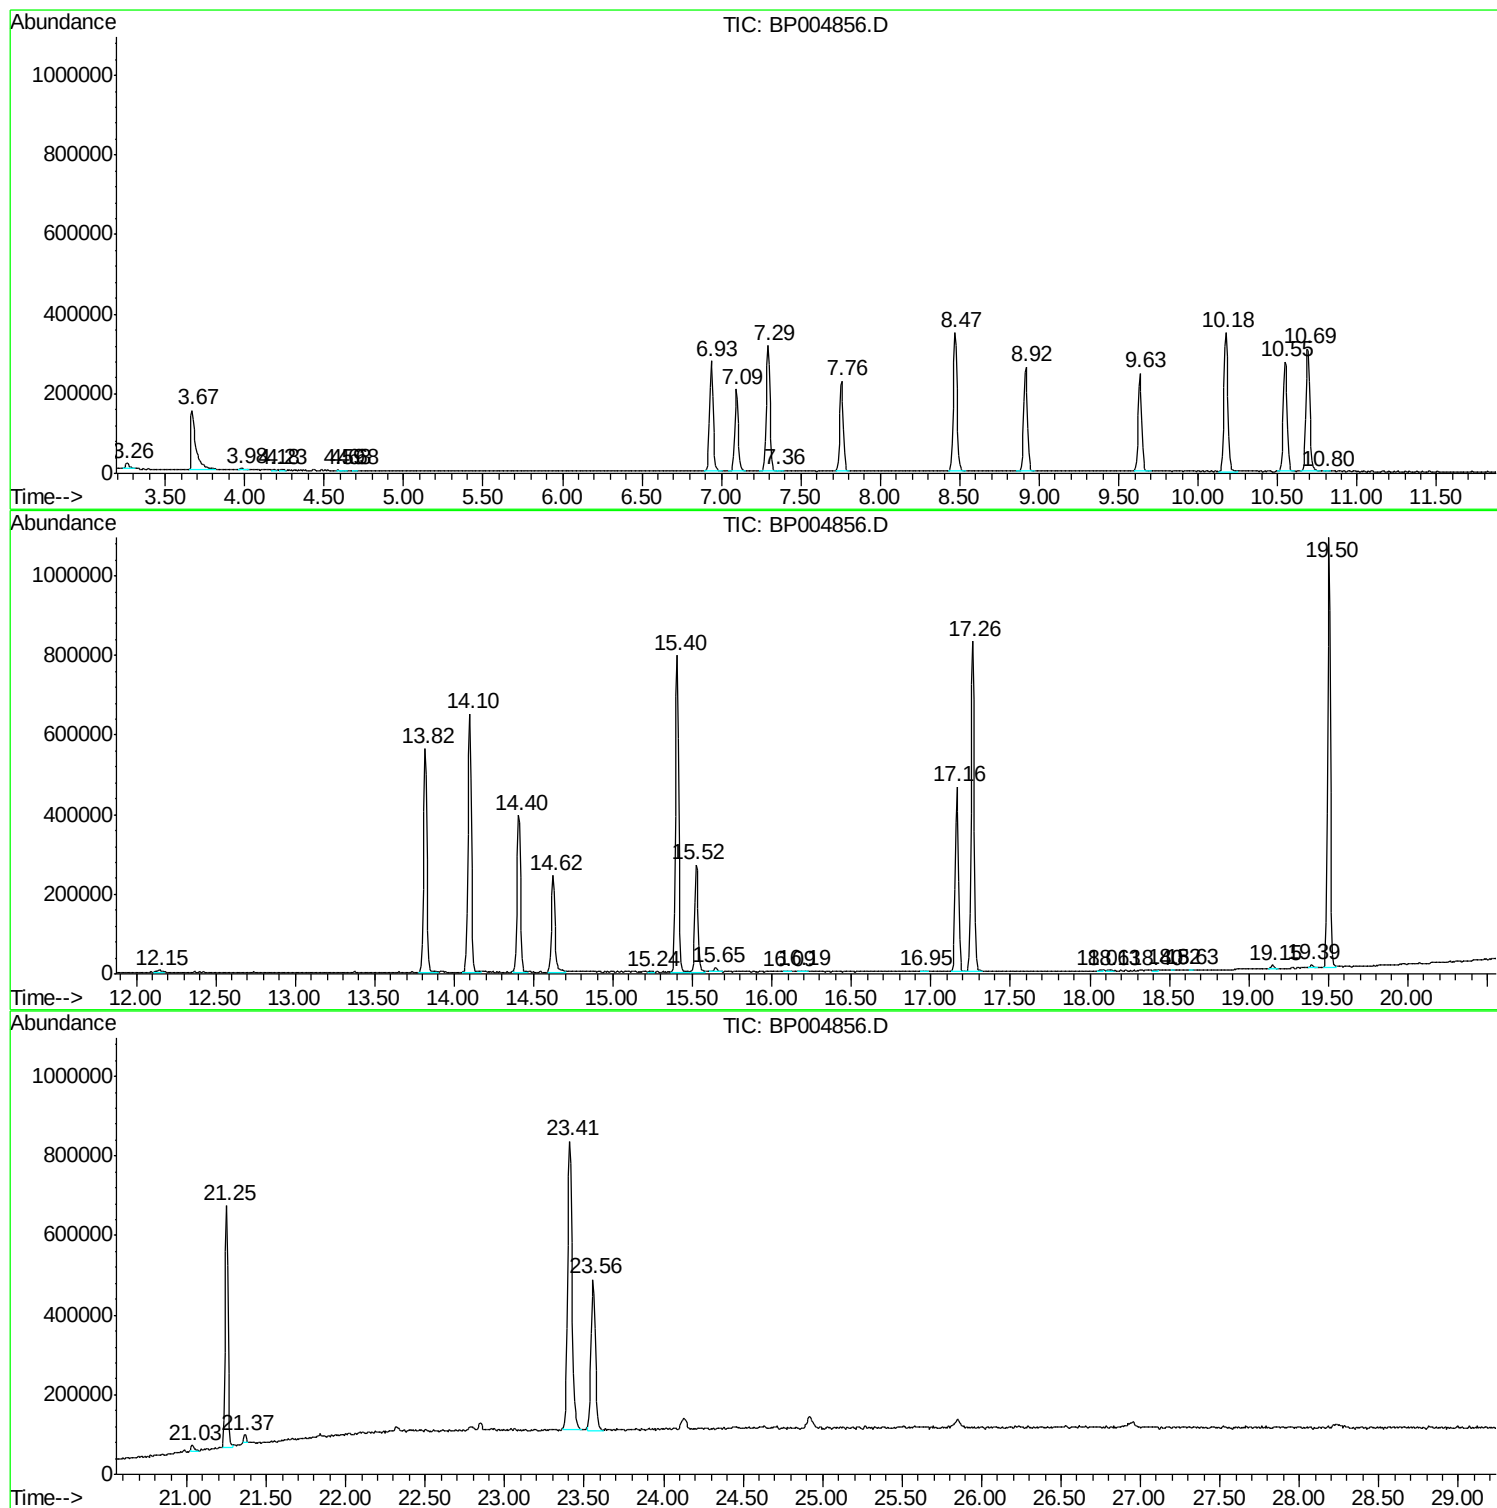

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022321\
Data File : BP004856.D
Acq On : 23 Feb 2021 15:05
Operator : CG/JU
Sample : PB134680BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK680

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP022221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022321\
Data File : BP004856.D
Acq On : 23 Feb 2021 15:05
Operator : CG/JU
Sample : PB134680BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK680

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP022221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc