
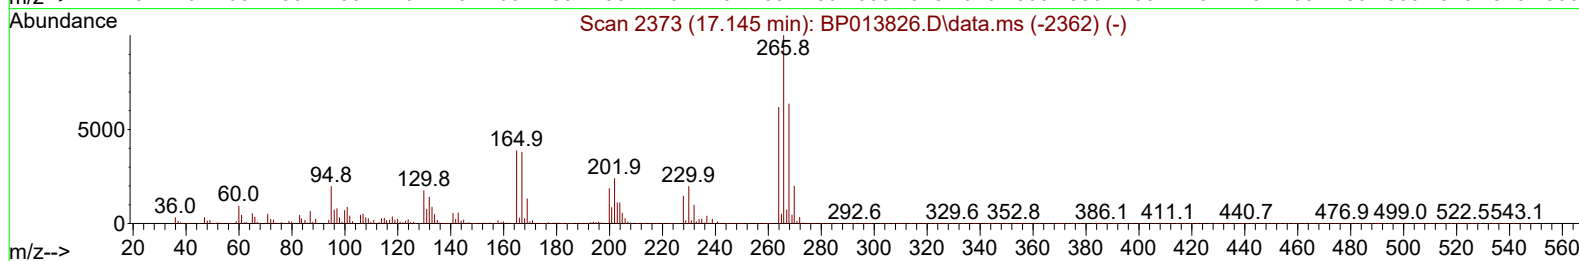
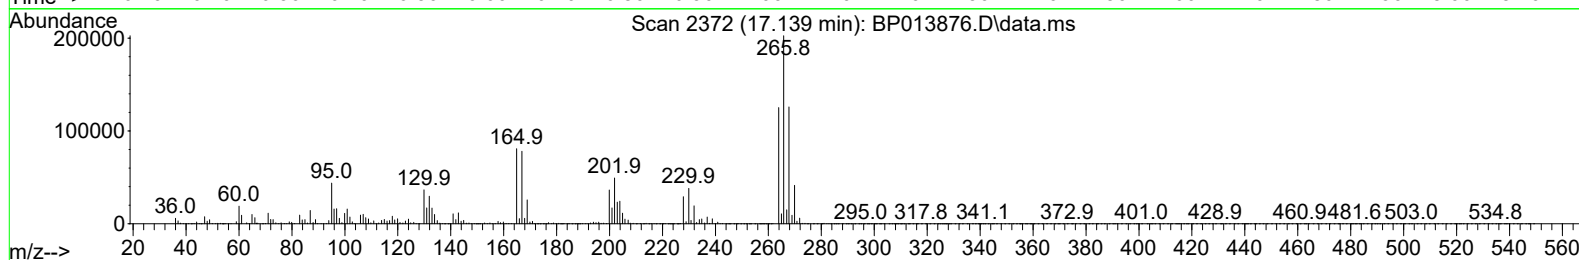


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022323\
 Data File : BP013876.D
 Acq On : 23 Feb 2023 12:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 24 03:34:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 24 01:37:56 2023
 Response via : Initial Calibration

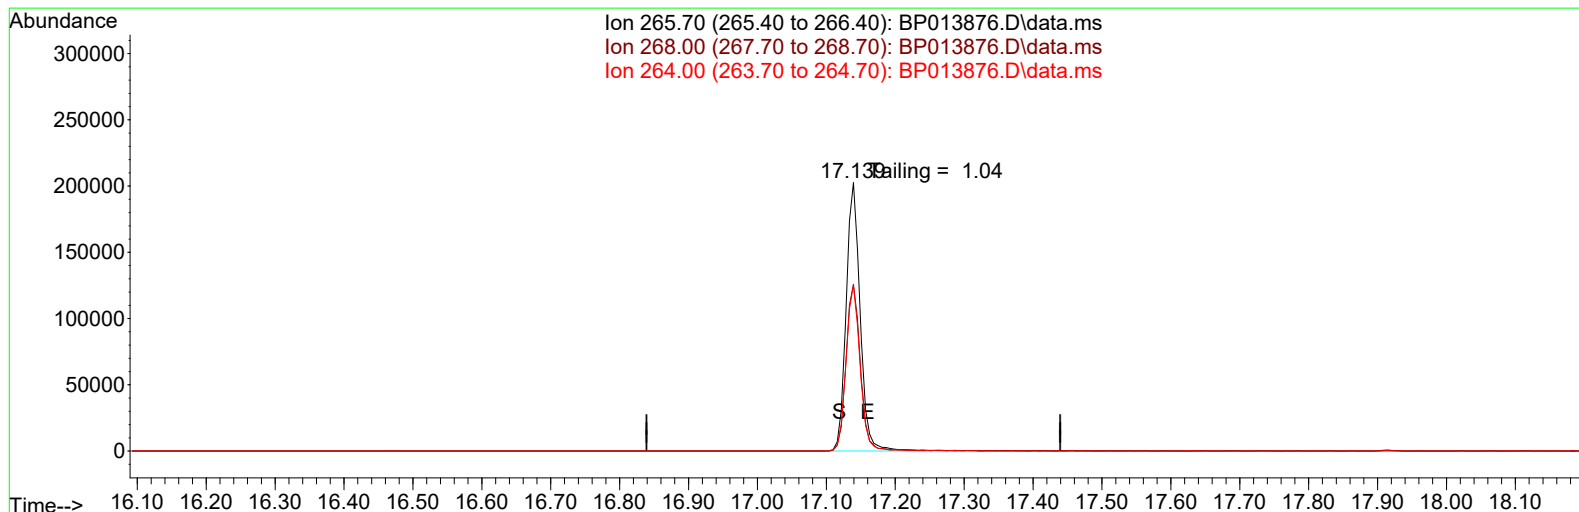

TIC: BP013876.D\data.ms

(70) Pentachlorophenol (C)




17.139min (-17.139) 0.00 ng

response 0

Ion	Exp%	Act%
265.70	100.00	0.00
268.00	63.60	0.00#
264.00	61.70	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022323\
 Data File : BP013876.D
 Acq On : 23 Feb 2023 12:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 24 03:34:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 24 01:37:56 2023
 Response via : Initial Calibration

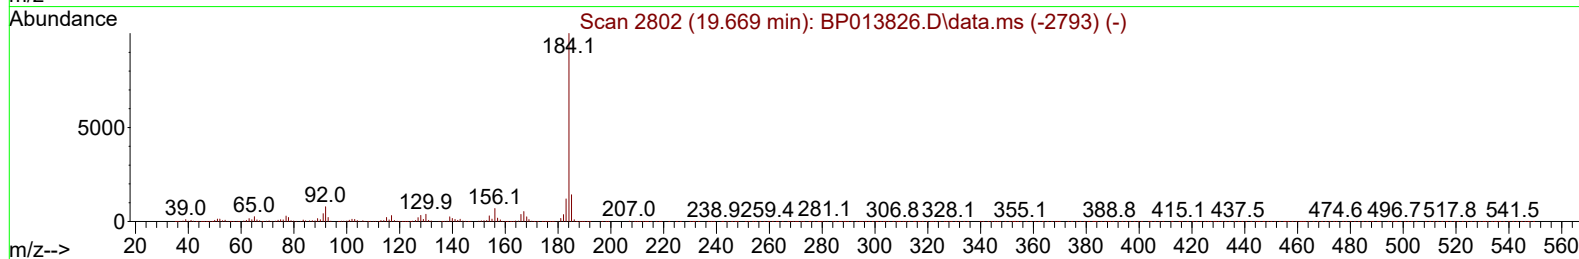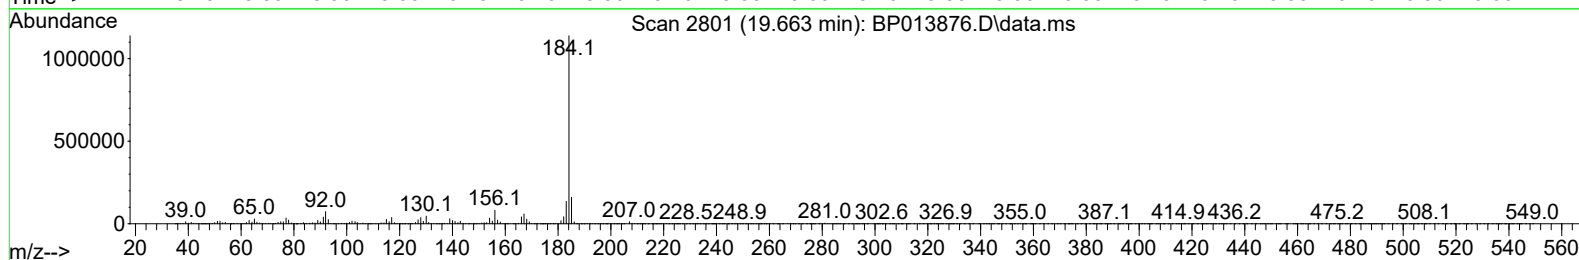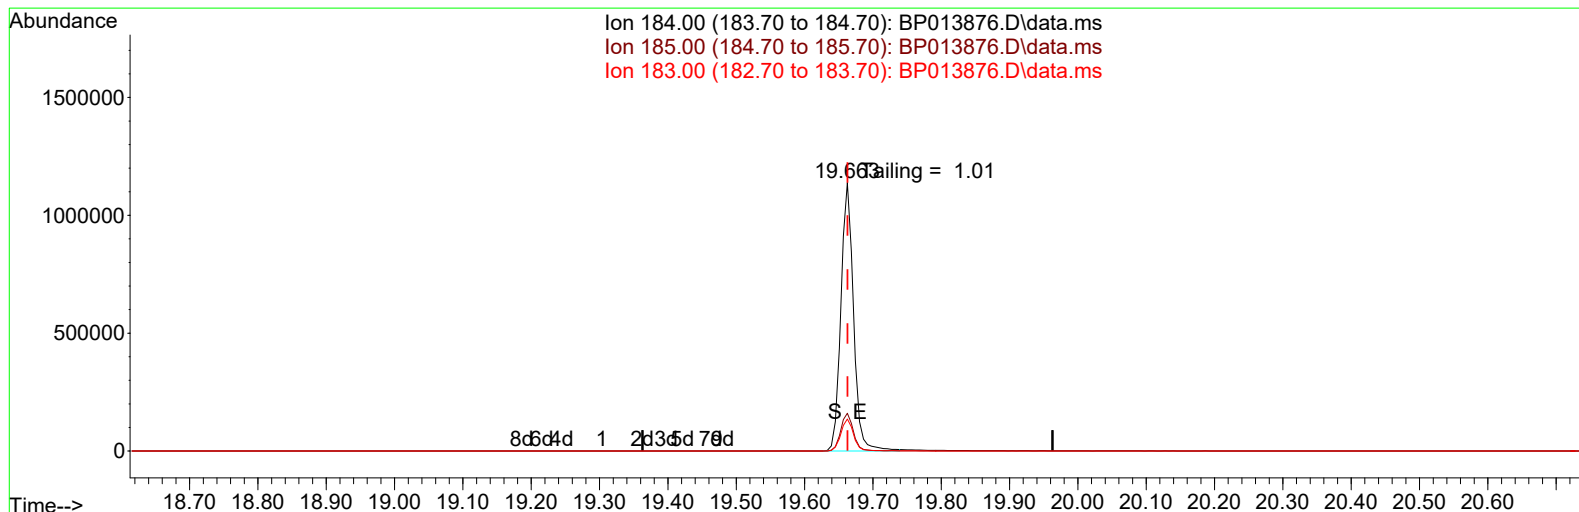

TIC: BP013876.D\data.ms

(77) Benzidine

19.663min (-0.000) 2277393.05 ng m

response 1465952

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.06
183.00	12.00	11.93
0.00	0.00	0.00