


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022323\
 Data File : BP013876.D
 Acq On : 23 Feb 2023 12:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 24 01:37:56 2023

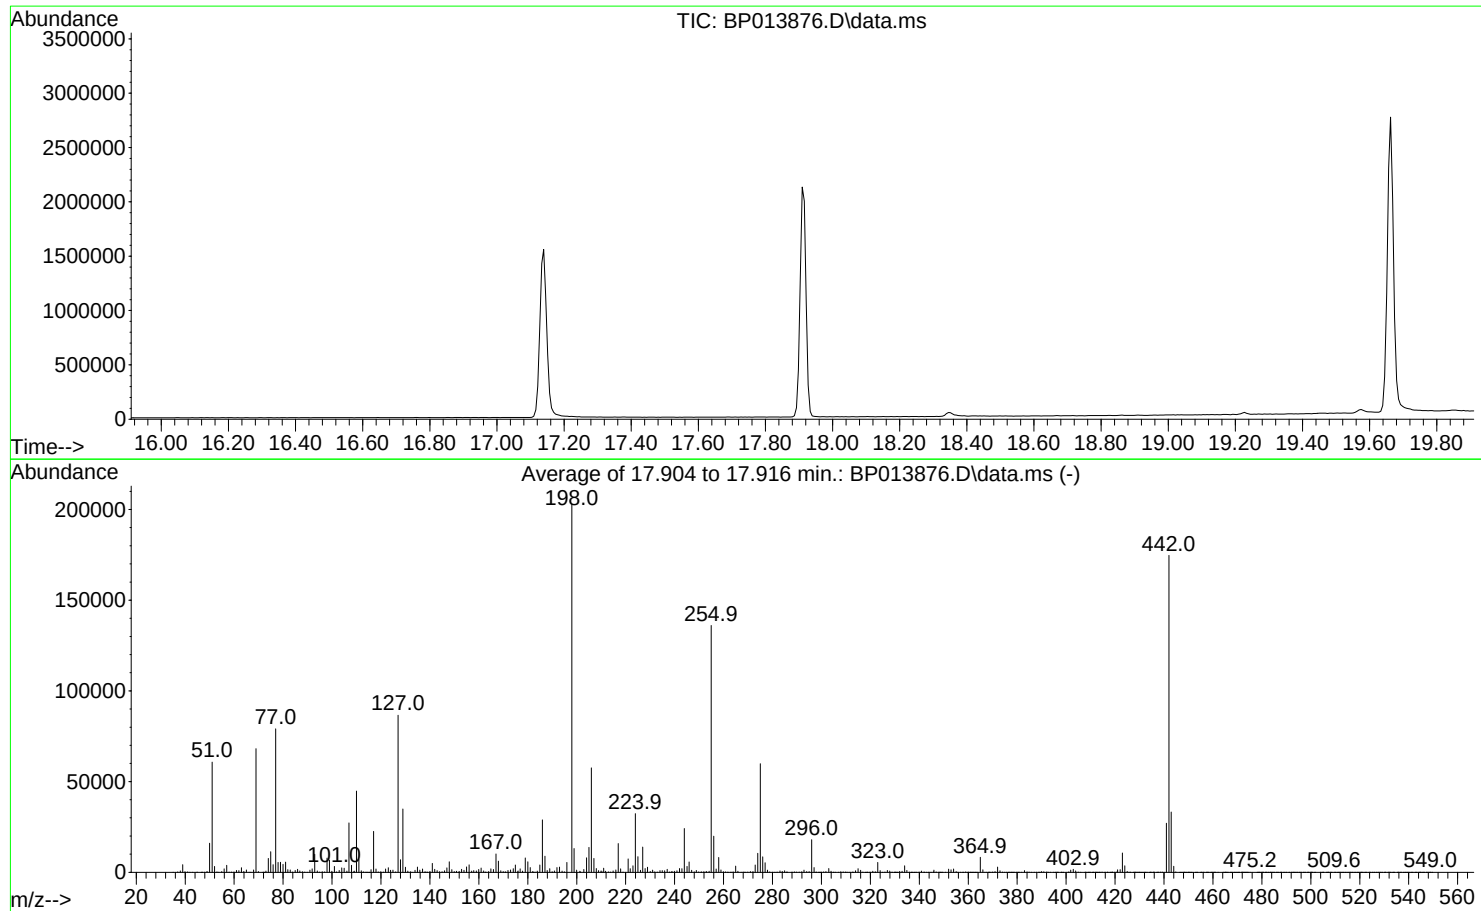




AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.9	60710	PASS
68	69	0.00	2	1.8	1242	PASS
69	198	0.00	100	33.6	68159	PASS
70	69	0.00	2	0.5	372	PASS
127	198	10	80	42.7	86598	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	202795	PASS
199	198	5	9	6.5	13094	PASS
275	198	10	60	29.5	59869	PASS
365	198	1	100	4.1	8275	PASS
441	198	0.01	100	13.3	27016	PASS
442	442	100	100	100.0	174707	PASS
443	442	15	24	19.0	33186	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022323\
Data File : BP013876.D
Acq On : 23 Feb 2023 12:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 24 03:34:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 01:37:56 2023
Response via : Initial Calibration

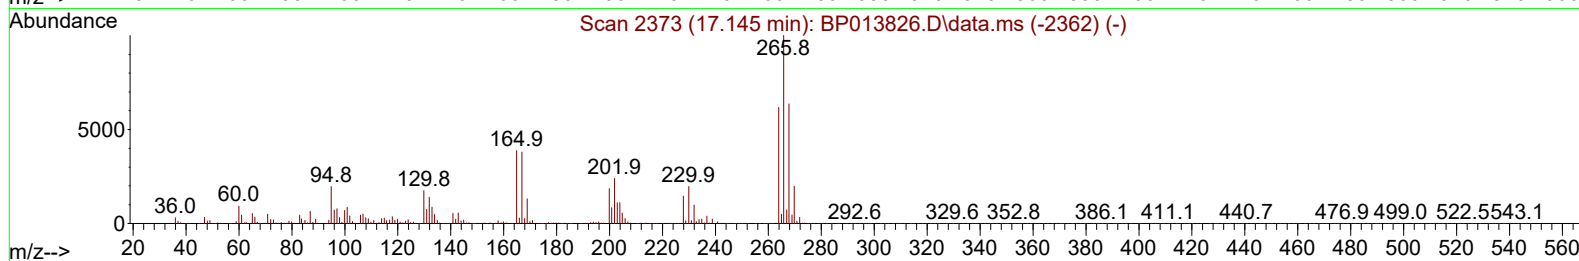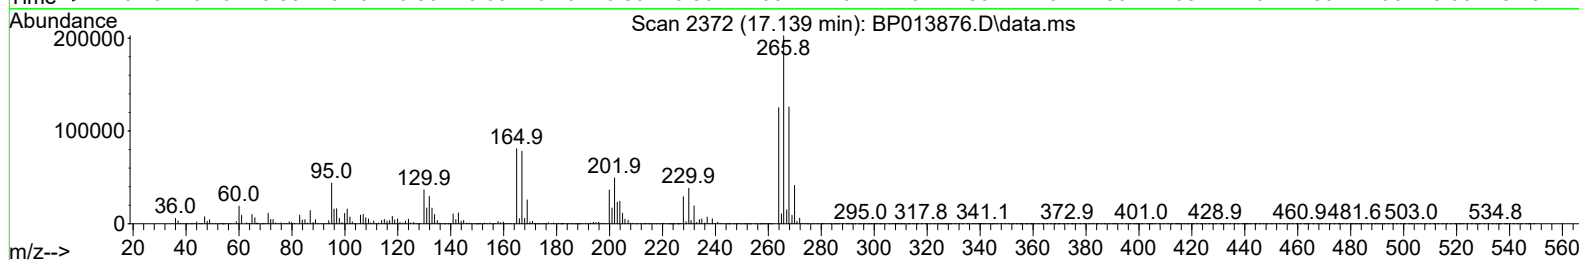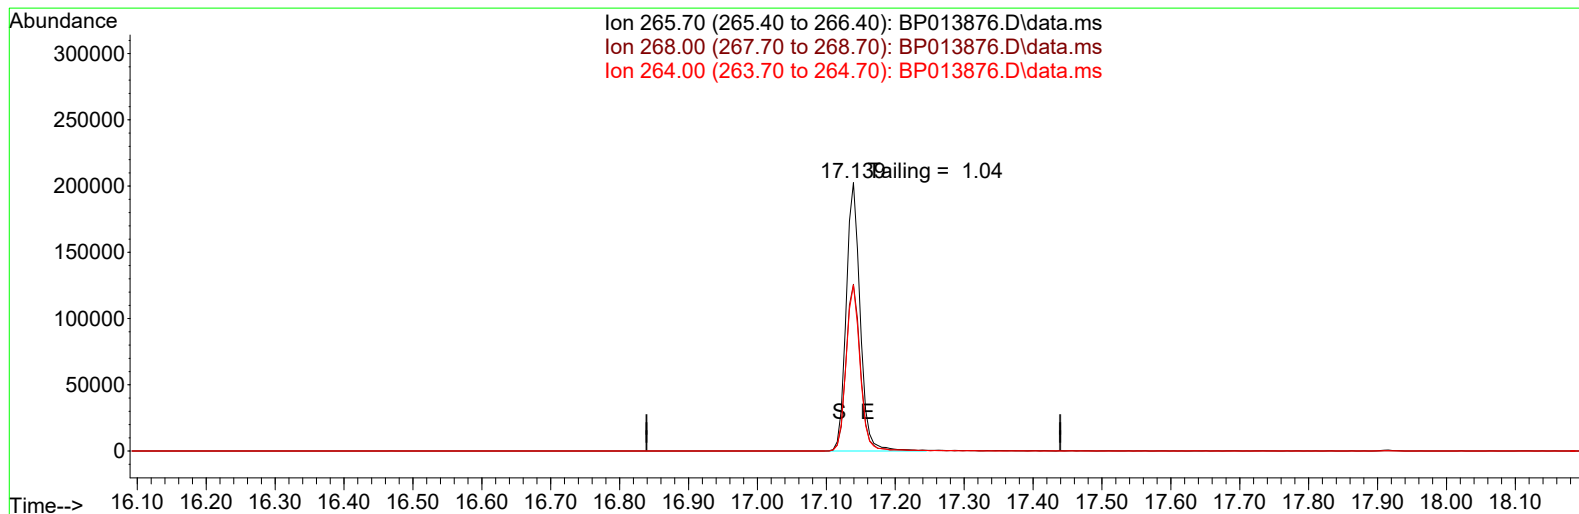

TIC: BP013876.D\data.ms

(70) Pentachlorophenol (C)

17.139min (-17.139) 0.00 ng




response 0

Ion	Exp%	Act%
265.70	100.00	0.00
268.00	63.60	0.00#
264.00	61.70	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022323\
 Data File : BP013876.D
 Acq On : 23 Feb 2023 12:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Feb 24 03:34:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 24 01:37:56 2023
 Response via : Initial Calibration

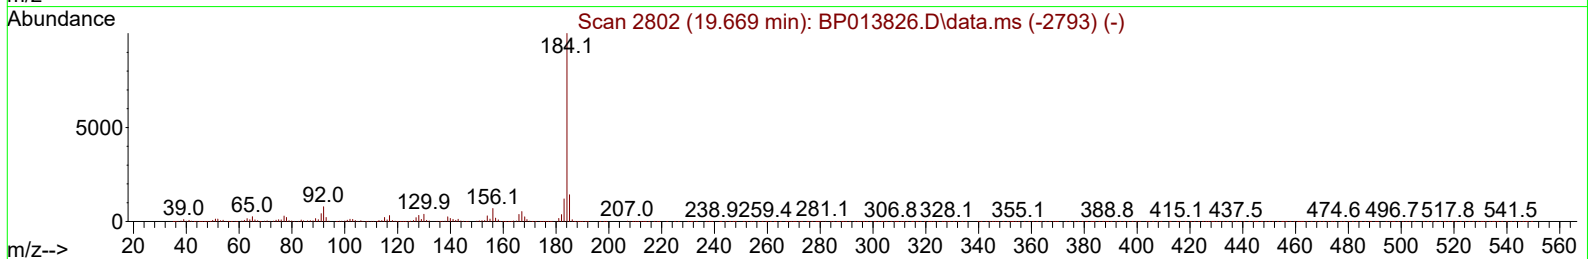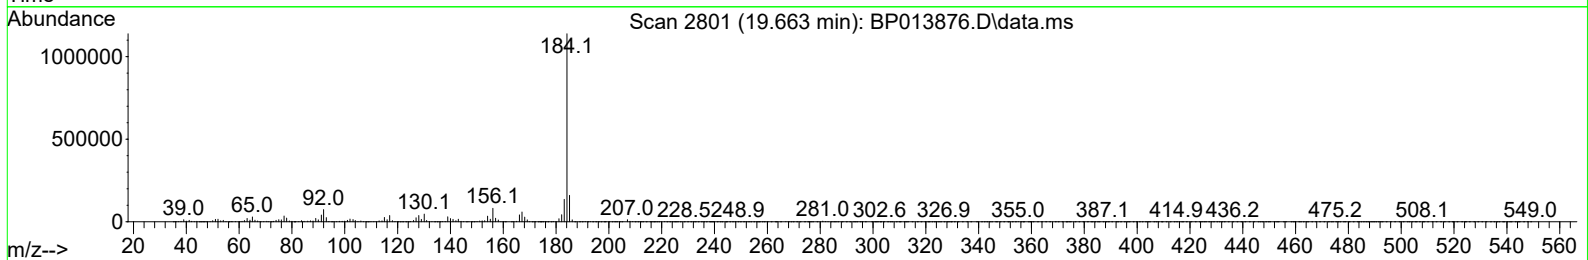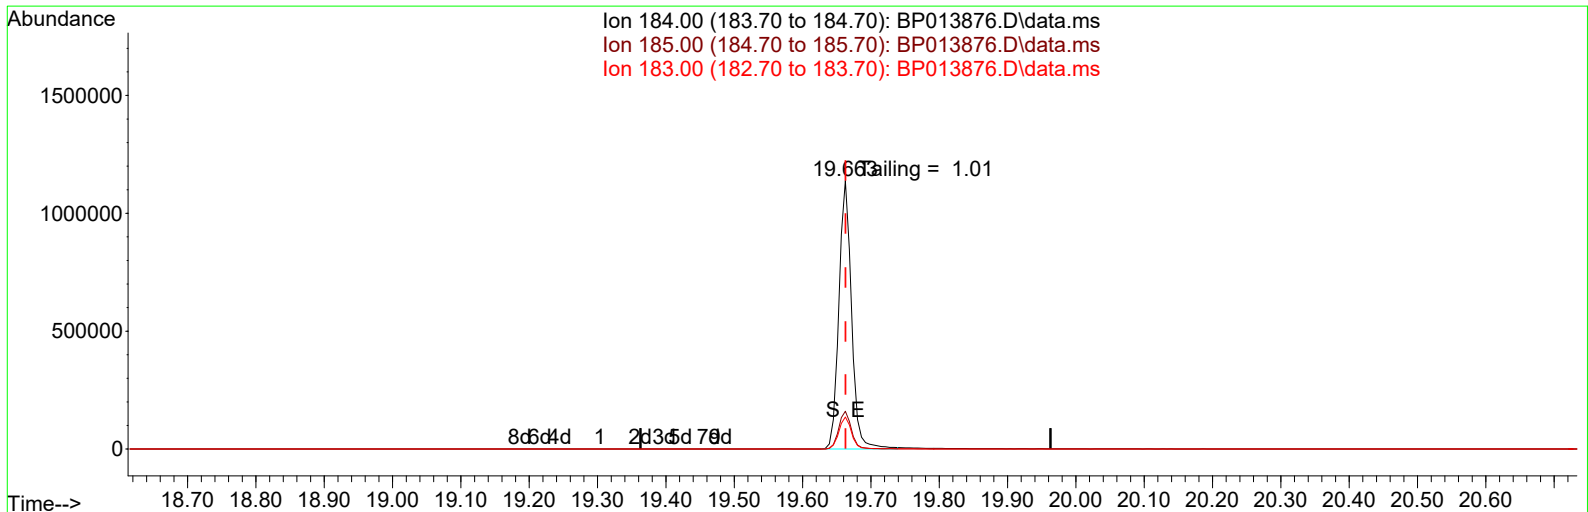

TIC: BP013876.D\data.ms

(77) Benzidine

19.663min (-0.000) 2277393.05 ng m

response 1465952

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.06
183.00	12.00	11.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/23/2023	BNA_P	<u>BP013876.D</u>
Compound Name	Response	Retention Time
DDT	779450	20.857
DDD	8798	20.48
DDE	433	19.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9231	788681	1.17

Instrument :
BNA_P
ClientSampleId :
DFTPP