
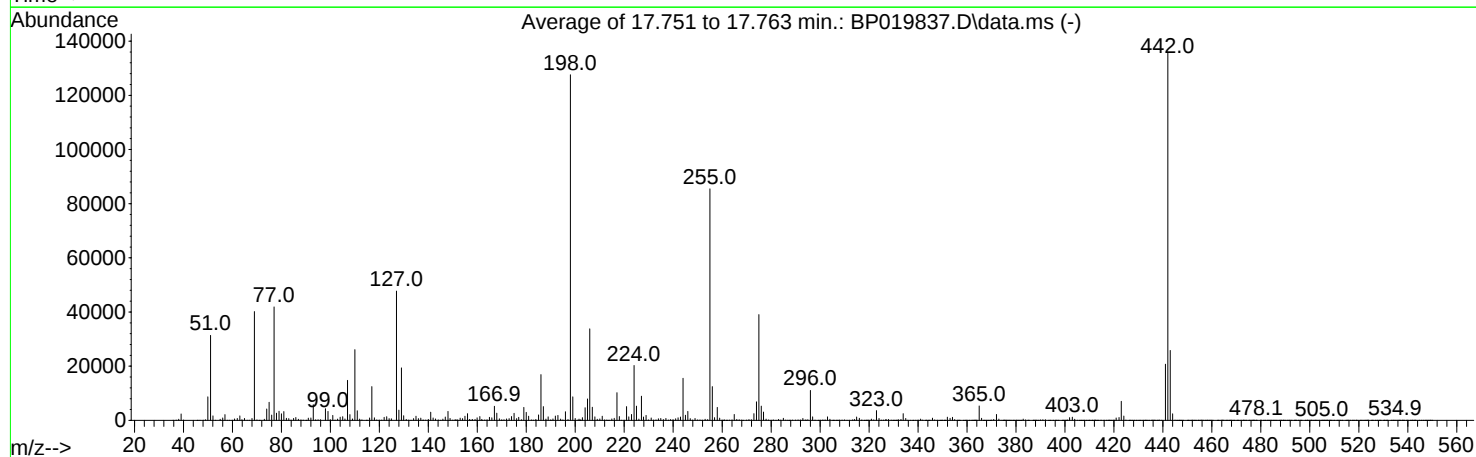


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022324\
Data File : BP019837.D
Acq On : 23 Feb 2024 09:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 23 13:10:49 2024

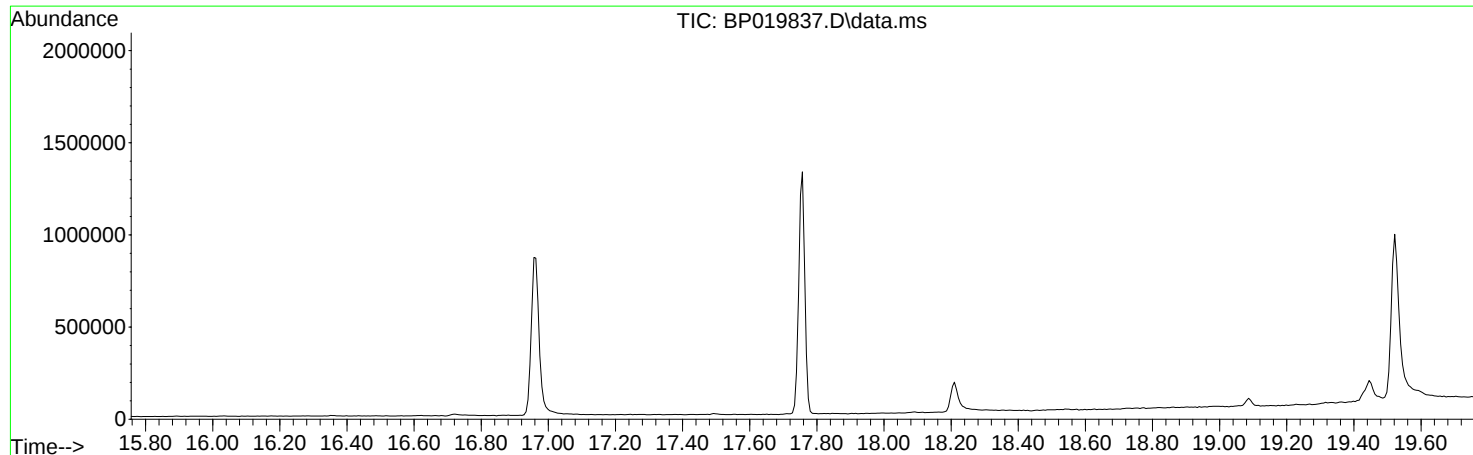




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.6	31368	PASS
68	69	0.00	2	1.8	706	PASS
69	198	0.00	100	31.5	40187	PASS
70	69	0.00	2	0.5	200	PASS
127	198	10	80	37.4	47712	PASS
197	198	0.00	2	0.3	320	PASS
198	198	100	100	100.0	127630	PASS
199	198	5	9	6.8	8710	PASS
275	198	10	60	30.6	39064	PASS
365	198	1	100	4.2	5303	PASS
441	198	0.01	100	16.3	20757	PASS
442	442	100	100	100.0	135810	PASS
443	442	15	24	19.0	25804	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022324\
Data File : BP019837.D
Acq On : 23 Feb 2024 09:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 23 09:50:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 19 23:35:42 2024
Response via : Initial Calibration

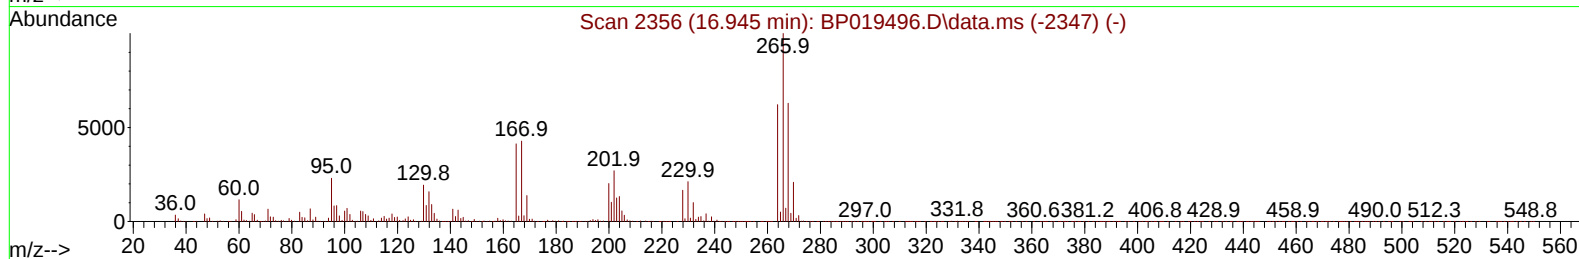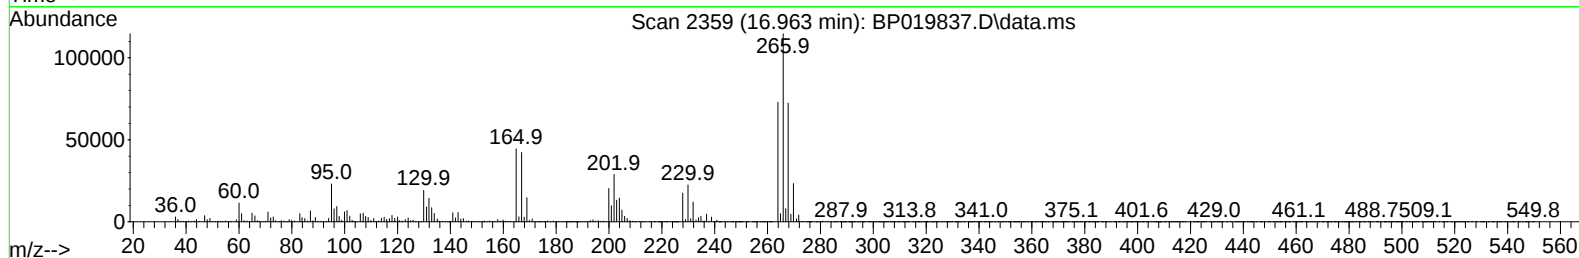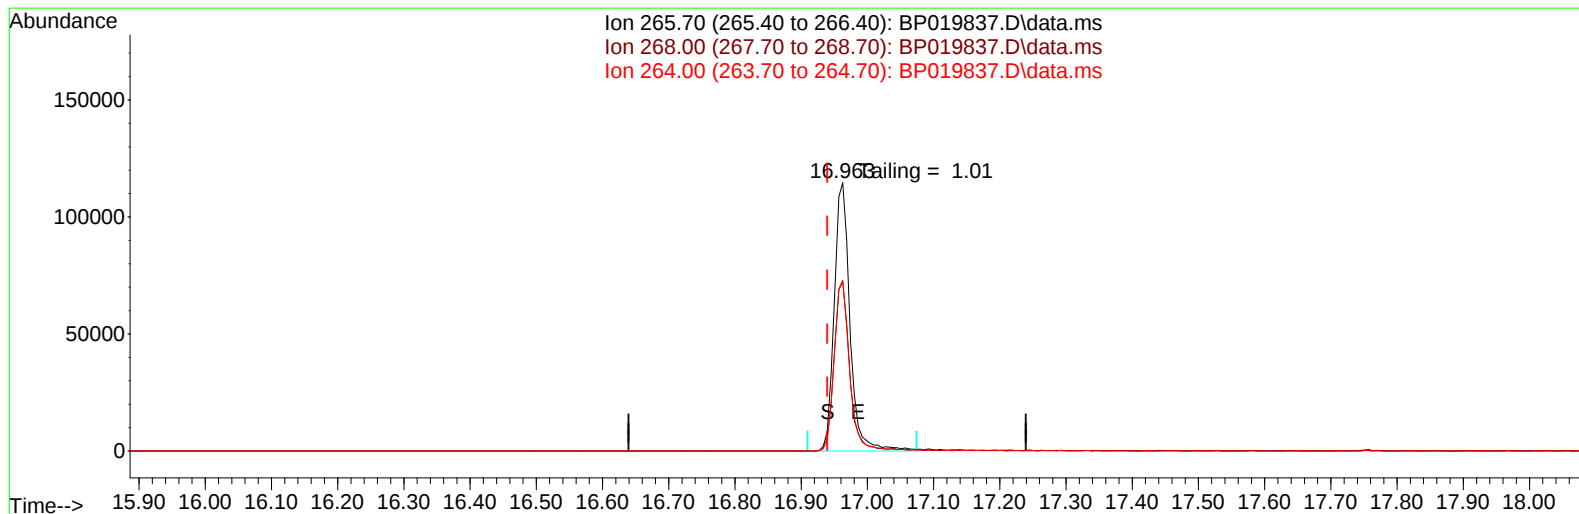

TIC: BP019837.D\data.ms

(70) Pentachlorophenol (C)

16.963min (+ 0.023) 204385.54 ng




response 189527

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	63.17
264.00	62.10	63.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022324\
Data File : BP019837.D
Acq On : 23 Feb 2024 09:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 23 09:50:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 19 23:35:42 2024
Response via : Initial Calibration

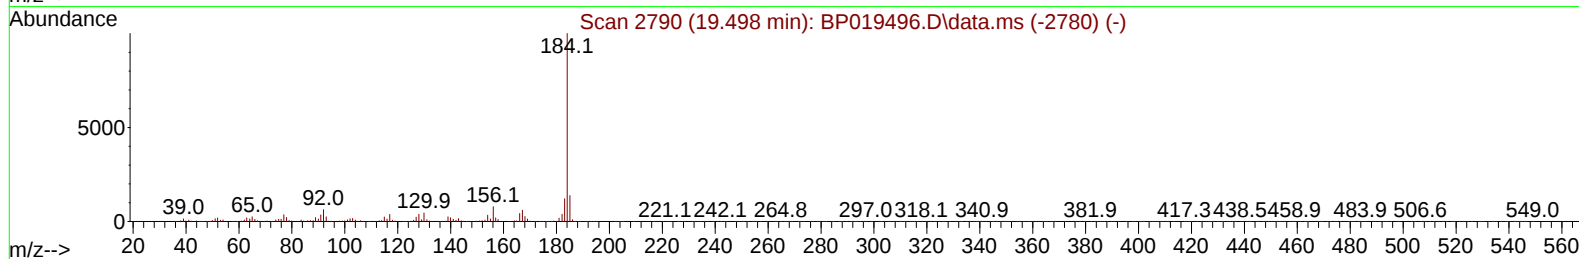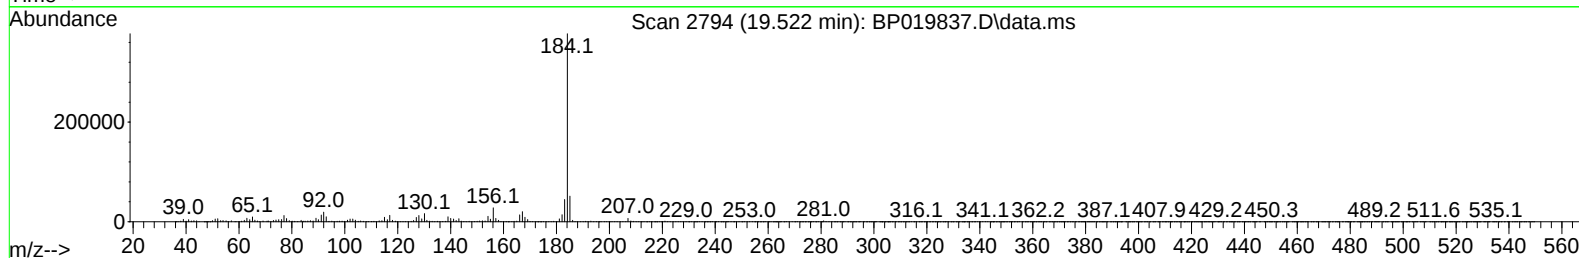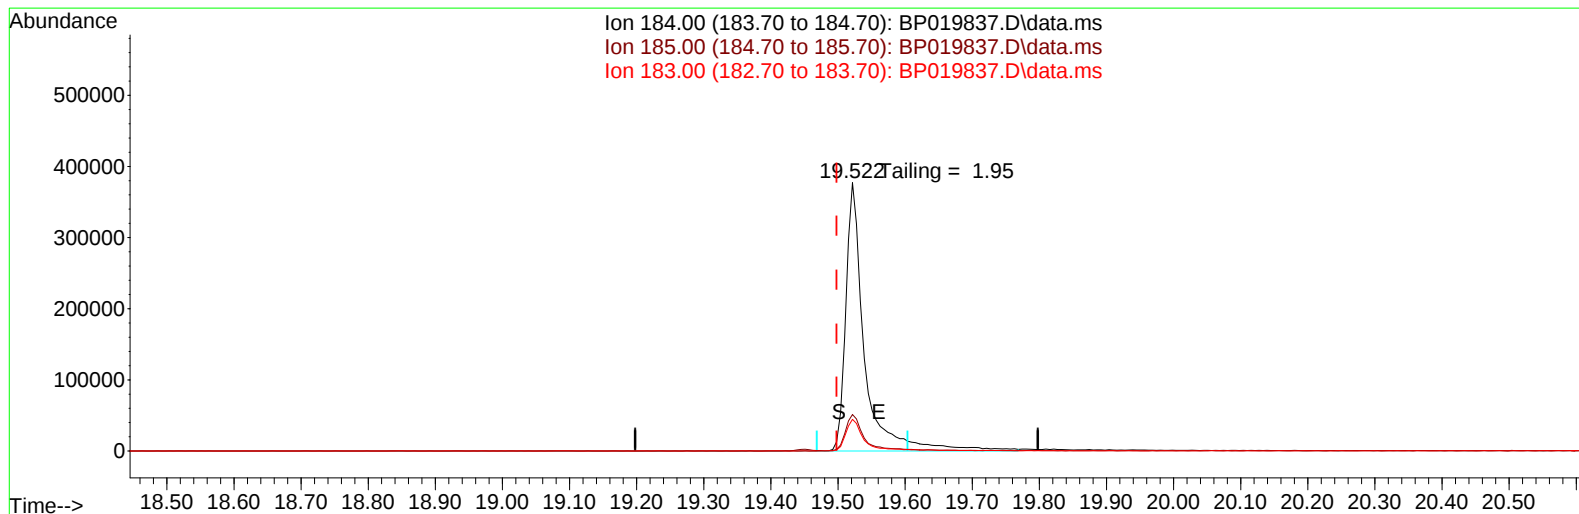

TIC: BP019837.D\data.ms

(77) Benzidine

19.522min (+ 0.023) 154926.80 ng m

response 738493

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.60
183.00	12.10	11.82
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/23/2024	BNA_P	<u>BP019837.D</u>
Compound Name	Response	Retention Time
DDT	482899	20.721
DDD	18252	20.292
DDE	1847	19.786
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20099	502998	4.00

Instrument :
BNA_P
ClientSampleId :
DFTPP