
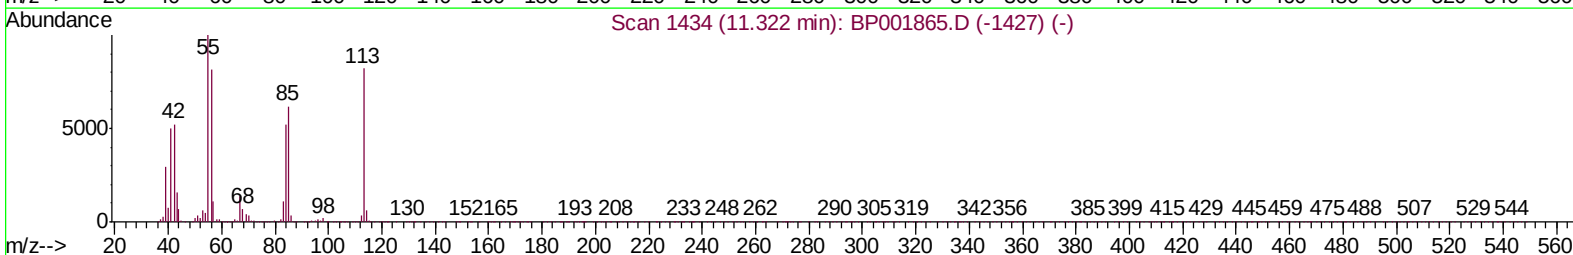
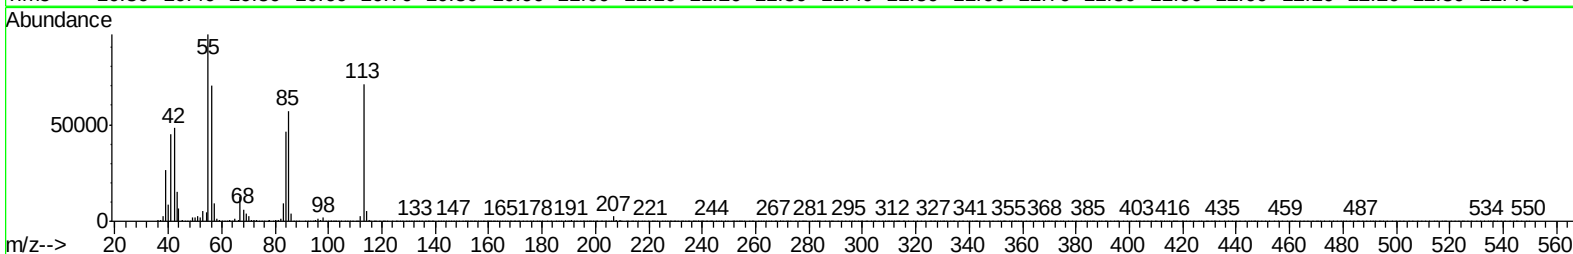


Data File : BP001883.D
Acq On : 25 Feb 2020 03:54
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Feb 25 06:01:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 05:55:24 2020
Response via : Initial Calibration

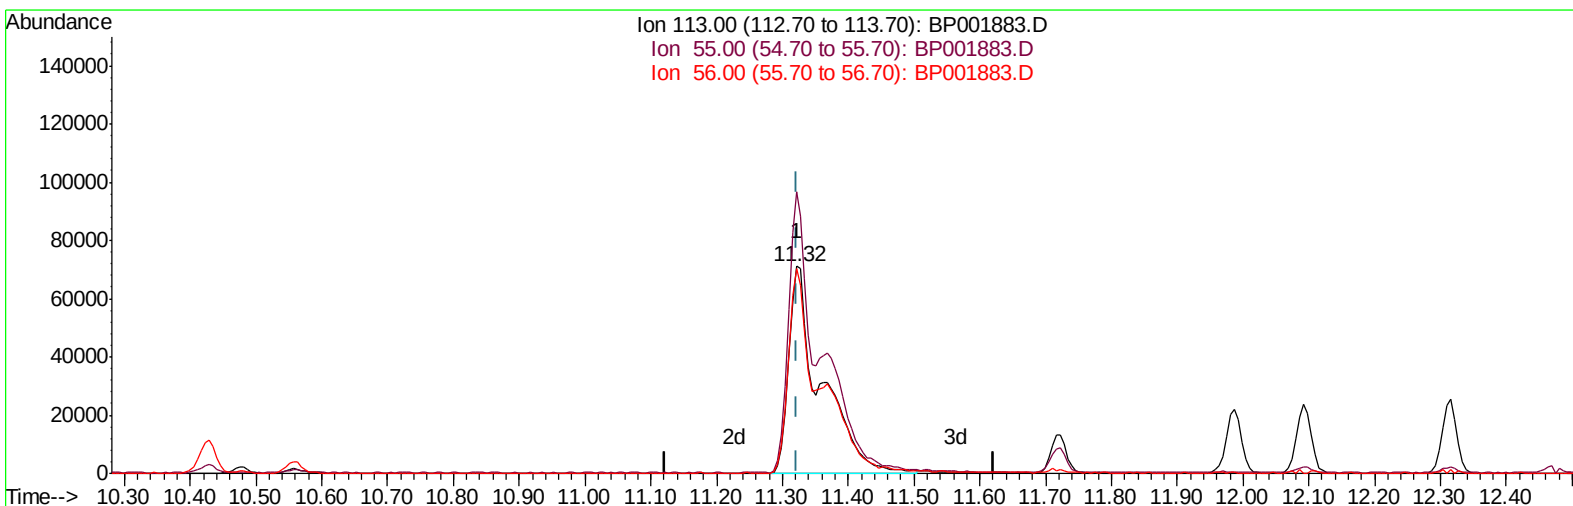

TIC: BP001883.D

(32) Caprolactam

11.322min (-0.000) 24.00ng/ul m

response 242503

Ion	Exp%	Act%
113.00	100	100
55.00	138.80	135.88
56.00	107.70	98.95
0.00	0.00	0.00