
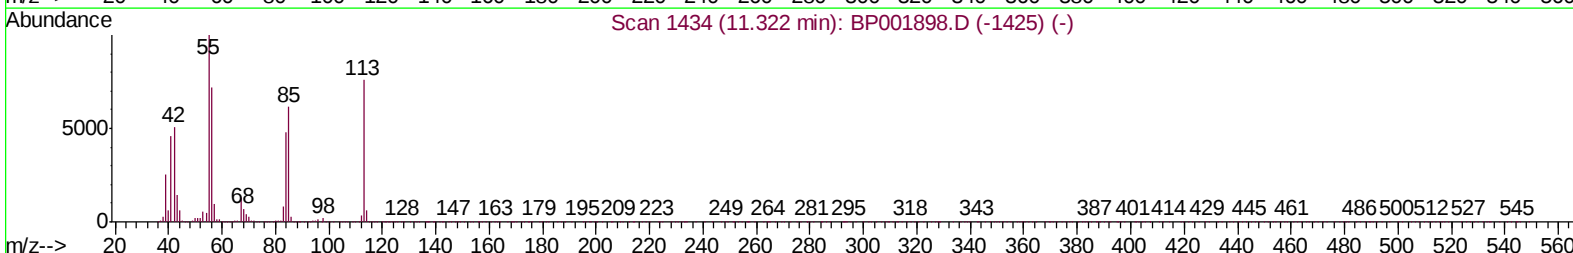
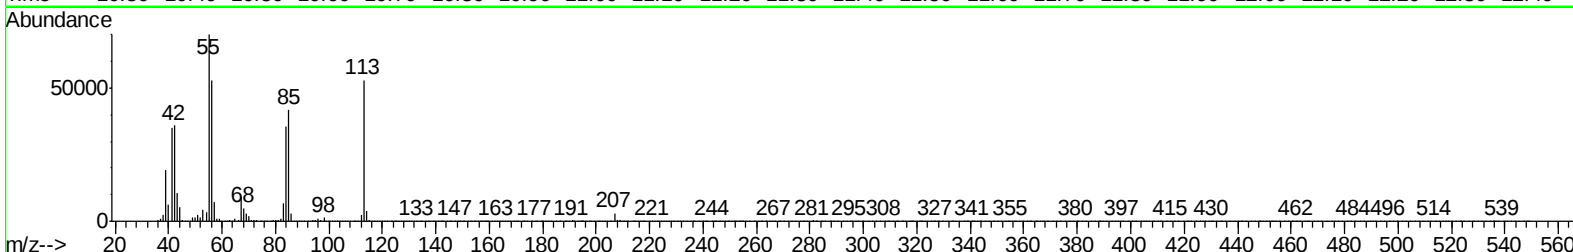


Data File : BP001910.D
Acq On : 25 Feb 2020 22:11
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 59 Sample Multiplier: 1

Quant Time: Feb 26 04:41:36 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 26 04:37:11 2020
Response via : Initial Calibration

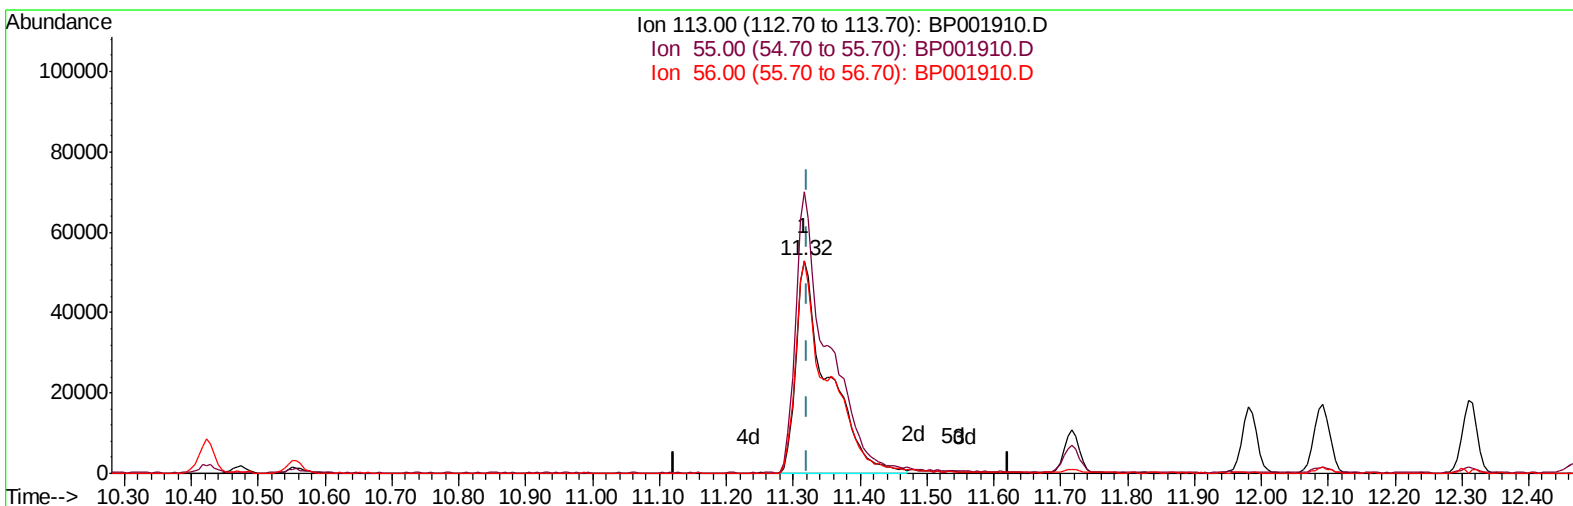

TIC: BP001910.D

(32) Caprolactam

11.316min (-0.006) 25.30ng/ul m

response 177063

Ion	Exp%	Act%
113.00	100	100
55.00	138.80	132.26
56.00	107.70	99.56
0.00	0.00	0.00