
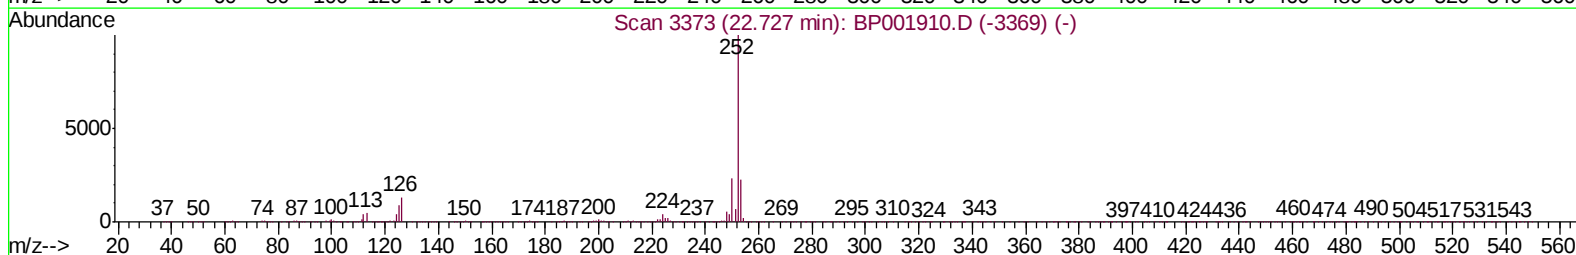
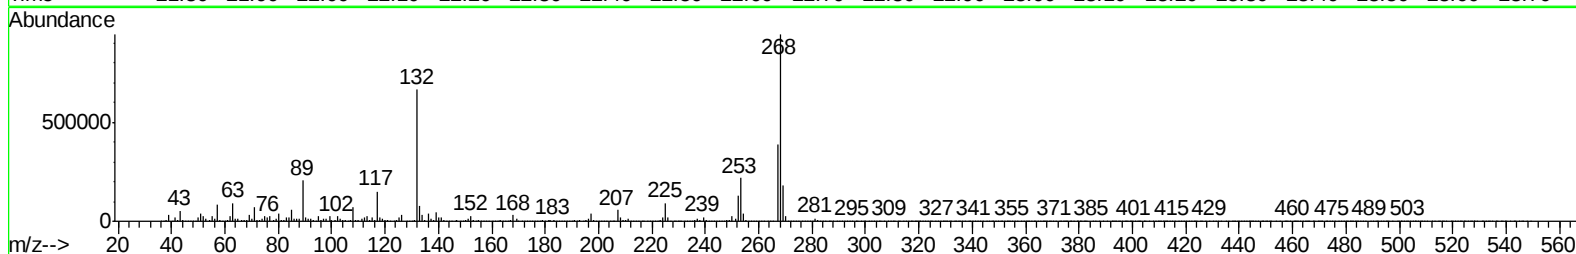


Data File : BP001915.D
Acq On : 26 Feb 2020 01:35
Operator : CG/JU
Sample : L1543-11
Misc :
ALS Vial : 64 Sample Multiplier: 1

Quant Time: Feb 26 05:56:21 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 26 05:53:41 2020
Response via : Initial Calibration

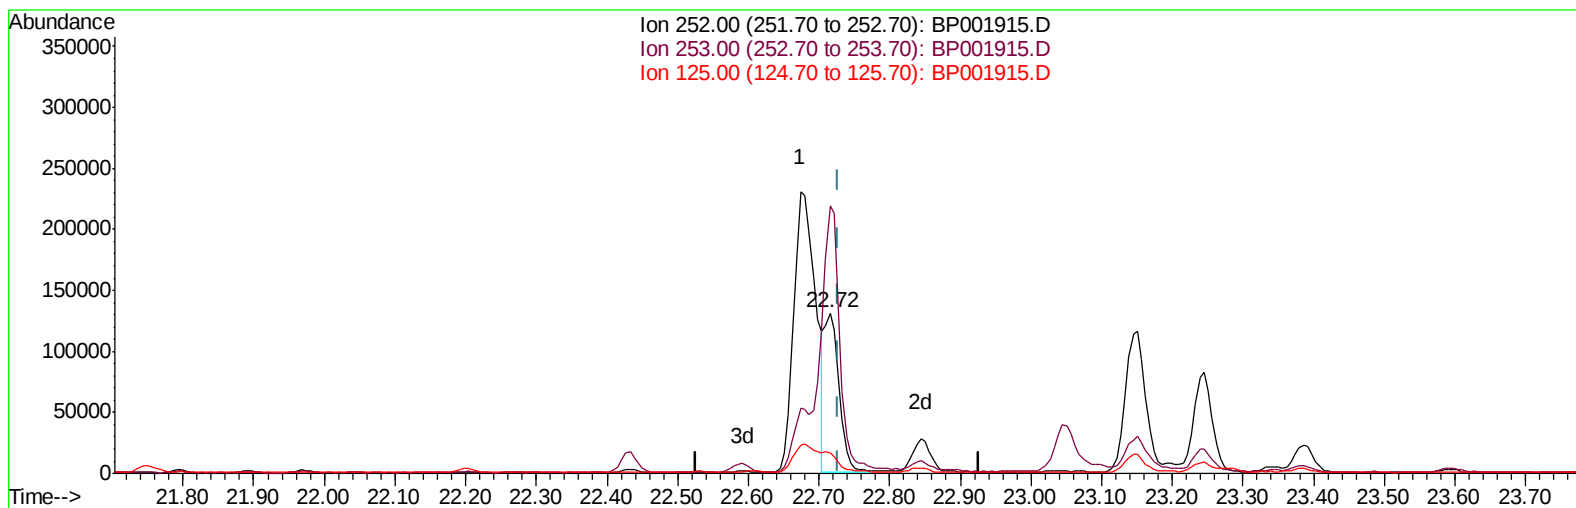

TIC: BP001915.D

(89) Benzo(k)fluoranthene

22.715min (-0.012) 1.22ng/ul m

response 186505

Ion	Exp%	Act%
252.00	100	100
253.00	22.20	167.15#
125.00	10.00	13.00#
0.00	0.00	0.00