
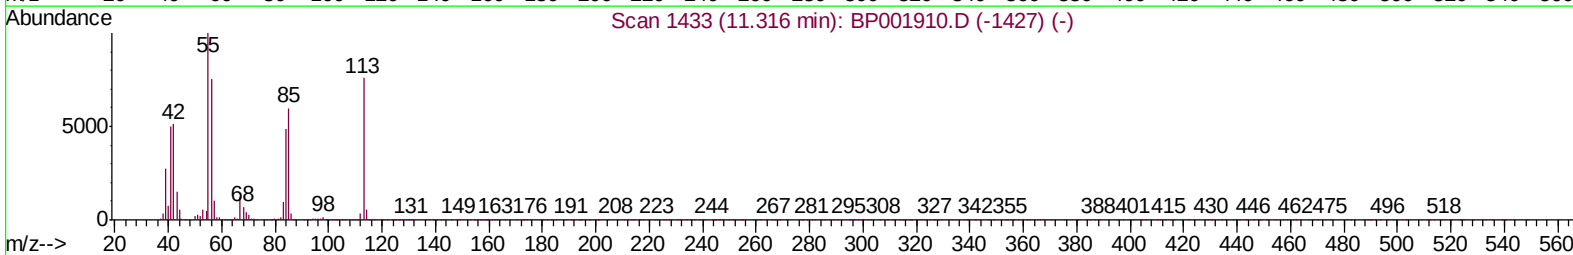
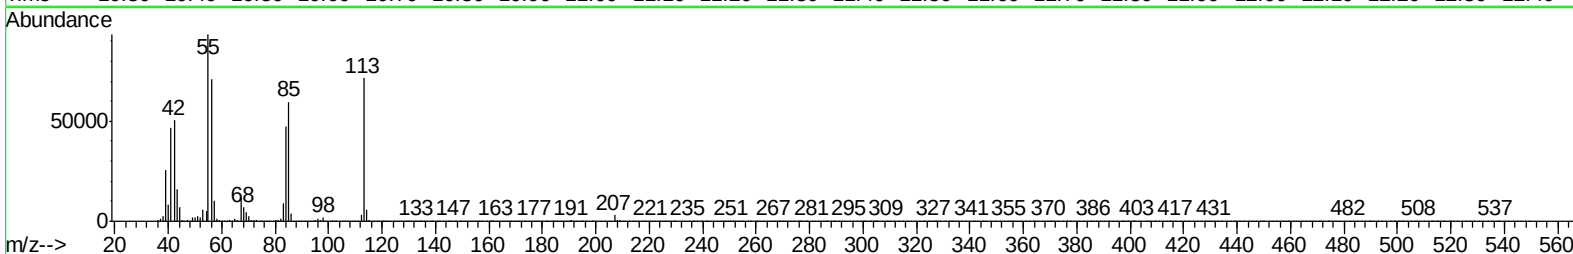


Data File : BP001917.D
Acq On : 26 Feb 2020 02:42
Operator : CG/JU
Sample : SSTDCCC020EC
Misc :
ALS Vial : 66 Sample Multiplier: 1

Quant Time: Feb 26 05:56:43 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 26 05:53:41 2020
Response via : Initial Calibration

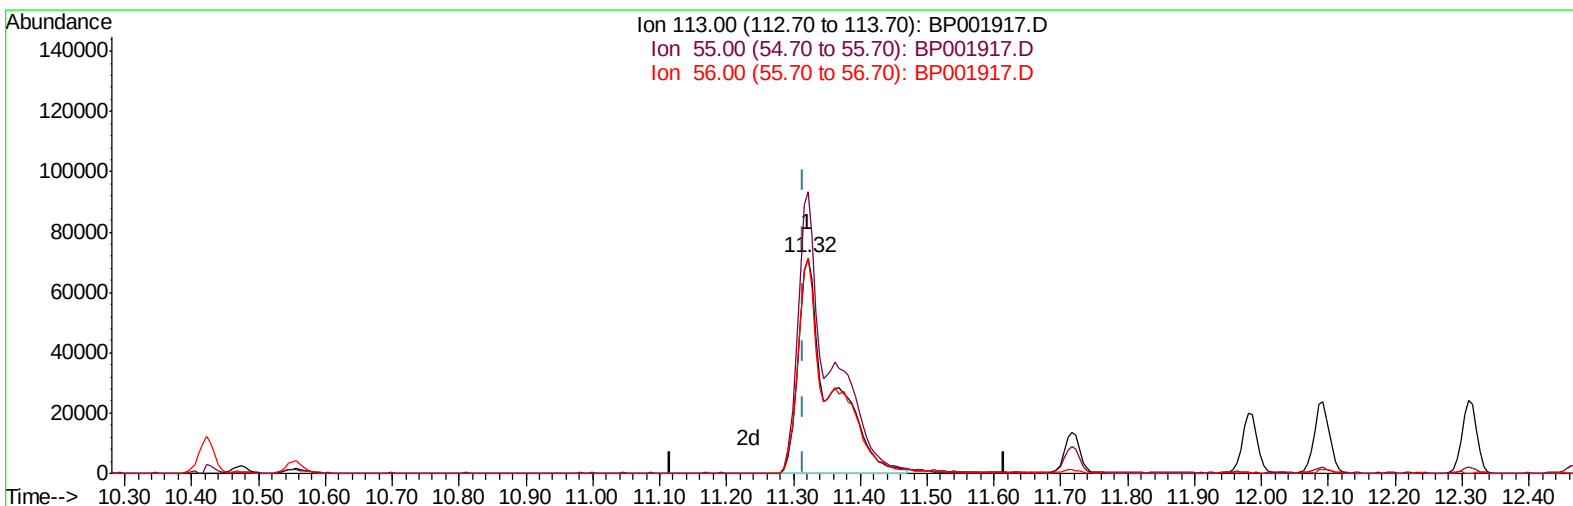

TIC: BP001917.D

(32) Caprolactam

11.322min (+0.006) 24.40ng/ul m

response 239652

Ion	Exp%	Act%
113.00	100	100
55.00	138.80	130.61
56.00	107.70	99.69
0.00	0.00	0.00