

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022420\
 Data File : BP001921.D
 Acq On : 26 Feb 2020 11:11
 Operator : CG/JU
 Sample : L1543-13
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Feb 27 03:13:05 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 26 05:53:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	311505	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	1344055	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	866409	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	1998494	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2167021	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	2134196	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.17	96	33396	4.45	ng/uL	0.00
5) Phenol-d5	6.83	99	688447	29.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	389327	28.47	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	612535	32.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	561108	30.05	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	306226	33.66	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	341068	41.45	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	637148	32.56	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	816014	35.26	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	2066363	33.99	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	2433057	32.50	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	360989	34.10	ng/ul	0.00
58) Fluorene-d10	15.28	176	1811956	33.14	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	249114	31.62	ng/ul	0.00
71) Anthracene-d10	17.13	188	3122120	35.46	ng/ul	0.00
79) Pyrene-d10	19.38	212	3828261	34.43	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.20	264	3966989	38.49	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.85	94	36561	1.466 ng/ul	92
45) Dimethylphthalate	13.75	163	261484	4.086 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022420\
Data File : BP001921.D
Acq On : 26 Feb 2020 11:11
Operator : CG/JU
Sample : L1543-13
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Feb 27 03:13:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 26 05:53:41 2020
Response via : Initial Calibration




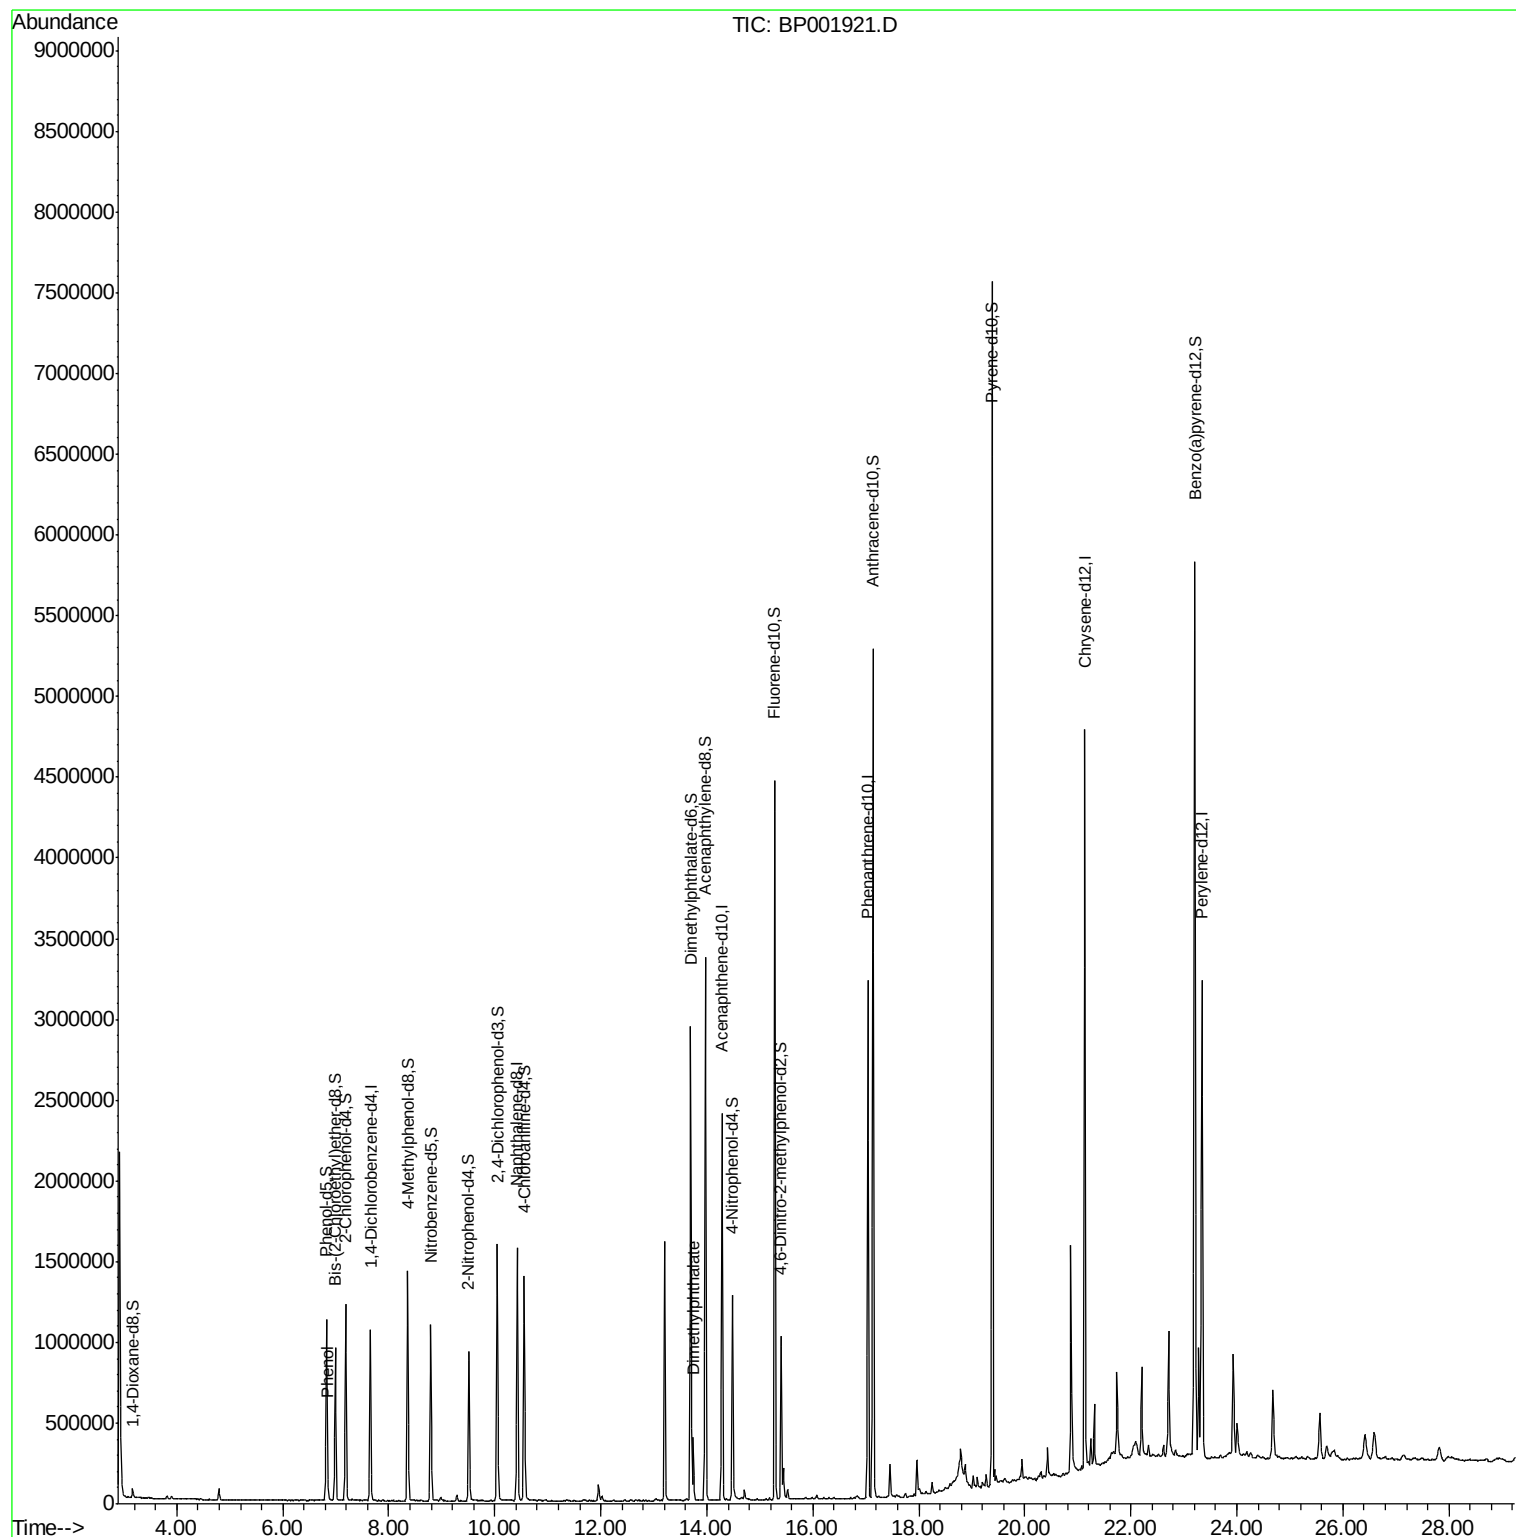


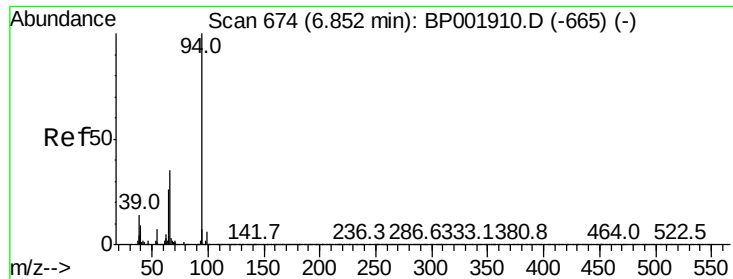

#6
Phenol
Concen: 1.466 ng/ul
RT: 6.85 min Scan# 674
Delta R.T. 0.00 min
Lab File: BP001921.D
Acq: 26 Feb 2020 11:11

Instrument :
BNA_P
ClientSampleId :

Tot Ion	94	Resp	36561
Ion Ratio	Lower	Upper	
94	100		
65	26.8	19.8	29.6
66	39.2	26.6	39.8

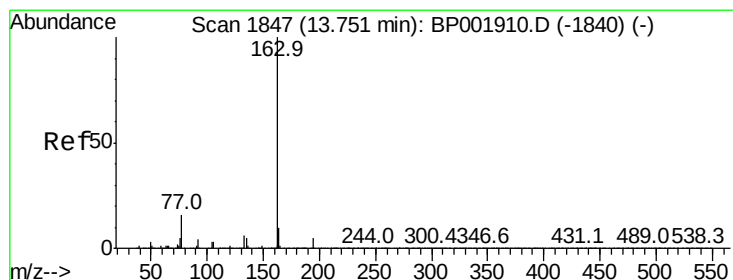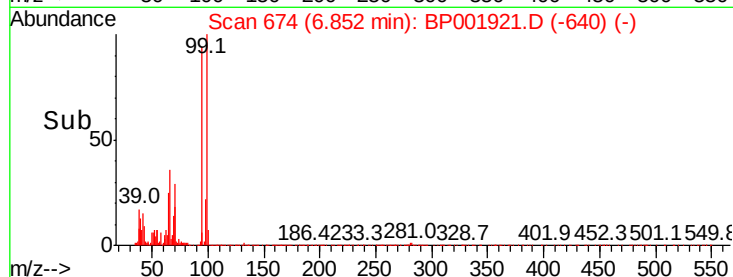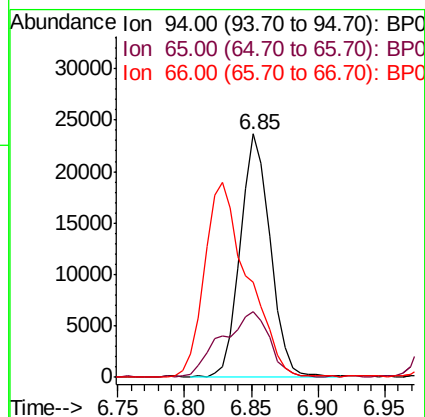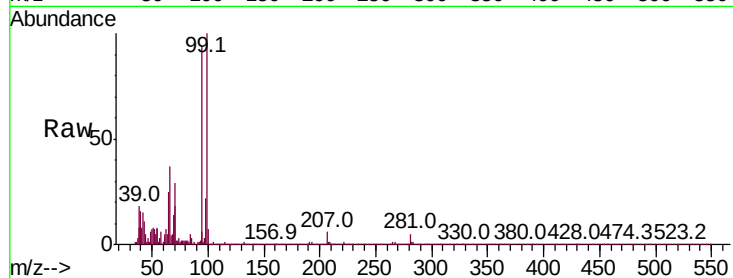

#45
Dimethylphthalate
Concen: 4.086 ng/ul
RT: 13.75 min Scan# 1846
Delta R.T. -0.01 min
Lab File: BP001921.D
Acq: 26 Feb 2020 11:11

Tgt Ion	163	Resp	261484
Ion Ratio	Lower	Upper	
163	100		
194	4.2	3.5	5.3
164	9.7	8.0	12.0

