

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022420\
Quantitation Report (QT Reviewed)


Data File : BP001869.D
Acq On : 24 Feb 2020 20:00
Operator : CG/JU
Sample : L1536-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB6X3

Manual Integrations
APPROVED

mohammad
2/25/2020 3:42:29 PM

Quant Time: Feb 25 06:17:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 05:55:24 2020
Response via : Initial Calibration

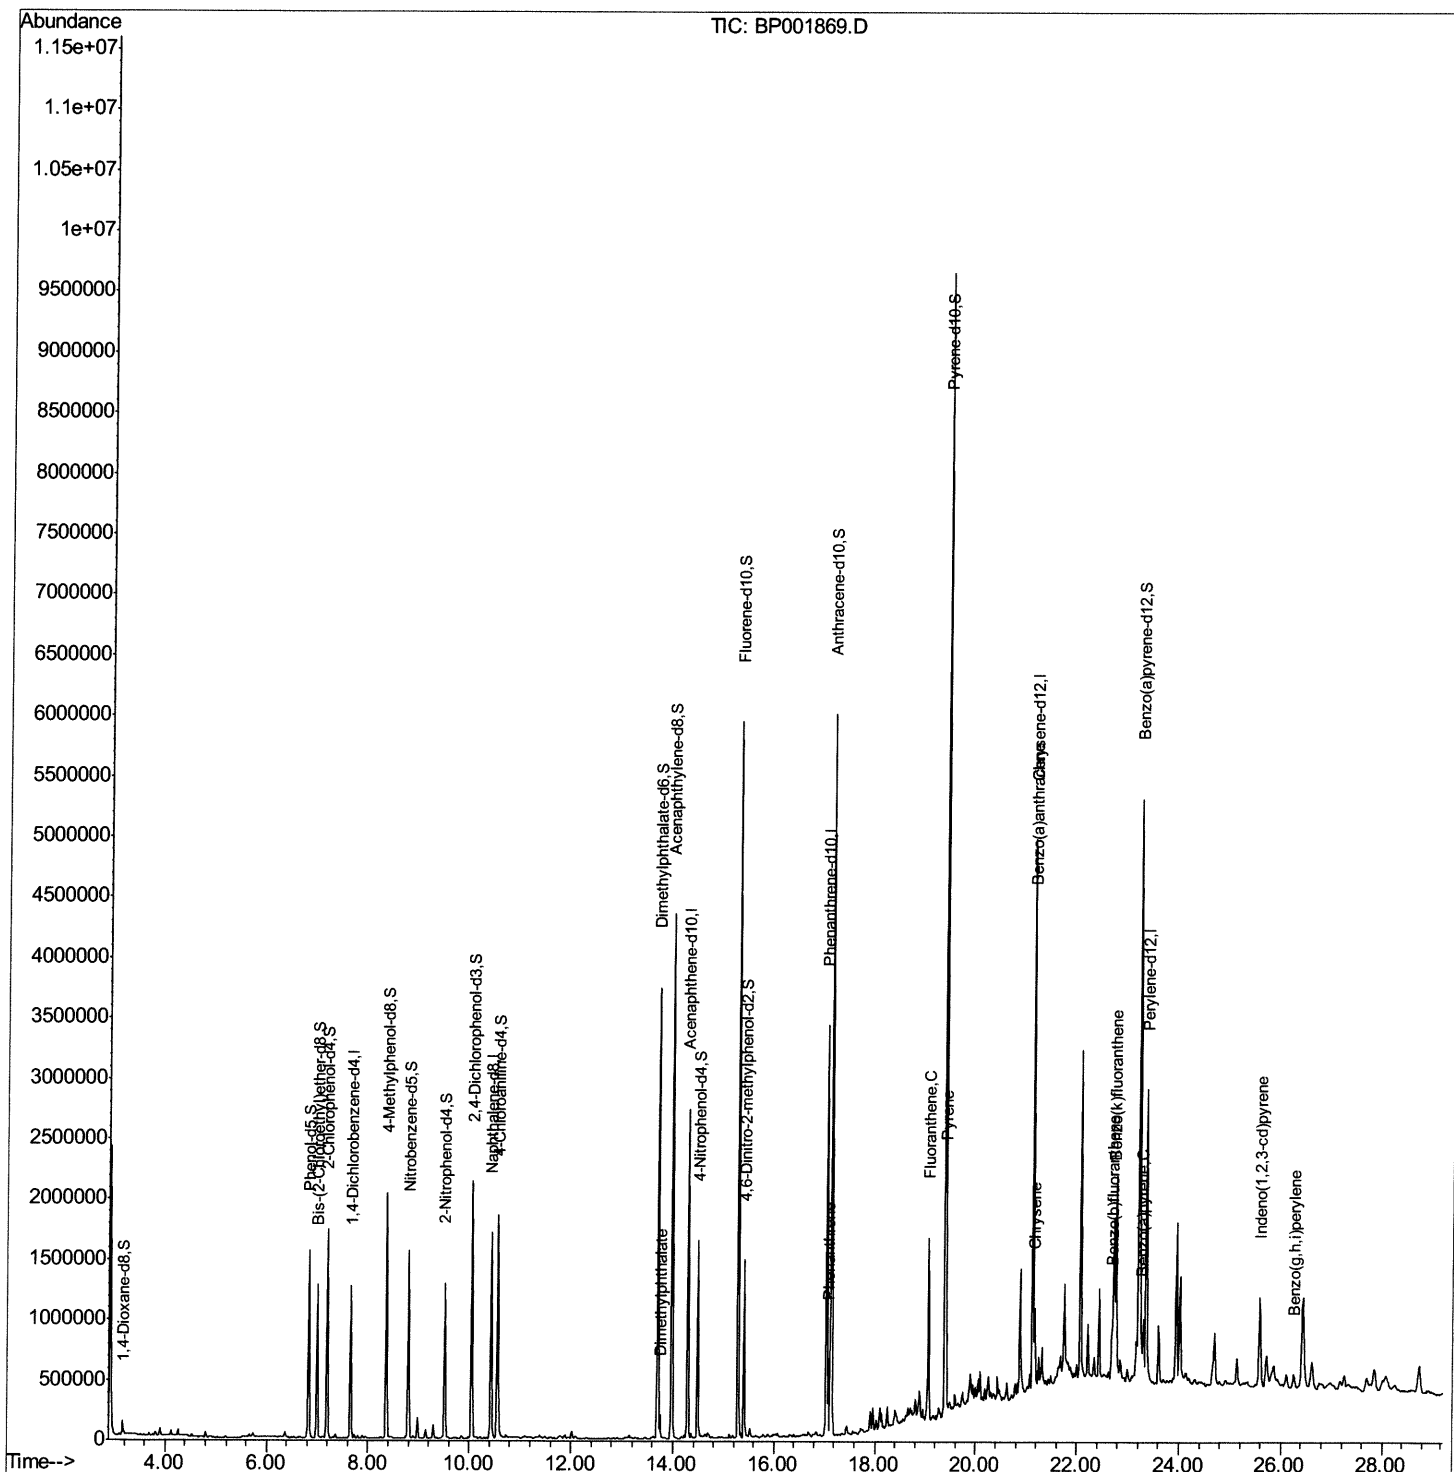

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022420\
Quantitation Report (Qedit)




Data File : BP001869.D
Acq On : 24 Feb 2020 20:00
Operator : CG/JU
Sample : L1536-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB6X3

Manual Integrations
APPROVED

mohammad
2/25/2020 3:42:29 PM

Quant Time: Feb 25 05:58:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 05:55:24 2020
Response via : Initial Calibration

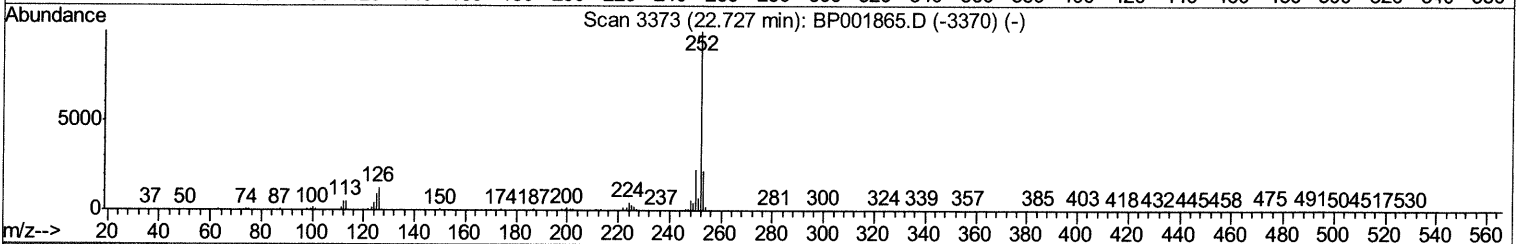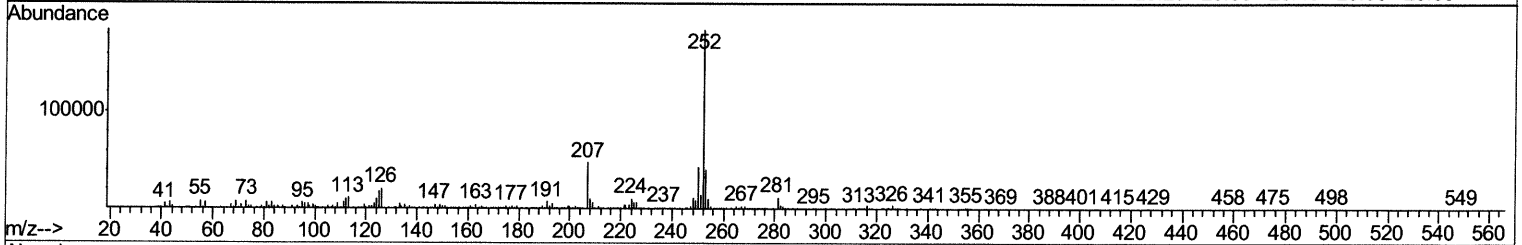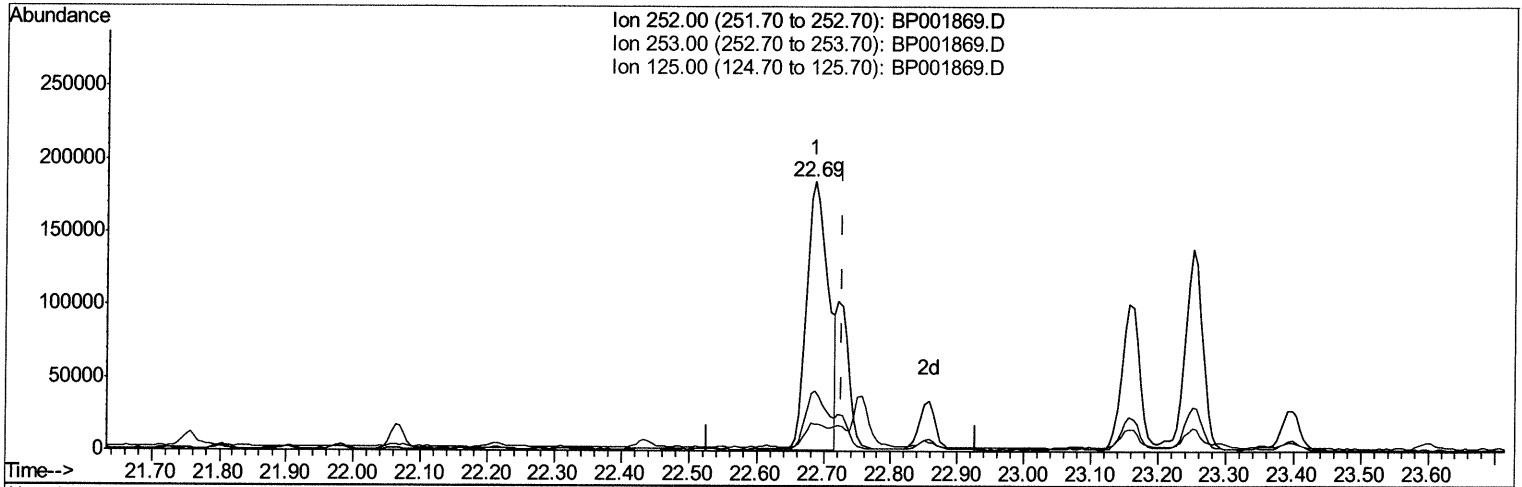

TIC: BP001869.D

(89) Benzo(k)fluoranthene
22.686min (-0.041) 3.88ng/ul
response 421693

Ion	Exp%	Act%
252.00	100	100
253.00	22.20	22.25
125.00	10.00	9.96
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022420\
Quantitation Report (Qedit)




Data File : BP001869.D
Acq On : 24 Feb 2020 20:00
Operator : CG/JU
Sample : L1536-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB6X3

Manual Integrations
APPROVED

mohammad
2/25/2020 3:42:29 PM

Quant Time: Feb 25 05:58:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 05:55:24 2020
Response via : Initial Calibration

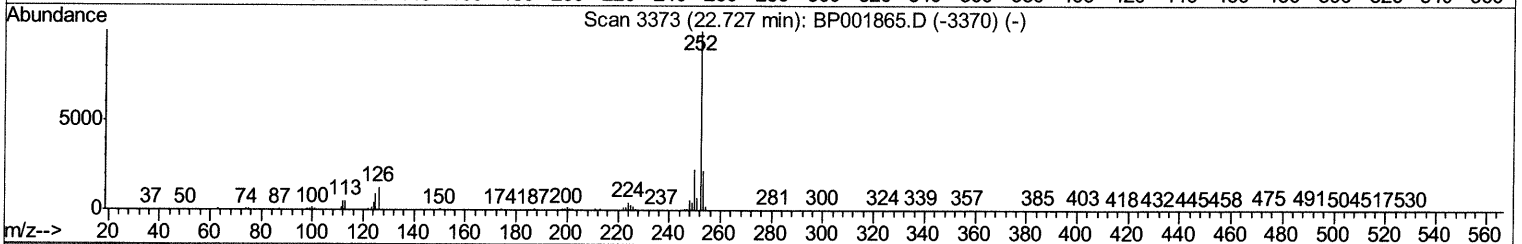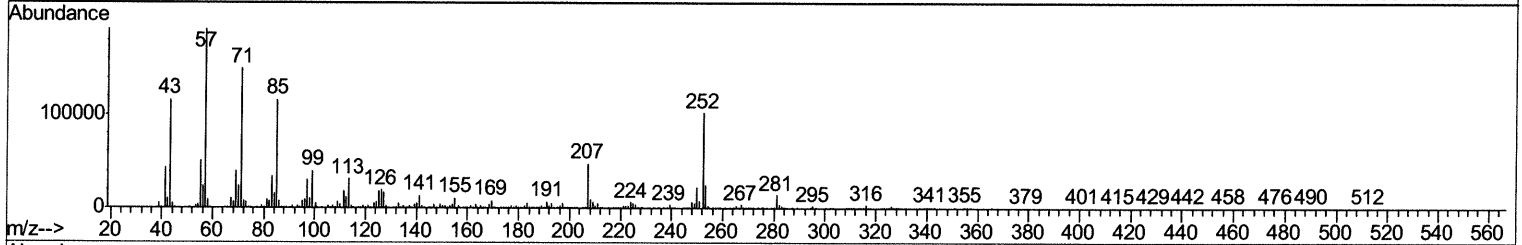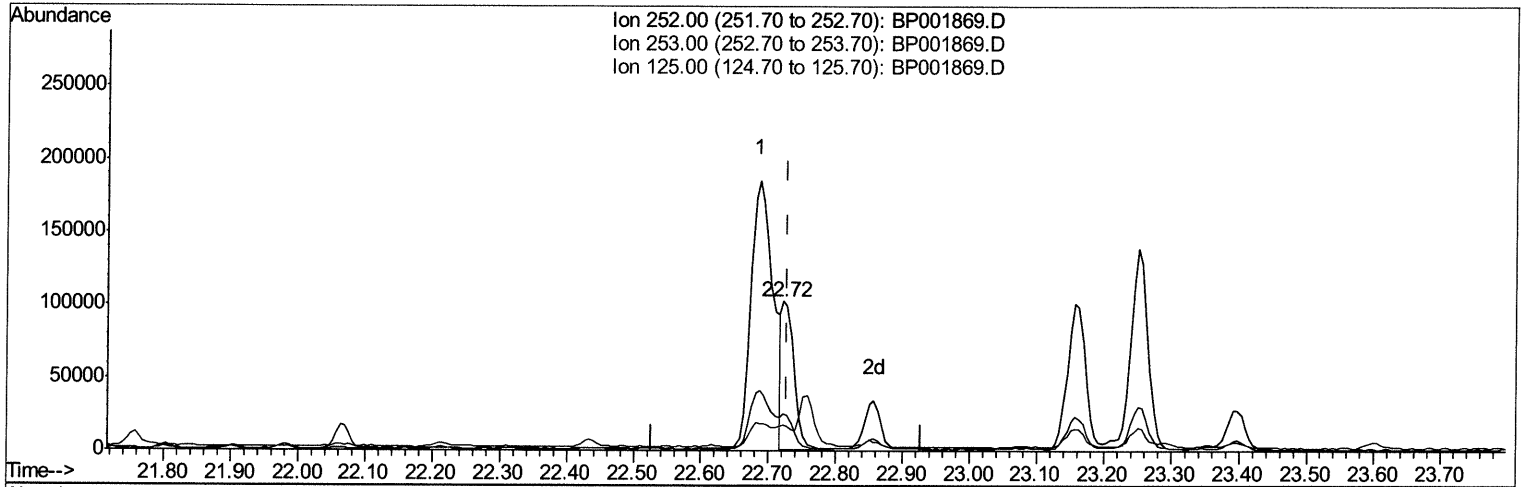

TIC: BP001869.D

(89) Benzo(k)fluoranthene

22.721min (-0.006) 1.17ng/ul m 24 02/27/20

response 127580

Ion	Exp%	Act%
252.00	100	100
253.00	22.20	24.88
125.00	10.00	17.37#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022420\
Quantitation Report (QT Reviewed)

Data File : BP001869.D
Acq On : 24 Feb 2020 20:00
Operator : CG/JU
Sample : L1536-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB6X3

Manual Integrations
APPROVED

mohammad
2/25/2020 3:42:29 PM

Quant Time: Feb 25 06:17:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 05:55:24 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	357540	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	1515888	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	963170	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	2153850	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	1910132	20.00	ng/ul	0.00
86) Perylene-d12	23.35	264	1781509	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.17	96	62587	7.27	ng/uL	0.00
5) Phenol-d5	6.83	99	939021	34.76	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	526709	33.56	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	844612	38.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	787968	36.77	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	422654	41.19	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	472918	50.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	863523	39.13	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	1068842	40.95	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	2652541	39.24	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	3198597	38.43	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	454561	38.62	ng/ul	0.00
58) Fluorene-d10	15.29	176	2312032	38.04	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	357479	42.10	ng/ul	0.00
71) Anthracene-d10	17.14	188	3477833	36.65	ng/ul	0.00
79) Pyrene-d10	19.39	212	5002343	51.03	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	3517004	40.88	ng/ul	0.00

Target Compounds

					Qvalue
45) Dimethylphthalate	13.75	163	130187	1.830 ng/ul	99
70) Phenanthrene	17.08	178	389580	3.280 ng/ul	100
77) Fluoranthene	19.06	202	899672	7.073 ng/ul	99
80) Pyrene	19.41	202	781412	6.014 ng/ul	98
83) Benzo(a)anthracene	21.12	228	348752	2.773 ng/ul	97
85) Chrysene	21.17	228	354853	2.888 ng/ul	99
88) Benzo(b)fluoranthene	22.69	252	421693	4.023 ng/ul	100
89) Benzo(k)fluoranthene	22.72	252	127580m >	1.174 ng/ul >	99
91) Benzo(a)pyrene	23.25	252	243656	2.480 ng/ul	99
92) Indeno(1,2,3-cd)pyrene	25.58	276	170223	1.387 ng/ul#	93
94) Benzo(g,h,i)perylene	26.26	276	134605	1.290 ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed