

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022420\
 Data File : BP001858.D
 Acq On : 24 Feb 2020 13:48
 Operator : CG/JU
 Sample : L1536-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB6R8

Quant Time: Feb 24 16:25:37 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 24 01:10:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	349772	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1416746	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	943361	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	2190315	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2160747	20.00	ng/ul	0.00
86) Perylene-d12	23.35	264	2364338	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	41642	4.95	ng/uL	-0.02
5) Phenol-d5	6.83	99	837950	31.71	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	471988	30.74	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	778966	36.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	709470	33.84	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	369835	38.56	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	415577	47.91	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	775278	37.59	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	984655	40.36	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	2401417	36.27	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	2933320	35.98	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	411362	35.69	ng/ul	0.00
58) Fluorene-d10	15.29	176	2185203	36.70	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	330747	38.30	ng/ul	0.00
71) Anthracene-d10	17.14	188	3411192	35.35	ng/ul	0.00
79) Pyrene-d10	19.39	212	3890362	35.09	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	4176998	36.58	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.75	163	90621	1.301	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022420\
Data File : BP001858.D
Acq On : 24 Feb 2020 13:48
Operator : CG/JU
Sample : L1536-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB6R8

Quant Time: Feb 24 16:25:37 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 01:10:13 2020
Response via : Initial Calibration

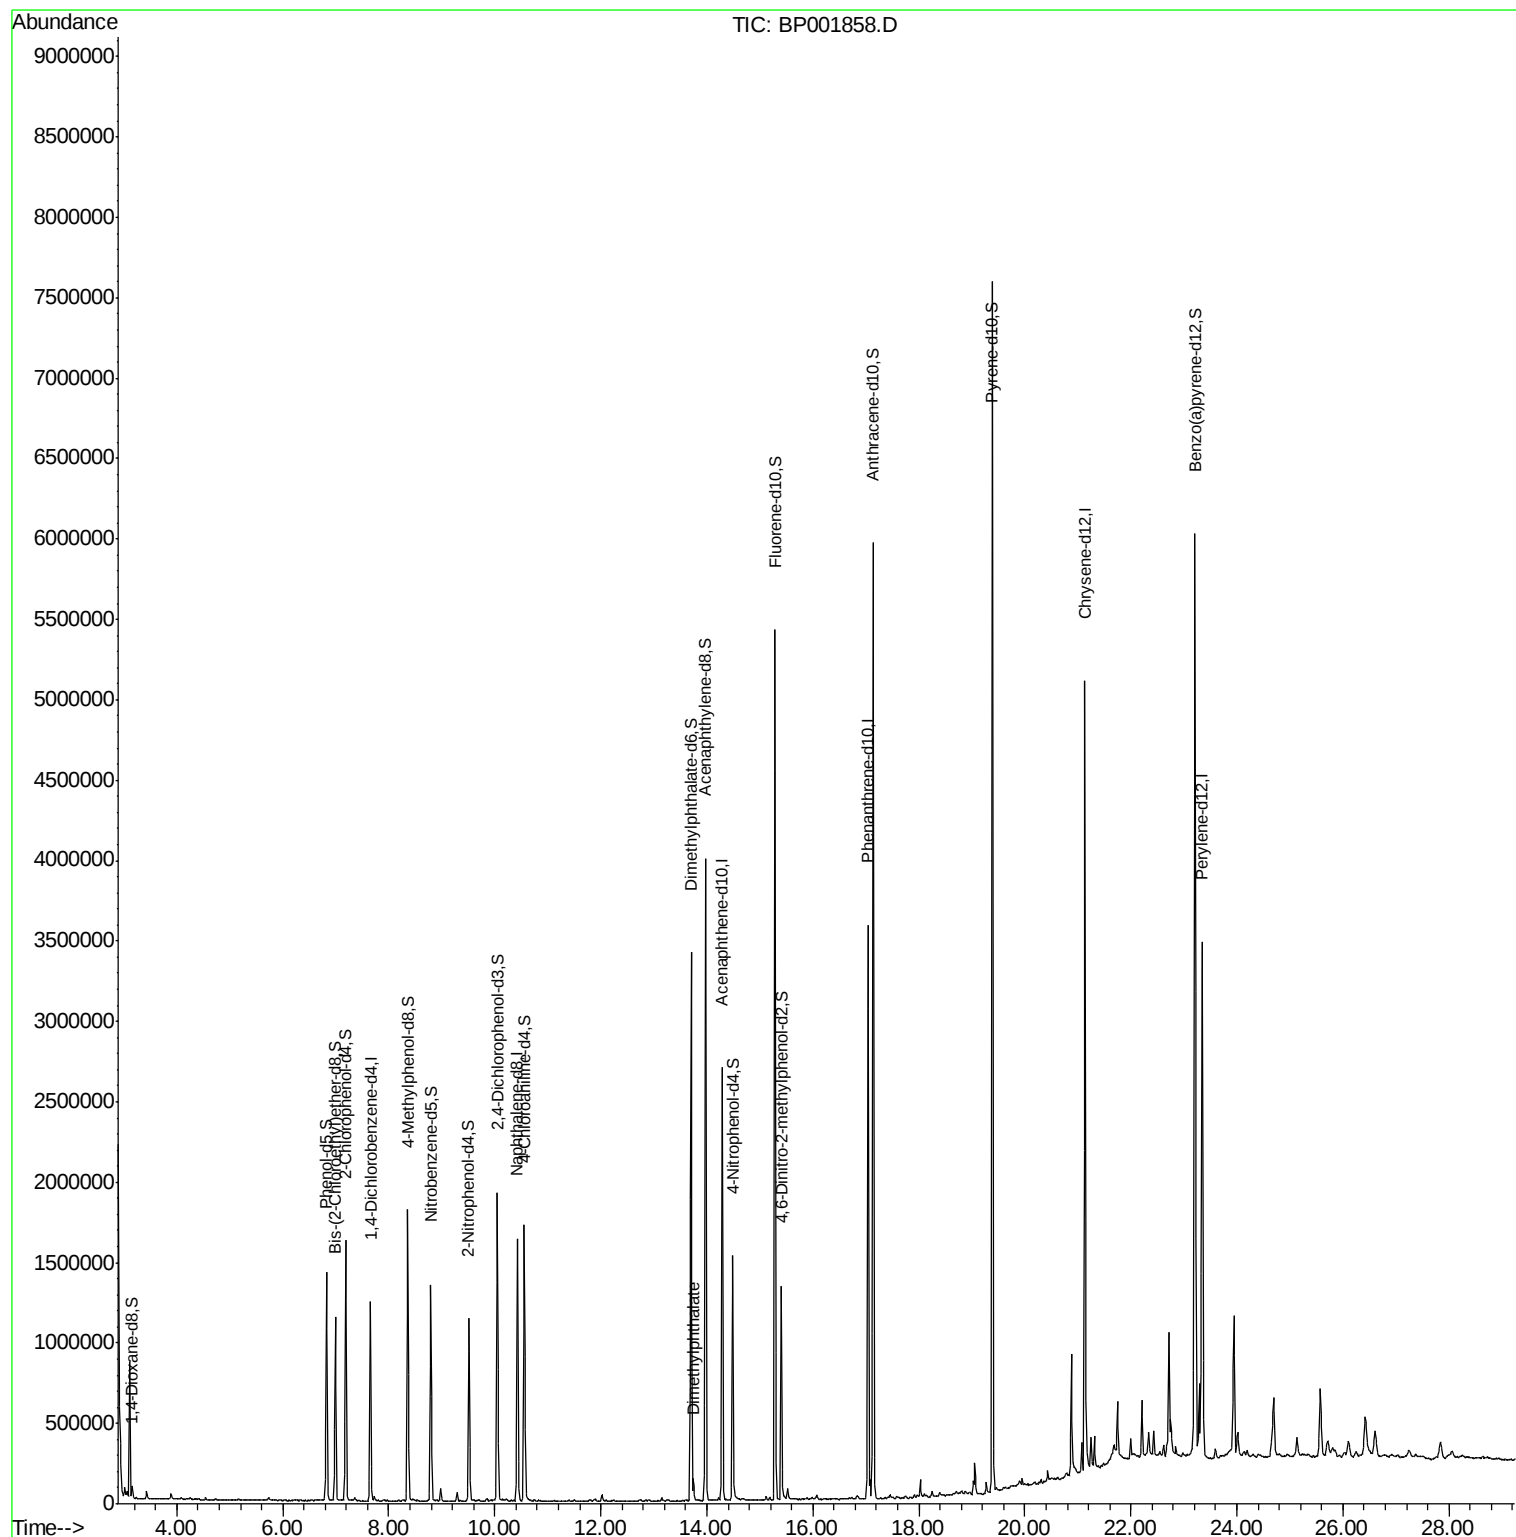

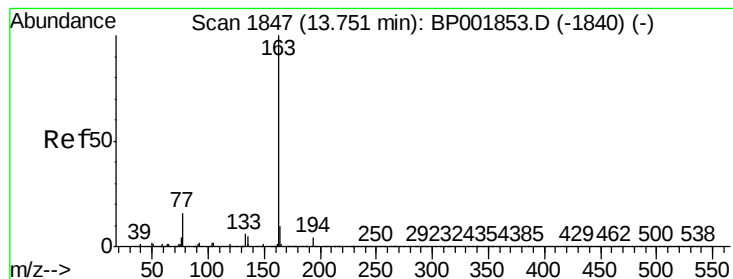

#45

Dimethylphthalate

Concen: 1.301 ng/ul

RT: 13.75 min Scan# 1846

Delta R.T. -0.01 min

Lab File: BP001858.D

Acq: 24 Feb 2020 13:48

Instrument :

BNA_P

ClientSampleId :

CB6R8


Tot Ion:163 Resp: 90621

Ion Ratio Lower Upper

163 100

194 4.4 3.5 5.3

164 10.6 8.0 12.0

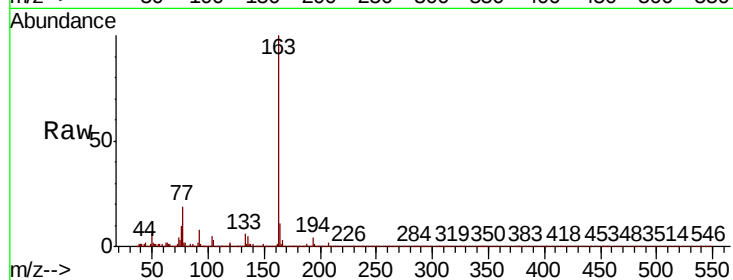

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

