

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022420\
 Data File : BP001860.D
 Acq On : 24 Feb 2020 14:55
 Operator : CG/JU
 Sample : L1536-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB6S0

Quant Time: Feb 24 17:04:41 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 24 01:10:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	414404	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	1753392	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1136791	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	2529127	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2490460	20.00	ng/ul	0.00
86) Perylene-d12	23.35	264	2656161	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.18	96	45291	4.54	ng/uL	0.00
5) Phenol-d5	6.83	99	881615	28.16	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	500254	27.50	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	776934	30.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	725700	29.22	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	393727	33.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	442738	41.24	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	804037	31.50	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	1017918	33.71	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	2605589	32.66	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	3075538	31.31	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	433981	31.24	ng/ul	0.00
58) Fluorene-d10	15.29	176	2260003	31.50	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	343993	34.50	ng/ul	0.00
71) Anthracene-d10	17.14	188	3414252	30.64	ng/ul	0.00
79) Pyrene-d10	19.39	212	4026667	31.51	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	4299000	33.51	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.75	163	170102	2.026	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022420\
Data File : BP001860.D
Acq On : 24 Feb 2020 14:55
Operator : CG/JU
Sample : L1536-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB6S0

Quant Time: Feb 24 17:04:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 01:10:13 2020
Response via : Initial Calibration

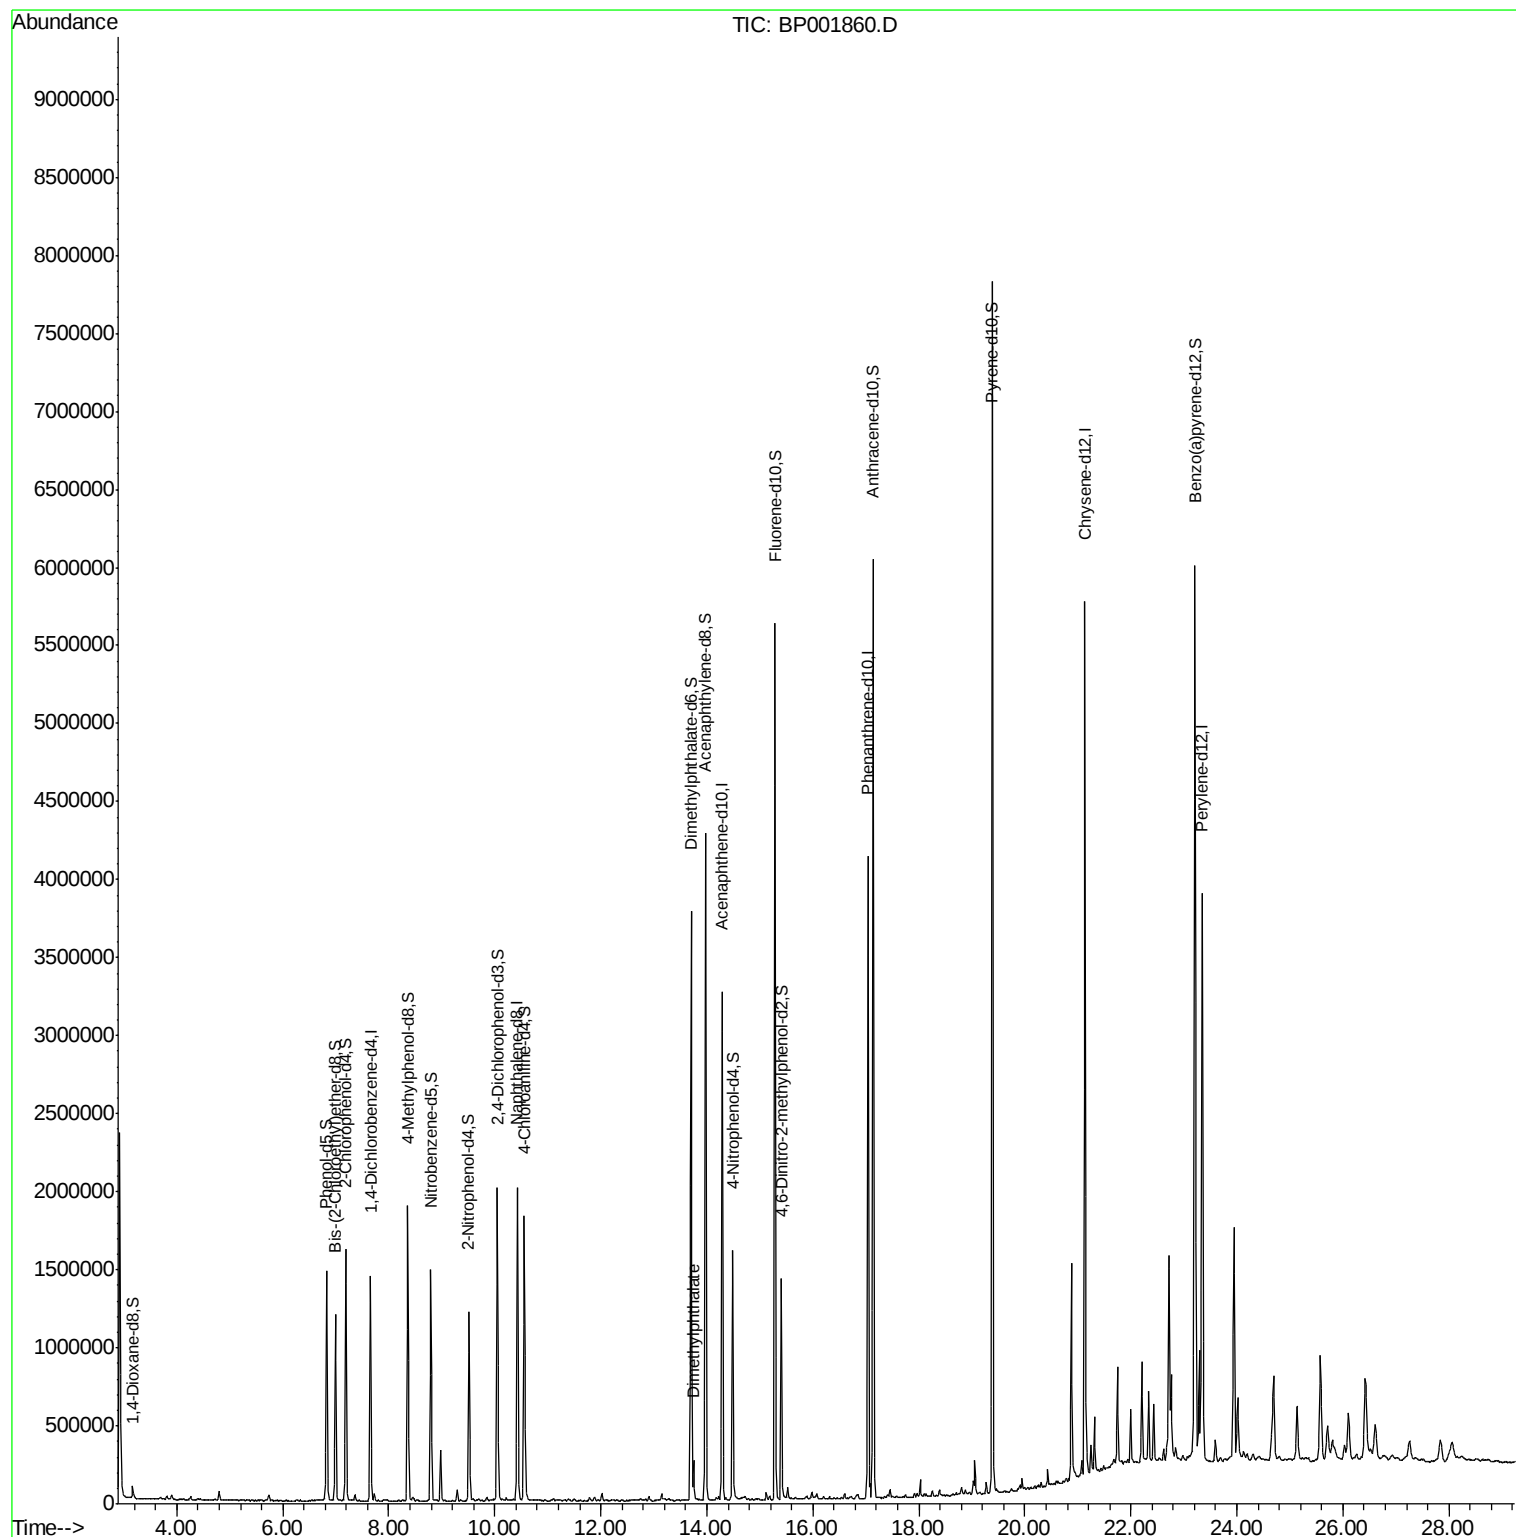

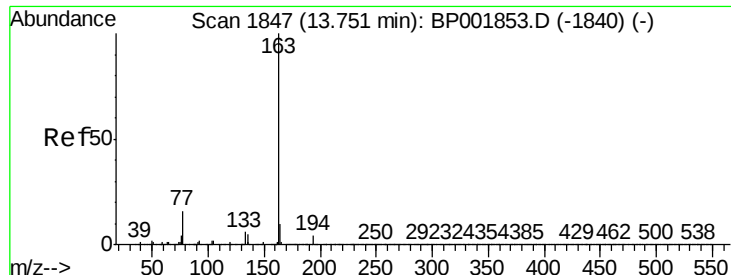

#45

Dimethylphthalate

Concen: 2.026 ng/ul

RT: 13.75 min Scan# 1847

Delta R.T. 0.00 min

Lab File: BP001860.D

Acq: 24 Feb 2020 14:55

Instrument :

BNA_P

ClientSampleId :

CB6S0


Tot Ion:163 Resp: 170102

Ion Ratio Lower Upper

163 100

194 4.2 3.5 5.3

164 10.0 8.0 12.0

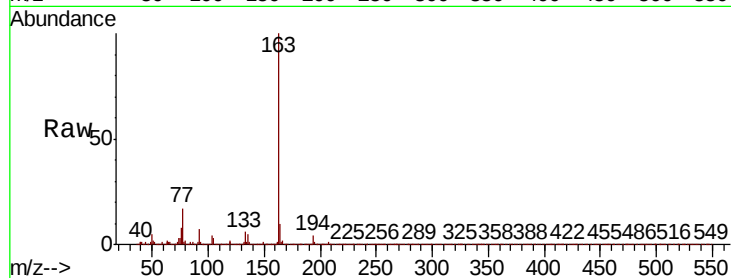

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

