

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022420\
 Data File : BP001868.D
 Acq On : 24 Feb 2020 19:26
 Operator : CG/JU
 Sample : L1536-12
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleID :
 CB6X2

Manual Integrations
 APPROVED

mohammad
 2/25/2020 3:42:27 PM

Quant Time: Feb 25 06:14:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 25 05:55:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	381054	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1602927	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1029178	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	2183964	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	1545496	20.00	ng/ul	0.00
86) Perylene-d12	23.35	264	1535488	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.17	96	52707	5.75	ng/uL	0.00
5) Phenol-d5	6.83	99	1027696	35.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	575500	34.40	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	913059	39.24	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	738656	32.34	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	605343	55.79	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	525195	53.52	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	953606	40.87	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	1005509	36.43	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	2958912	40.97	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	3561639	40.05	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	497988	39.60	ng/ul	0.00
58) Fluorene-d10	15.29	176	2604720	40.10	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	407052m	47.27	ng/ul	0.00
71) Anthracene-d10	17.14	188	3615217	37.58	ng/ul	0.00
79) Pyrene-d10	19.39	212	3971137	50.07	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	3192723	43.05	ng/ul	0.00

Target Compounds

					Ovalue	
4) Benzaldehyde	6.79	77	19788	1.123	ng/ul	95
28) Naphthalene	10.48	128	136522	1.594	ng/ul	98
34) 2-Methylnaphthalene	12.09	142	63199	1.070	ng/ul	99
45) Dimethylphthalate	13.75	163	172307	2.267	ng/ul	99
48) Acenaphthylene	14.00	152	154860	1.605	ng/ul	98
50) Acenaphthene	14.35	153	136579	2.072	ng/ul	99
54) Dibenzofuran	14.69	168	131625	1.418	ng/ul	96
59) Fluorene	15.34	166	147182	1.993	ng/ul#	95
70) Phenanthrene	17.08	178	2265128	18.807	ng/ul	100
72) Anthracene	17.17	178	503215	4.230	ng/ul	99
75) Carbazole	17.44	167	212708	2.144	ng/ul	99
77) Fluoranthene	19.06	202	3469009	26.897	ng/ul	95
80) Pyrene	19.42	202	2905138	27.635	ng/ul	96
83) Benzo(a)anthracene	21.12	228	1540179	15.133	ng/ul	97
84) Bis(2-ethylhexyl)phthalate	21.07	149	93091	1.722	ng/ul#	99
85) Chrysene	21.17	228	1391215	13.992	ng/ul	99
88) Benzo(b)fluoranthene	22.69	252	1784701	19.753	ng/ul	99
89) Benzo(k)fluoranthene	22.73	252	557138	5.949	ng/ul	98
91) Benzo(a)pyrene	23.25	252	1125263	13.289	ng/ul	99
92) Indeno(1,2,3-cd)pyrene	25.58	276	874422	8.267	ng/ul	95
93) Dibenzo(a,h)anthracene	25.59	278	237395	2.672	ng/ul#	95
94) Benzo(a,h,i)perylene	26.26	276	718676	7.993	ng/ul	96

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022420\
Data File : BP001868.D
Acq On : 24 Feb 2020 19:26
Operator : CG/JU
Sample : L1536-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB6X2

Manual Integrations
APPROVED

mohammad
2/25/2020 3:42:27 PM

Quant Time: Feb 25 06:14:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 05:55:24 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022420\
Data File : BP001868.D
Acq On : 24 Feb 2020 19:26
Operator : CG/JU
Sample : L1536-12
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampled :
CB6X2

Quant Time: Feb 25 06:14:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 05:55:24 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
2/25/2020 3:42:27 PM

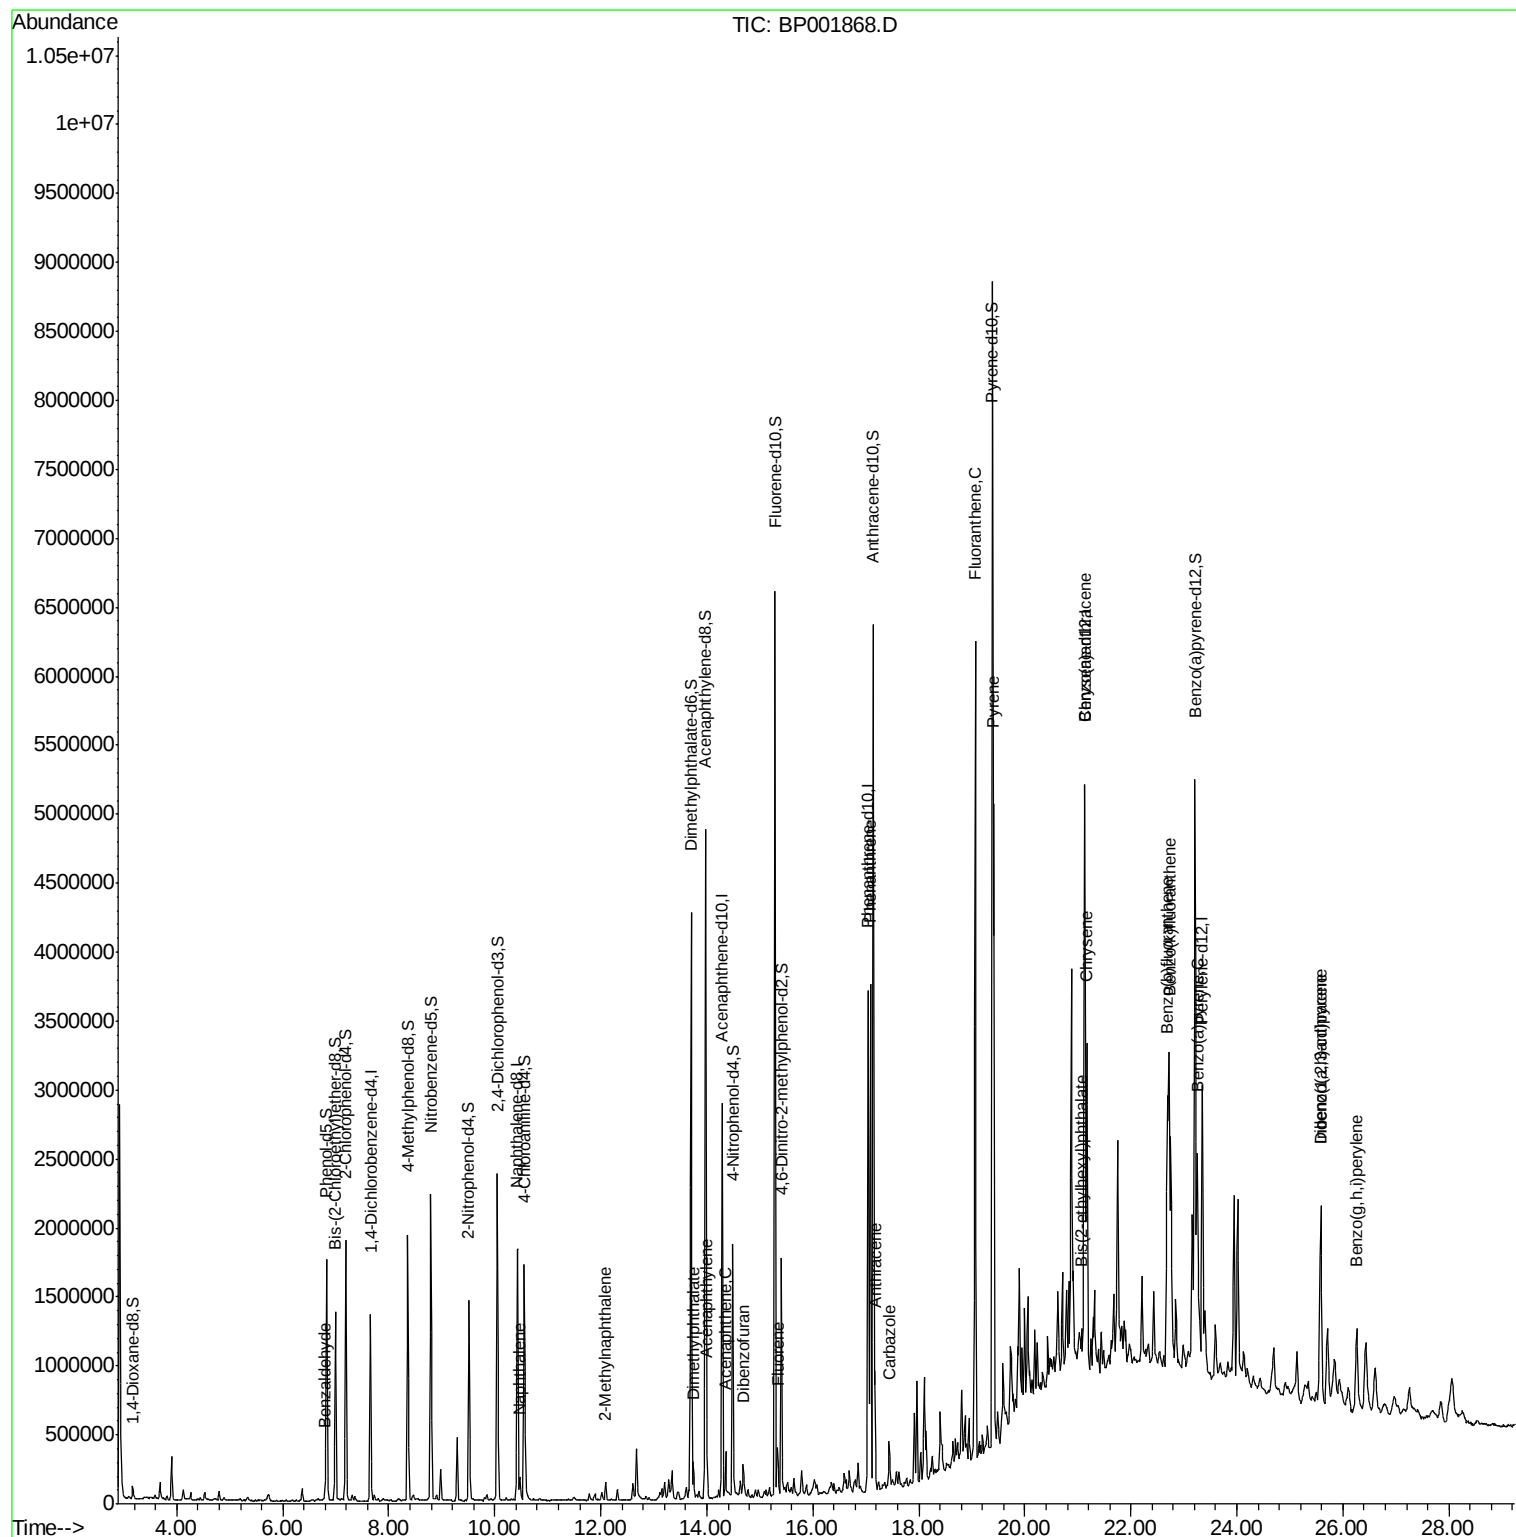



#4

Benzaldehyde

Concen: 1.123 ng/ul

RT: 6.79 min Scan# 664

Delta R.T. 0.00 min

Lab File: BP001868.D

Acq: 24 Feb 2020 19:26

Instrument :

BNA_P

ClientSampleId :

CB6X2

Tot Ion: 77 Resp: 19788

Ion Ratio Lower Upper





77 100

105 105.9 82.0 123.0

106 104.5 78.9 118.3

Manual Integrations
APPROVED

mohammad
2/25/2020 3:42:27 PM

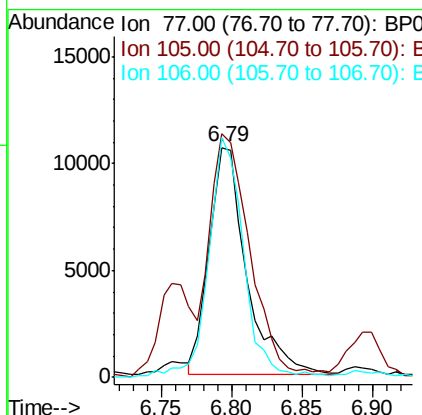

#28

Naphthalene

Concen: 1.594 ng/ul

RT: 10.48 min Scan# 1290

Delta R.T. -0.00 min

Lab File: BP001868.D

Acq: 24 Feb 2020 19:26




Tgt Ion: 128 Resp: 136522


Ion Ratio Lower Upper

128 100

129 11.2 8.7 13.1

127 13.7 10.2 15.4

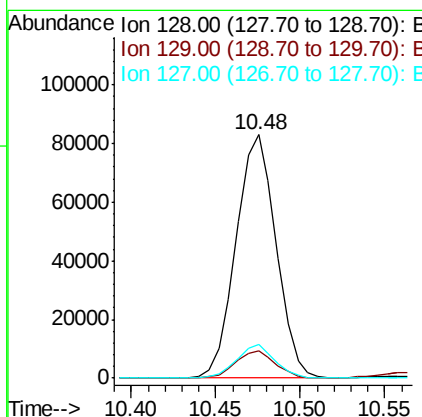







#34
 2-Methylnaphthalene
 Concen: 1.070 ng/ul
 RT: 12.09 min Scan# 1565
 Delta R.T. 0.00 min
 Lab File: BP001868.D
 Acq: 24 Feb 2020 19:26

Instrument :
 BNA_P
 ClientSampleId :
 CB6X2

Tot Ion	Ratio	Lower	Upper
142	100		
141	88.6	70.2	105.4




Manual Integrations
 APPROVED


mohammad
 2/25/2020 3:42:27 PM

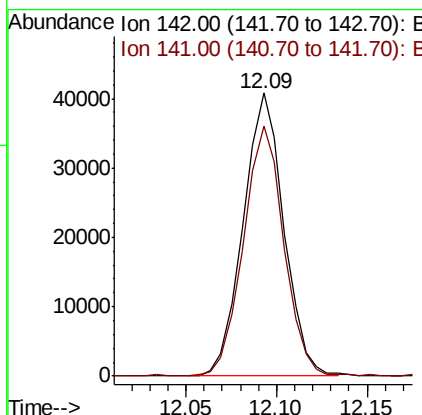

#45
 Dimethylphthalate
 Concen: 2.267 ng/ul
 RT: 13.75 min Scan# 1847
 Delta R.T. 0.00 min
 Lab File: BP001868.D
 Acq: 24 Feb 2020 19:26

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.5	3.5	5.3
164	10.3	8.0	12.0

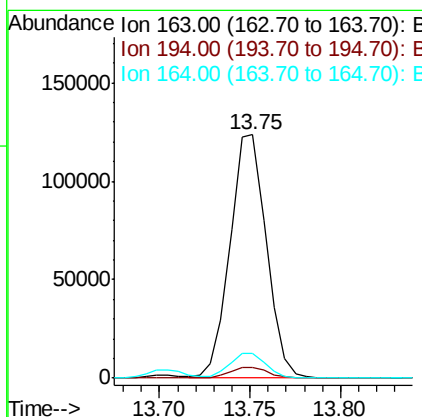

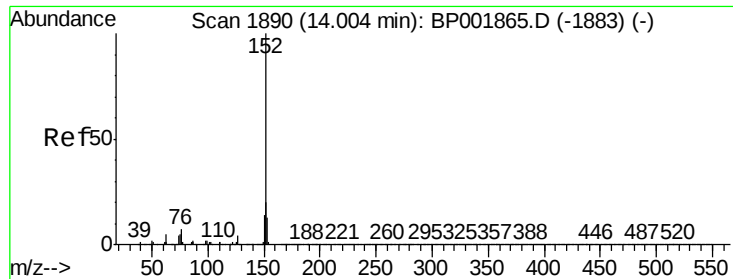

#48

Acenaphthylene

Concen: 1.605 ng/ul

RT: 14.00 min Scan# 1890

Delta R.T. 0.00 min

Lab File: BP001868.D

Acq: 24 Feb 2020 19:26

Instrument :

BNA_P





ClientSampled :

CB6X2

Tot Ion:	152	Resp:	154860
Ion Ratio	Lower	Upper	
152	100		
151	20.6	15.7	23.5
153	13.9	10.7	16.1

Manual Integrations
APPROVED

mohammad
2/25/2020 3:42:27 PM

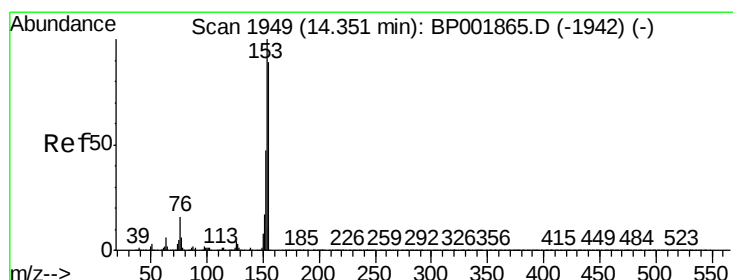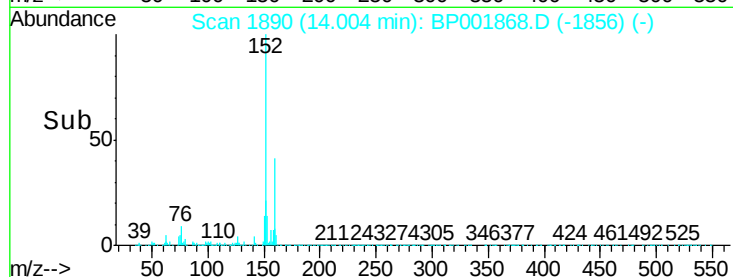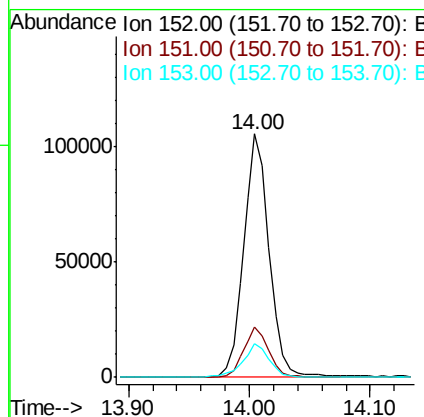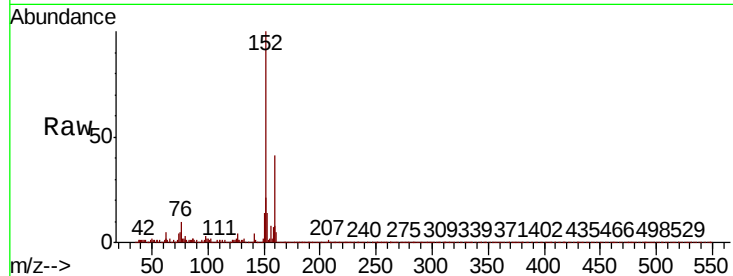

#50

Acenaphthene

Concen: 2.072 ng/ul




RT: 14.35 min Scan# 1949


Delta R.T. 0.00 min

Lab File: BP001868.D

Acq: 24 Feb 2020 19:26

Tgt Ion:	153	Resp:	136579
Ion Ratio	Lower	Upper	
153	100		
152	49.0	37.8	56.8
154	90.4	71.9	107.9

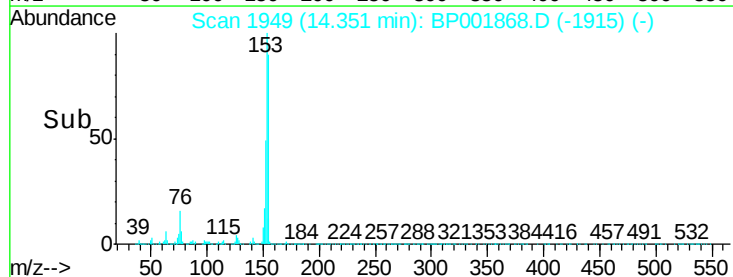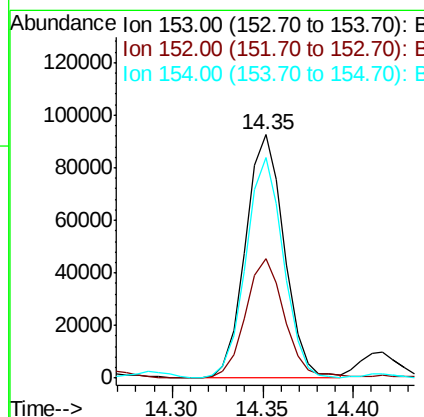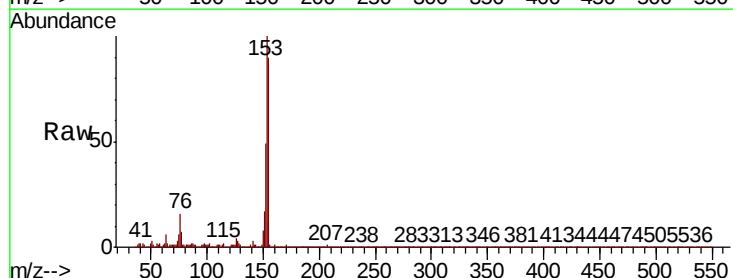







#54
Dibenzenofuran
Concen: 1.418 ng/ul
RT: 14.69 min Scan# 2006
Delta R.T. -0.01 min
Lab File: BP001868.D
Acq: 24 Feb 2020 19:26

Instrument :
BNA_P
ClientSampleId :
CB6X2

Tot Ion	Ratio	Lower	Upper
168	100		
139	38.0	28.6	43.0




Manual Integrations
APPROVED


mohammad
2/25/2020 3:42:27 PM

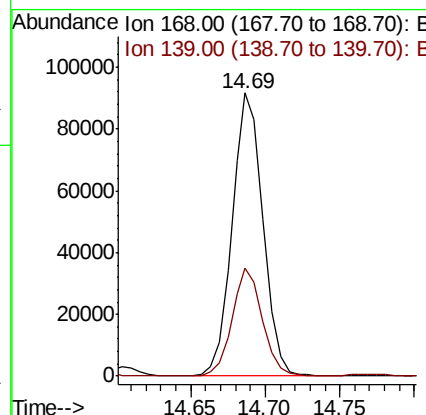

#59
Fluorene
Concen: 1.993 ng/ul
RT: 15.34 min Scan# 2117
Delta R.T. 0.00 min
Lab File: BP001868.D
Acq: 24 Feb 2020 19:26

Tgt Ion	Ratio	Lower	Upper
166	100		
165	101.2	77.3	115.9
167	16.8	11.0	16.6#

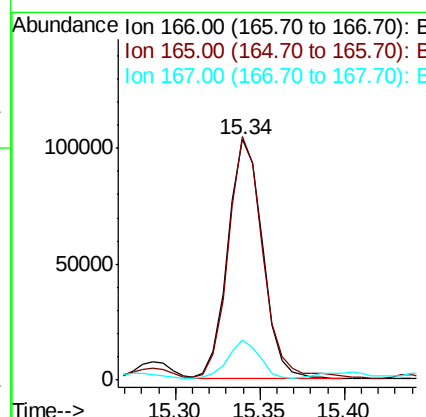







#70
Phenanthrene
Concen: 18.807 ng/ul
RT: 17.08 min Scan# 2413
Delta R.T. -0.00 min
Lab File: BP001868.D
Acq: 24 Feb 2020 19:26

Instrument :
BNA_P
ClientSampleId :
CB6X2

Tot Ion	Ratio	Lower	Upper
178	100		
179	15.6	12.3	18.5
176	19.2	15.3	22.9




Manual Integrations
APPROVED


mohammad
2/25/2020 3:42:27 PM

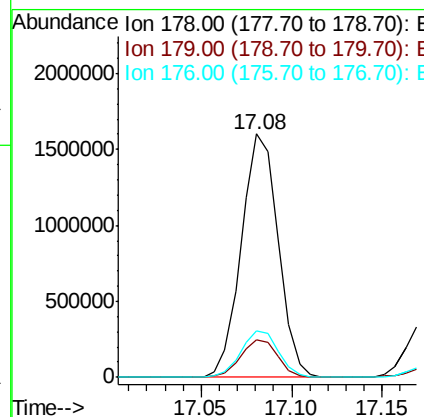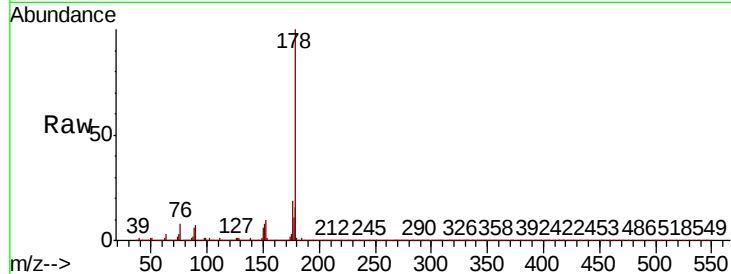

#72
Anthracene
Concen: 4.230 ng/ul
RT: 17.17 min Scan# 2429
Delta R.T. 0.00 min
Lab File: BP001868.D
Acq: 24 Feb 2020 19:26

Tgt Ion	Ratio	Lower	Upper
178	100		
179	14.7	12.4	18.6
176	18.2	14.8	22.2

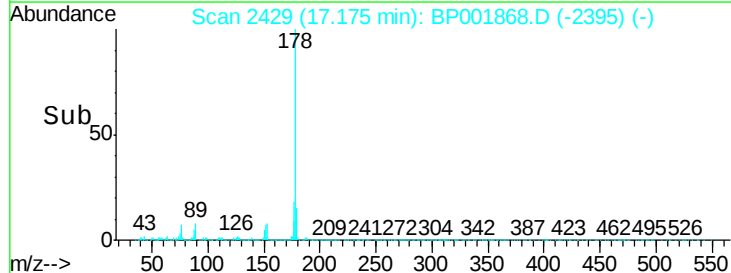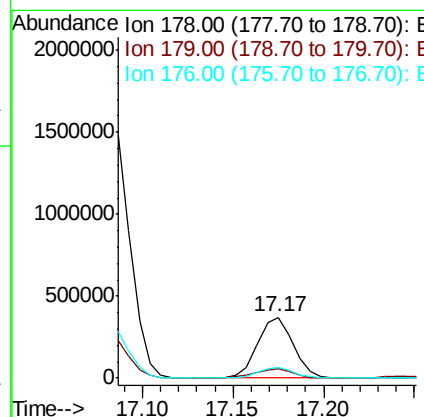



#75

Carbazole

Concen: 2.144 ng/ul

RT: 17.44 min Scan# 2474

Delta R.T. -0.01 min

Lab File: BP001868.D

Acq: 24 Feb 2020 19:26

Instrument :

BNA_P





ClientSampleId :

CB6X2

Tot Ion:	167	Resp:	212708
Ion Ratio	Lower	Upper	
167	100		
166	21.2	17.1	25.7
139	12.0	10.2	15.2

Manual Integrations
APPROVED

mohammad
2/25/2020 3:42:27 PM

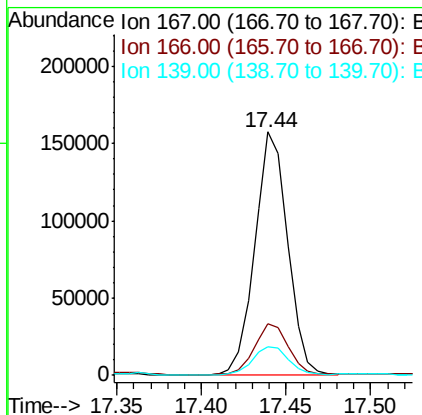

#77

Fluoranthene

Concen: 26.897 ng/ul




RT: 19.06 min Scan# 2750


Delta R.T. 0.00 min

Lab File: BP001868.D

Acq: 24 Feb 2020 19:26

Tgt Ion:	202	Resp:	3469009
Ion Ratio	Lower	Upper	
202	100		
101	9.3	9.1	13.7
100	7.1	6.6	9.8

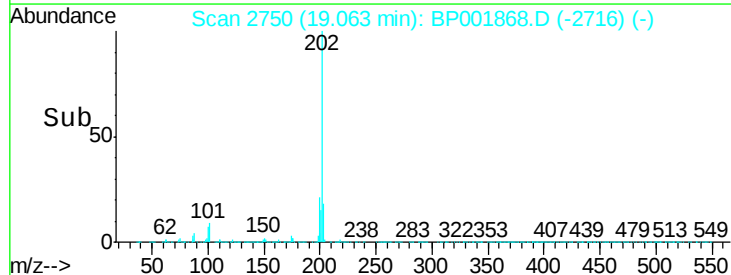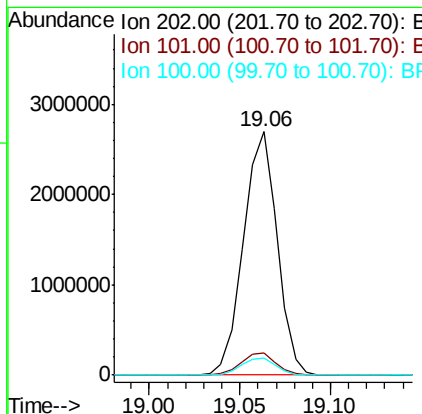







#80
Pvrene
Concen: 27.635 ng/ul
RT: 19.42 min Scan# 2810
Delta R.T. 0.01 min
Lab File: BP001868.D
Acq: 24 Feb 2020 19:26

Instrument :
BNA_P
ClientSampled :
CB6X2

Tot Ion	Ratio	Lower	Upper
202	100		
101	10.8	10.2	15.2
100	8.9	8.2	12.2




Manual Integrations
APPROVED


mohammad
2/25/2020 3:42:27 PM

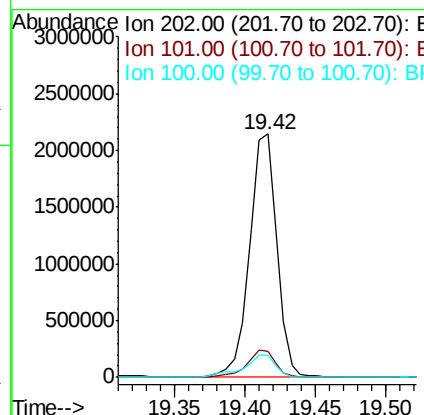

#83
Benzo(a)anthracene
Concen: 15.133 ng/ul
RT: 21.12 min Scan# 3100
Delta R.T. 0.00 min
Lab File: BP001868.D
Acq: 24 Feb 2020 19:26

Tgt Ion	Ratio	Lower	Upper
228	100		
229	20.3	16.2	24.4
226	29.8	22.0	33.0

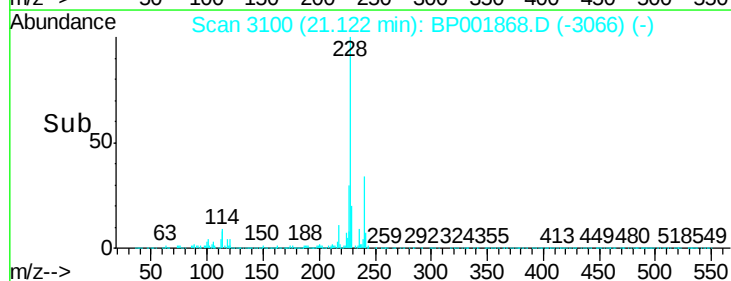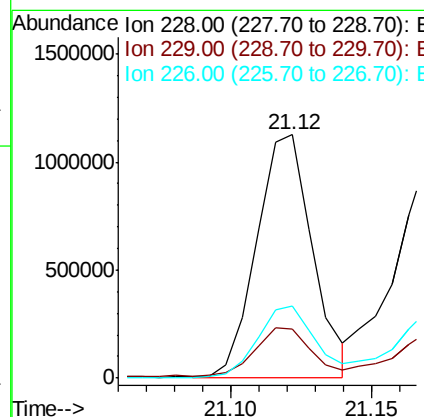







#84
 Bis(2-ethylhexyl)phthalate
 Concen: 1.722 ng/ul
 RT: 21.07 min Scan# 3092
 Delta R.T. 0.00 min
 Lab File: BP001868.D
 Acq: 24 Feb 2020 19:26

Instrument :
 BNA_P
 ClientSampleID :
 CB6X2

Tot Ion	Ratio	Lower	Upper
149	100		
167	28.6	22.6	34.0
279	5.9	3.6	5.4




Manual Integrations
 APPROVED


mohammad
 2/25/2020 3:42:27 PM

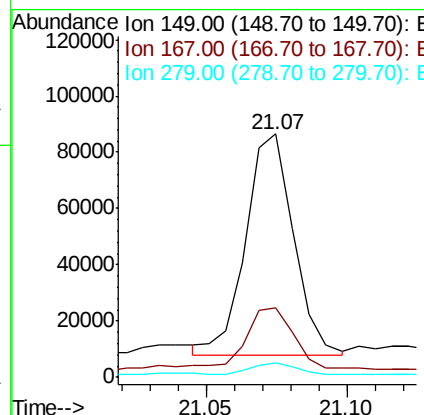

#85
 Chrysene
 Concen: 13.992 ng/ul
 RT: 21.17 min Scan# 3108
 Delta R.T. 0.00 min
 Lab File: BP001868.D
 Acq: 24 Feb 2020 19:26

Tgt Ion	Ratio	Lower	Upper
228	100		
226	29.9	24.2	36.2
229	20.5	15.7	23.5

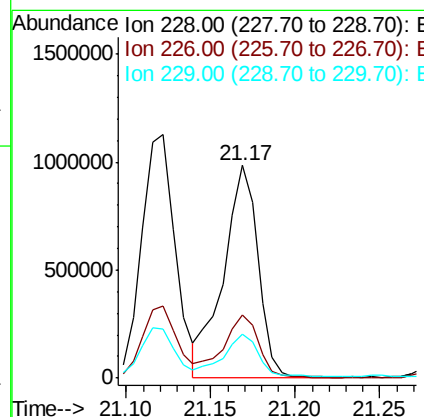



#88

Benzo(b)fluoranthene

Concen: 19.753 ng/ul

RT: 22.69 min Scan# 3366

Delta R.T. 0.00 min

Lab File: BP001868.D

Acq: 24 Feb 2020 19:26

Instrument :

BNA_P

ClientSampleId :

CB6X2

Tot Ion:252 Resp: 1784701

Ion Ratio Lower Upper


252 100

253 22.6 17.7 26.5




125 9.9 7.8 11.6

Manual Integrations
APPROVED

mohammad
2/25/2020 3:42:27 PM



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

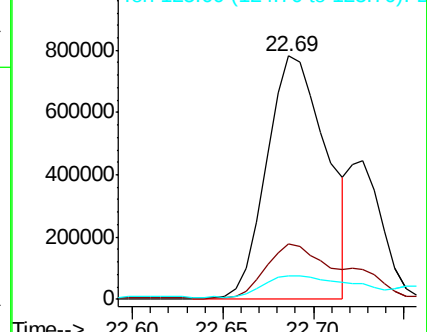

#89

Benzo(k)fluoranthene

Concen: 5.949 ng/ul

RT: 22.73 min Scan# 3373

Delta R.T. 0.00 min

Lab File: BP001868.D

Acq: 24 Feb 2020 19:26


Tgt Ion:252 Resp: 557138

Ion Ratio Lower Upper



252 100


253 21.5 17.8 26.6

125 11.0 8.0 12.0



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

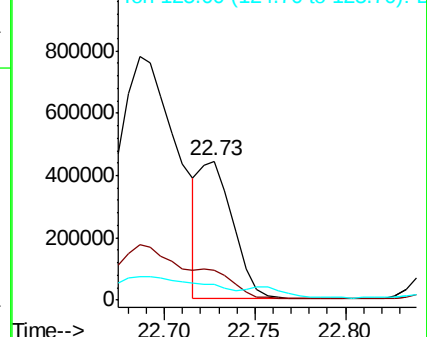







#91
Benzo(a)pyrene
Concen: 13.289 ng/ul
RT: 23.25 min Scan# 3462
Delta R.T. 0.00 min
Lab File: BP001868.D
Acq: 24 Feb 2020 19:26

Instrument :
BNA_P
ClientSampleId :
CB6X2

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.6	17.6	26.4
125	10.9	8.3	12.5




Manual Integrations
APPROVED


mohammad
2/25/2020 3:42:27 PM

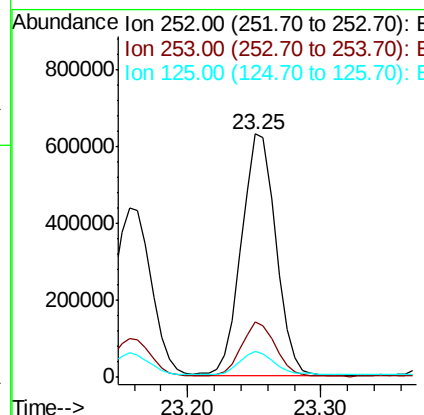

#92
Indeno(1,2,3-cd)pyrene
Concen: 8.267 ng/ul
RT: 25.58 min Scan# 3858
Delta R.T. 0.00 min
Lab File: BP001868.D
Acq: 24 Feb 2020 19:26

Tgt Ion	Ratio	Lower	Upper
276	100		
138	19.5	19.3	28.9
277	25.3	20.0	30.0

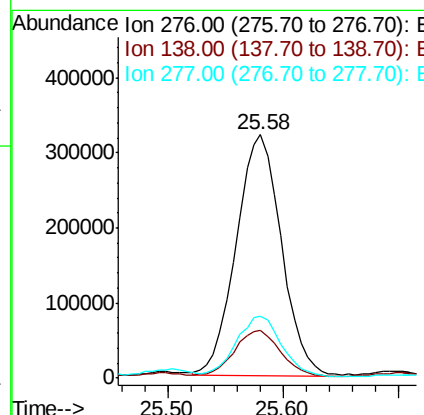







#93
Dibenzo(a,h)anthracene
Concen: 2.672 ng/ul
RT: 25.59 min Scan# 3859
Delta R.T. -0.01 min
Lab File: BP001868.D
Acq: 24 Feb 2020 19:26

Instrument :
BNA_P
ClientSampleId :
CB6X2

Tot Ion	Ratio	Lower	Upper
278	100		
139	20.4	13.3	19.9#
279	25.4	19.3	28.9

Manual Integrations
APPROVED

mohammad
2/25/2020 3:42:27 PM

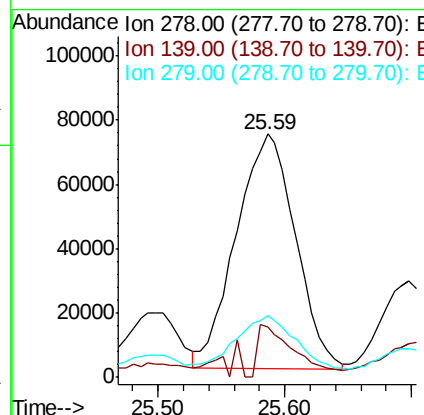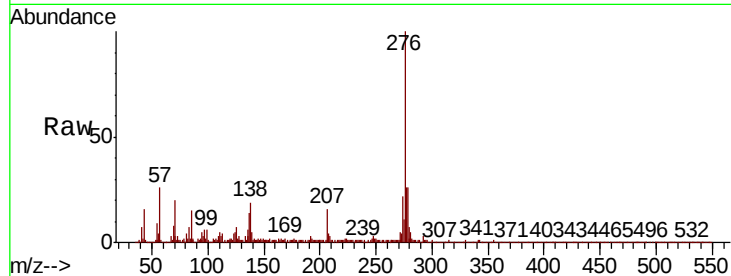

#94
Benzo(g,h,i)perylene
Concen: 7.993 ng/ul
RT: 26.26 min Scan# 3974
Delta R.T. 0.00 min
Lab File: BP001868.D
Acq: 24 Feb 2020 19:26

Tgt Ion	Ratio	Lower	Upper
276	100		
138	19.9	17.7	26.5
277	24.7	18.8	28.2

