

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022420\
 Data File : BP001871.D
 Acq On : 24 Feb 2020 21:08
 Operator : CG/JU
 Sample : L1536-15
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB6Y3

Quant Time: Feb 25 05:58:48 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 25 05:55:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	511169	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1672158	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1060509	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	2334626	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2080628	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	2508761	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.18	96	92329	7.50	ng/uL	0.00
5) Phenol-d5	6.83	99	1630708	42.22	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	903797	40.28	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	1505196	48.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	1037247	33.86	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	552427	48.80	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	631925	61.73	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	1123197	46.14	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	1517604	52.71	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	3329154	44.73	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	4022291	43.89	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	591227	45.62	ng/ul	0.00
58) Fluorene-d10	15.29	176	3851927	57.55	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	592987	64.42	ng/ul	0.00
71) Anthracene-d10	17.14	188	4314922	41.95	ng/ul	0.00
79) Pyrene-d10	19.39	212	4762825	44.61	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	5628509	46.45	ng/ul	0.00


Target Compounds				Ovalue
45) Dimethylphthalate	13.75	163	389751	4.976 ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022420\
Data File : BP001871.D
Acq On : 24 Feb 2020 21:08
Operator : CG/JU
Sample : L1536-15
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB6Y3

Quant Time: Feb 25 05:58:48 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 05:55:24 2020
Response via : Initial Calibration

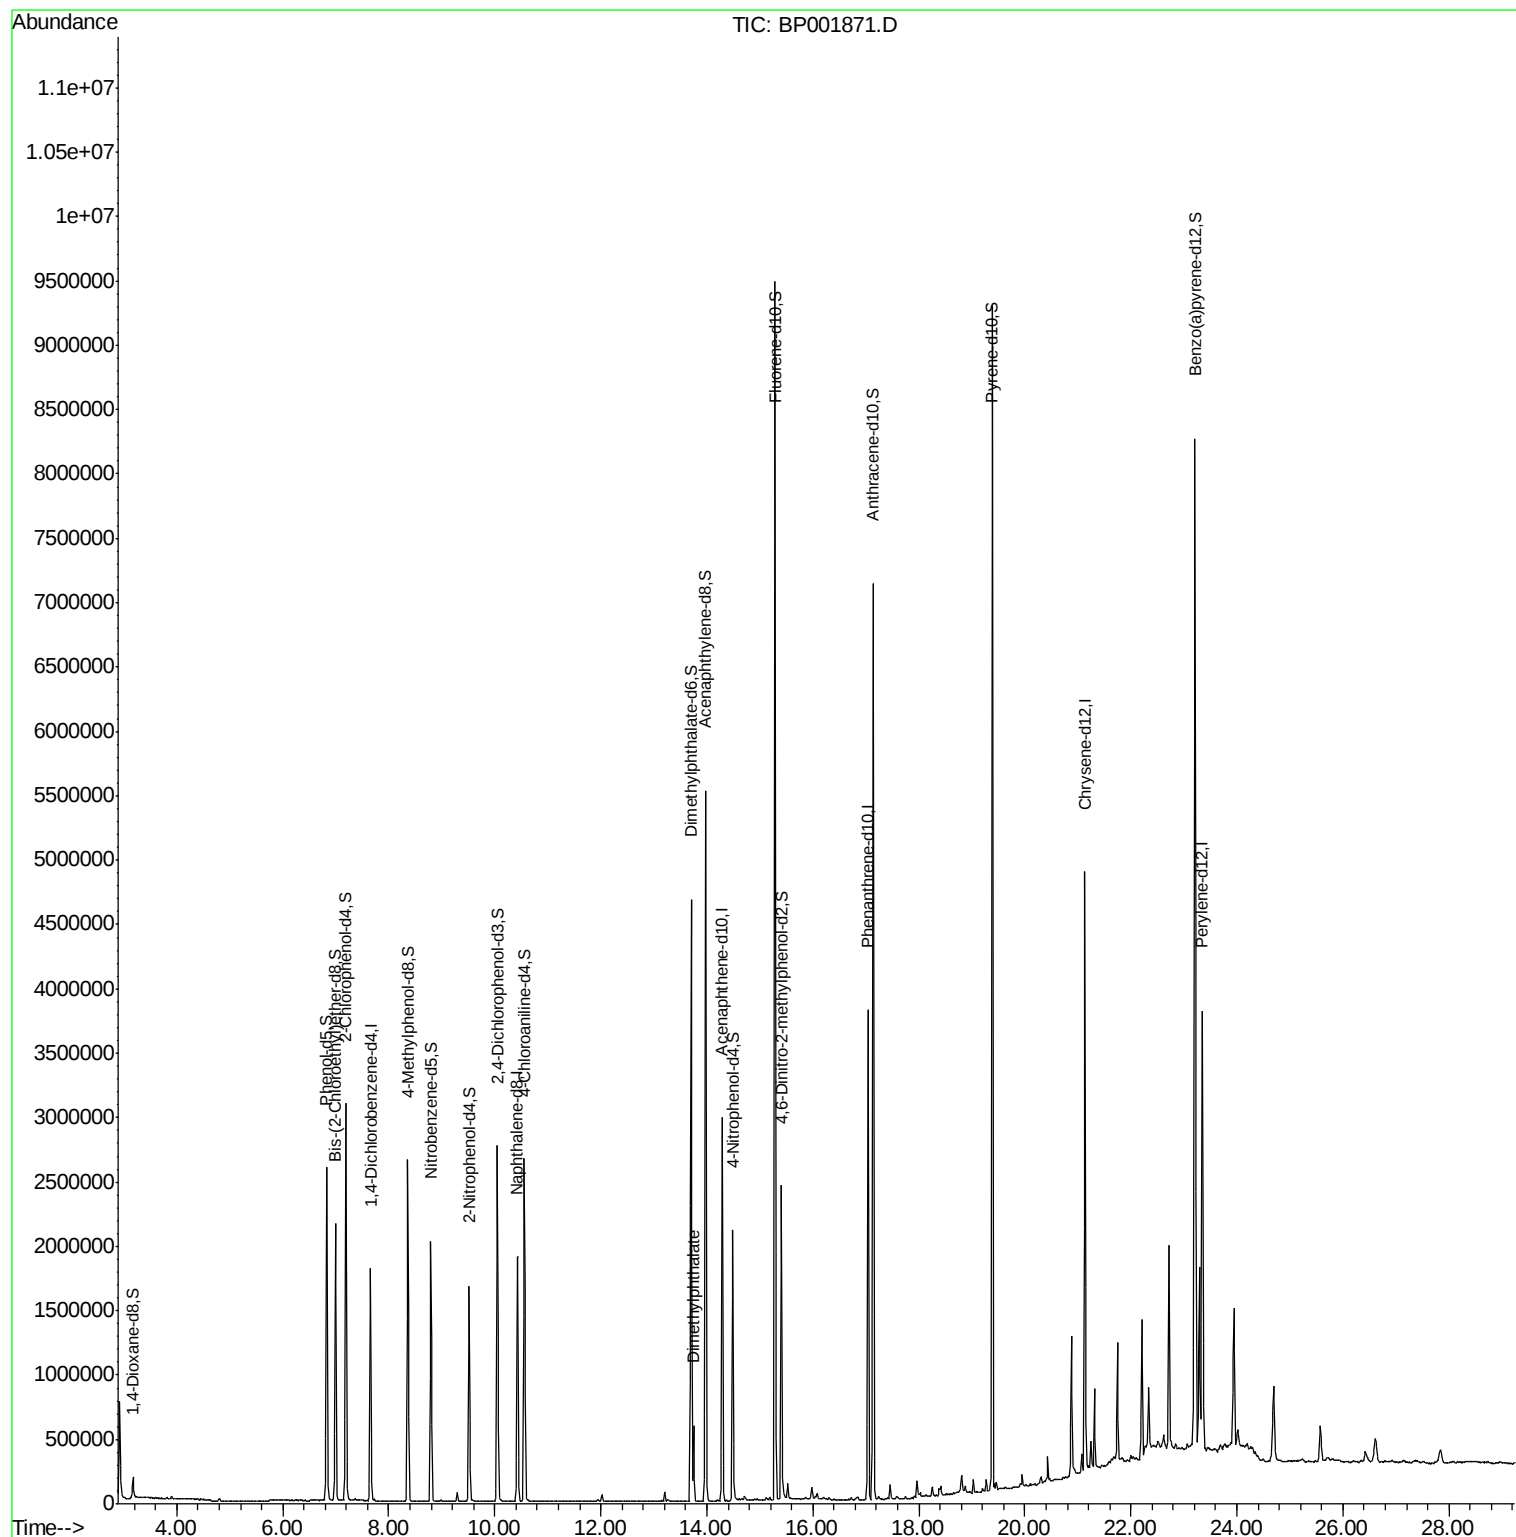

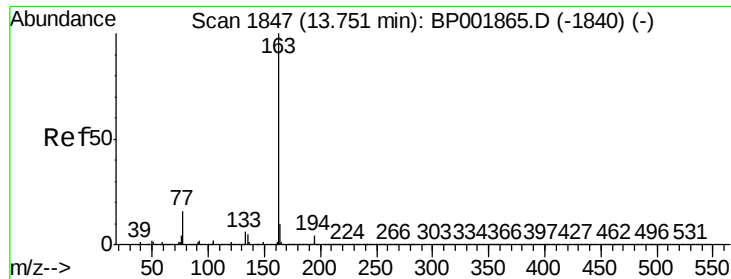

#45

Dimethylphthalate

Concen: 4.976 ng/ul

RT: 13.75 min Scan# 1847

Delta R.T. -0.00 min

Lab File: BP001871.D

Acq: 24 Feb 2020 21:08

Instrument :

BNA_P

ClientSampleId :

CB6Y3


Tot Ion:163 Resp: 389751

Ion Ratio Lower Upper

163 100

194 4.3 3.5 5.3

164 10.0 8.0 12.0

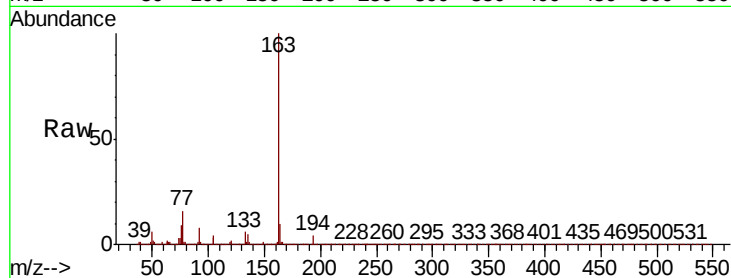

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

