

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022420\
 Data File : BP001890.D
 Acq On : 25 Feb 2020 08:24
 Operator : CG/JU
 Sample : L1542-15
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBD51

Quant Time: Feb 25 12:11:14 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 25 07:02:36 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	469086	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	1996254	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1318395	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	3019193	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	3080332	20.00	ng/ul	0.00
86) Perylene-d12	23.35	264	2896686	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.18	96	45499	4.03	ng/uL	0.00
5) Phenol-d5	6.83	99	916829	25.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	526209	25.55	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	809537	28.26	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	766196	27.25	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	400591	29.64	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	445292	36.44	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	836162	28.77	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	1148820	33.42	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	2582950	27.92	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	3169722	27.82	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	417154	25.89	ng/ul	0.00
58) Fluorene-d10	15.29	176	2346085	28.20	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	269286	22.62	ng/ul	0.00
71) Anthracene-d10	17.14	188	3621033	27.22	ng/ul	0.00
79) Pyrene-d10	19.38	212	4165394	26.35	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.20	264	3911840	27.96	ng/ul	0.00


Target Compounds				Ovalue		
6) Phenol	6.85	94	37584	1.001	ng/ul#	84
45) Dimethylphthalate	13.75	163	307368	3.156	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022420\
Data File : BP001890.D
Acq On : 25 Feb 2020 08:24
Operator : CG/JU
Sample : L1542-15
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBD51

Quant Time: Feb 25 12:11:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 07:02:36 2020
Response via : Initial Calibration

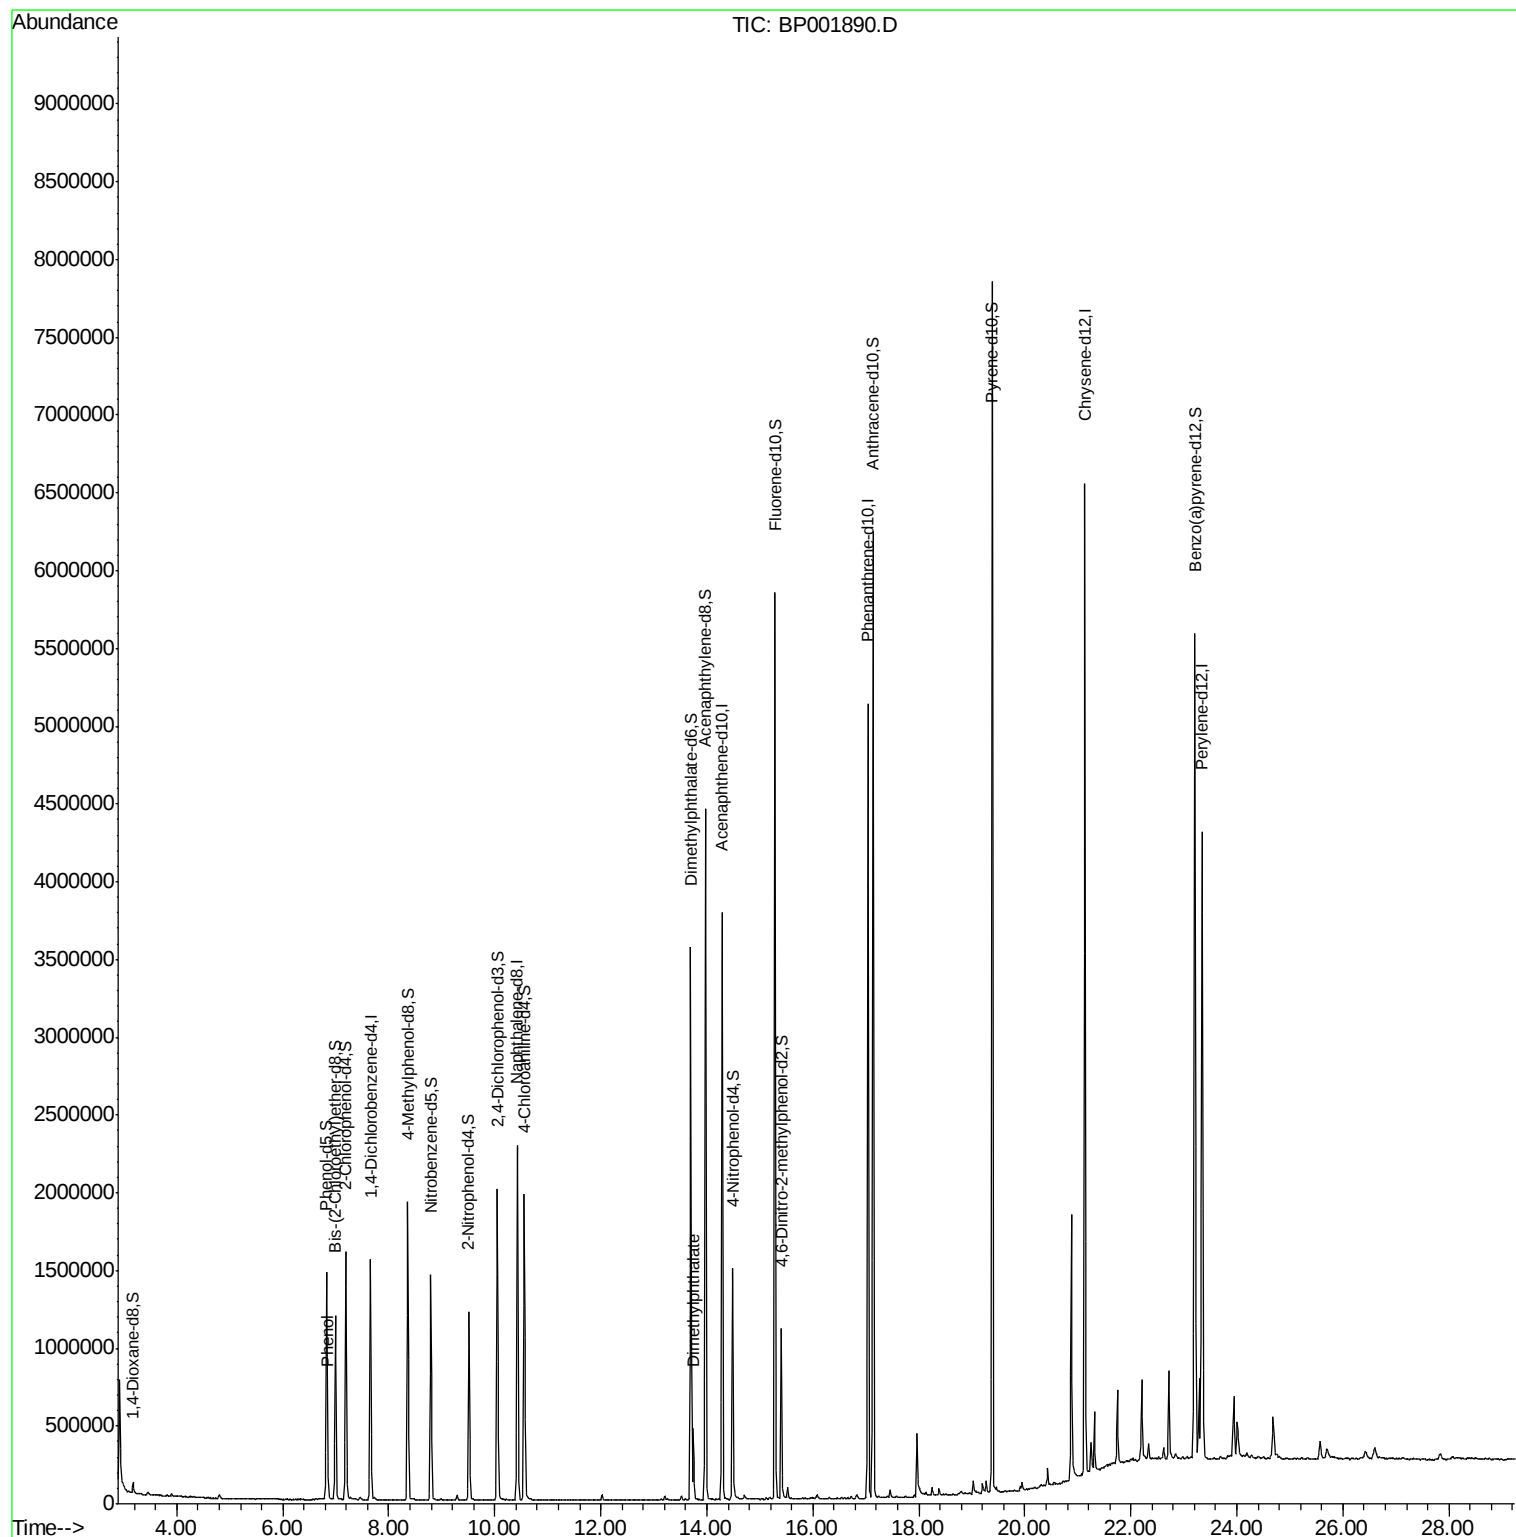

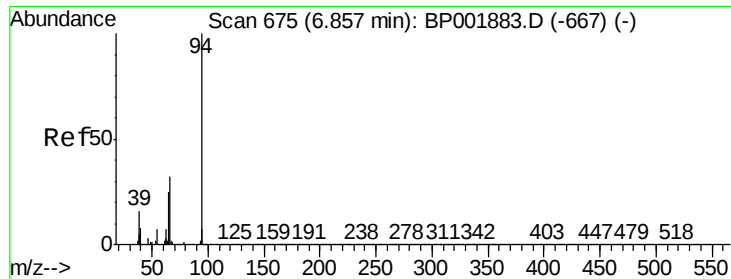

#6

Phenol

Concen: 1.001 ng/ul

RT: 6.85 min Scan# 674

Delta R.T. -0.01 min

Lab File: BP001890.D

Acq: 25 Feb 2020 08:24

Instrument :

BNA_P

ClientSampleId :

DBD51


Tot Ion: 94 Resp: 37584

Ion Ratio Lower Upper




94 100

65 28.0 19.8 29.6

66 46.3 26.6 39.8#

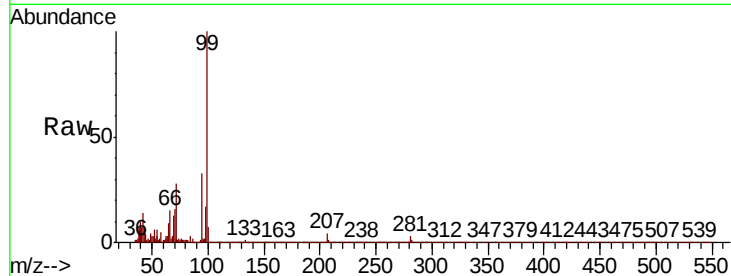

Abundance Ion 94.00 (93.70 to 94.70): BP0
Ion 65.00 (64.70 to 65.70): BP0
Ion 66.00 (65.70 to 66.70): BP0

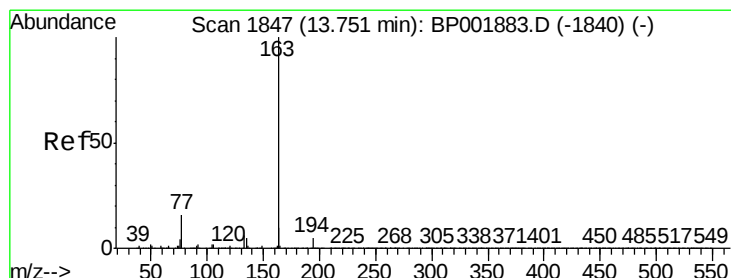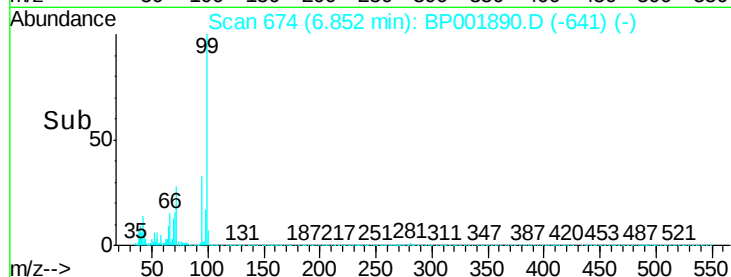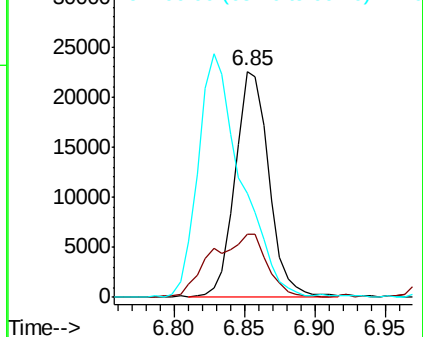

#45

Dimethylphthalate

Concen: 3.156 ng/ul

RT: 13.75 min Scan# 1846

Delta R.T. -0.01 min

Lab File: BP001890.D

Acq: 25 Feb 2020 08:24


Tgt Ion:163 Resp: 307368

Ion Ratio Lower Upper

163 100

194 4.2 3.5 5.3

164 10.1 8.0 12.0

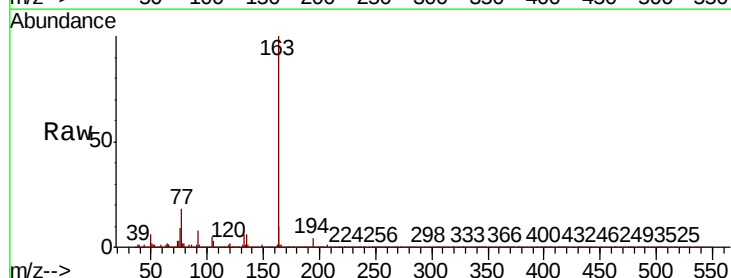

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

