

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022420\
 Data File : BP001894.D
 Acq On : 25 Feb 2020 11:13
 Operator : CG/JU
 Sample : L1542-20
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBD54

Quant Time: Feb 25 12:29:39 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 25 07:02:36 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	367251	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	1564054	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1030650	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	2400161	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2650300	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	2666628	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.17	96	50493	5.71	ng/uL	0.00
5) Phenol-d5	6.83	99	946297	34.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	537838	33.36	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	838971	37.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	787642	35.78	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	405860	38.33	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	450375	47.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	863315	37.92	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	1093535	40.60	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	2504673	34.63	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	3205601	35.99	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	376369	29.88	ng/ul	0.00
58) Fluorene-d10	15.29	176	2318285	35.64	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	242641	25.64	ng/ul	0.00
71) Anthracene-d10	17.14	188	3593706	33.99	ng/ul	0.00
79) Pyrene-d10	19.38	212	4254660	31.28	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.20	264	4510623	35.02	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.75	163	226391	2.974	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022420\
Data File : BP001894.D
Acq On : 25 Feb 2020 11:13
Operator : CG/JU
Sample : L1542-20
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBD54

Quant Time: Feb 25 12:29:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 07:02:36 2020
Response via : Initial Calibration

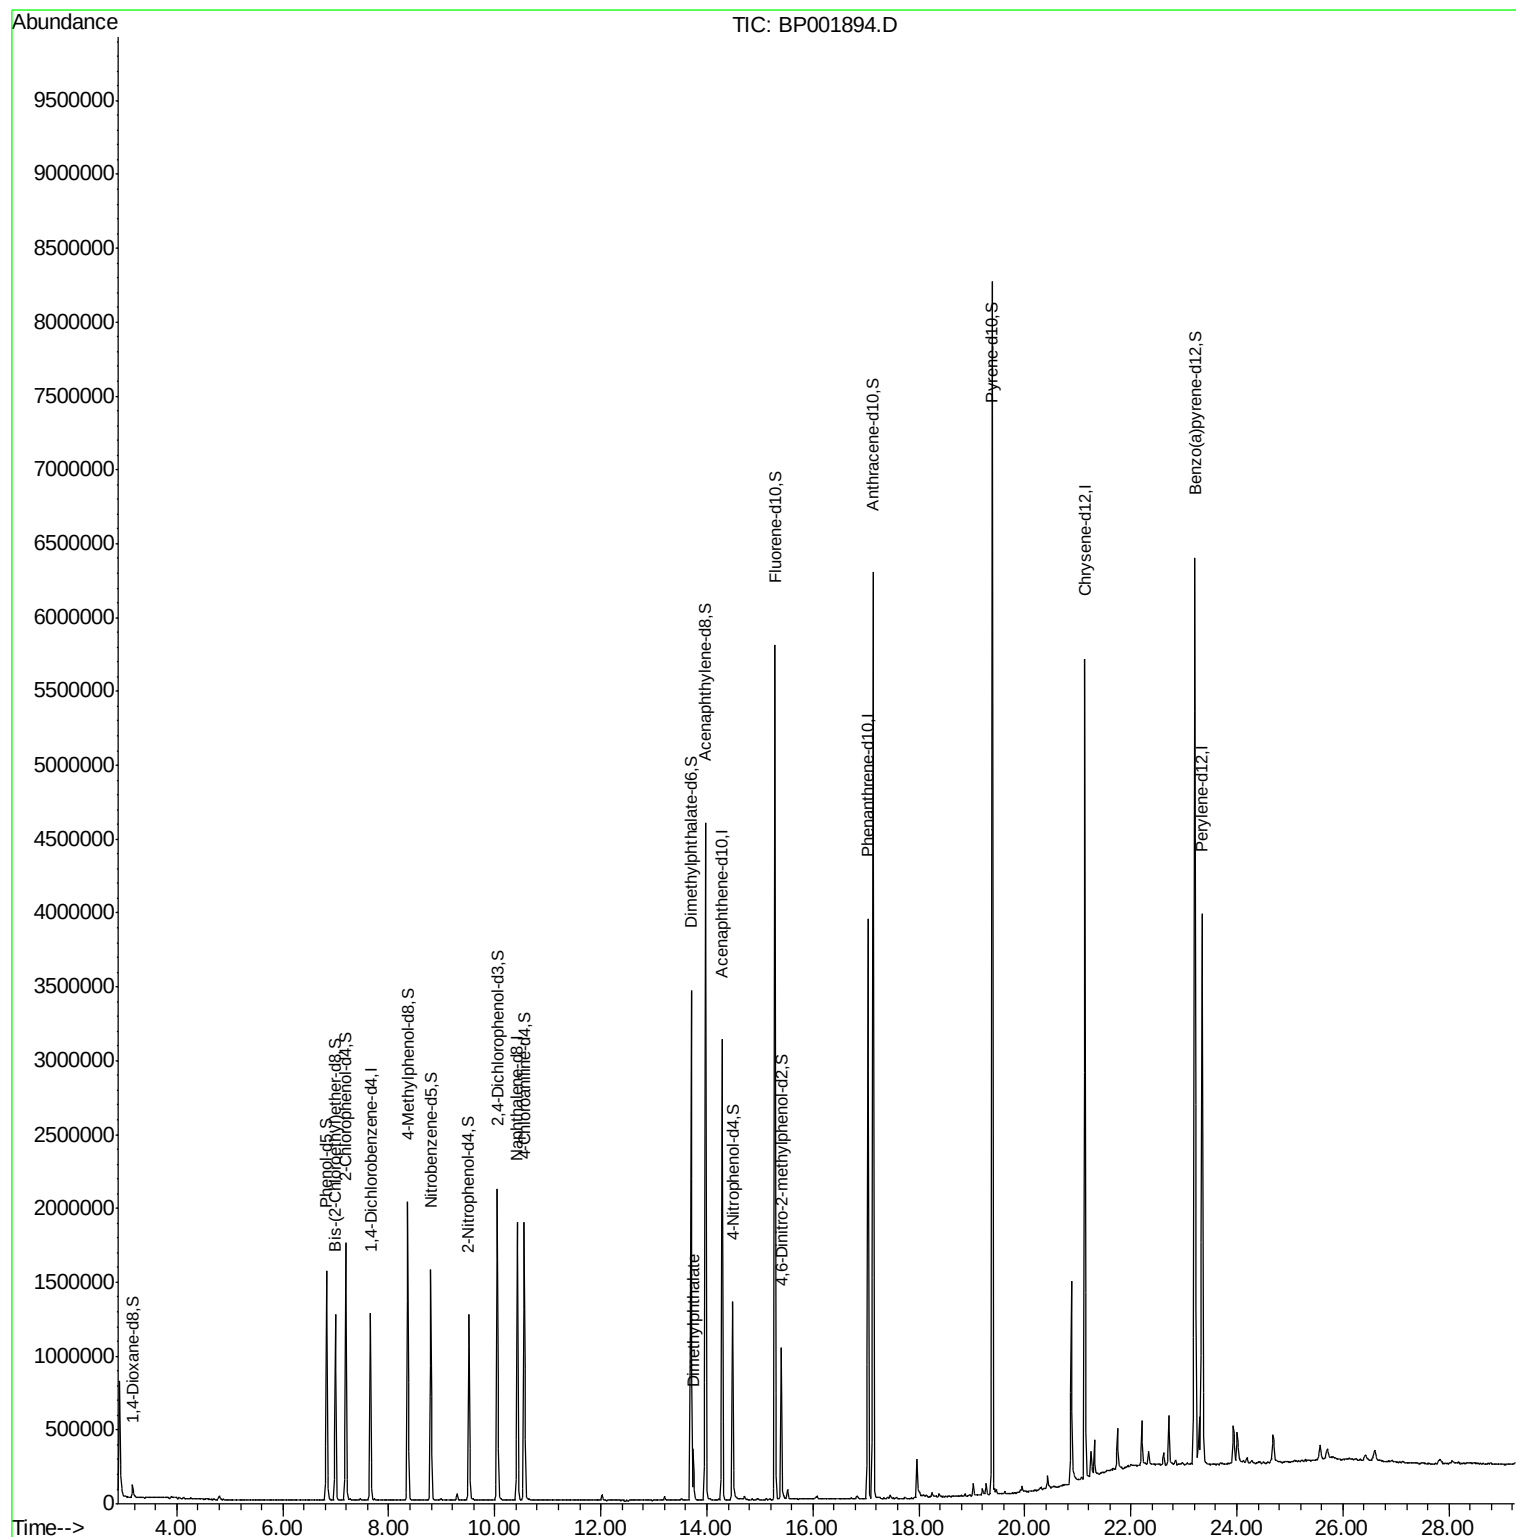

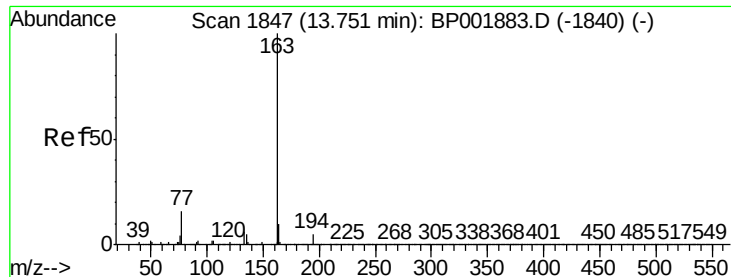

#45

Dimethylphthalate

Concen: 2.974 ng/ul

RT: 13.75 min Scan# 1846

Delta R.T. -0.01 min

Lab File: BP001894.D

Acq: 25 Feb 2020 11:13

Instrument :

BNA_P

ClientSampleId :

DBD54

Tot Ion:163 Resp: 226391

Ion Ratio Lower Upper

163 100

194 4.0 3.5 5.3

164 10.2 8.0 12.0

