

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022420\
 Data File : BP001895.D
 Acq On : 25 Feb 2020 11:47
 Operator : CG/JU
 Sample : L1542-21
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBD55

Quant Time: Feb 25 14:20:36 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 25 07:02:36 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	375197	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	1613776	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1058521	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	2488427	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2786535	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	2819047	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.17	96	47753	5.29	ng/uL	0.00
5) Phenol-d5	6.83	99	918784	32.41	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	518177	31.46	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	801231	34.97	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	762602	33.91	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	396720	36.31	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	447102	45.25	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	842919	35.88	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	1163807	41.88	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	2603585	35.05	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	3202258	35.01	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	447135	34.57	ng/ul	0.00
58) Fluorene-d10	15.29	176	2375287	35.56	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	297185	30.29	ng/ul	0.00
71) Anthracene-d10	17.14	188	3763093	34.33	ng/ul	0.00
79) Pyrene-d10	19.38	212	4432092	30.99	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	4801263	35.27	ng/ul	0.00
Target Compounds						
6) Phenol	6.85	94	31660	1.054	ng/ul#	81
45) Dimethylphthalate	13.75	163	208624	2.668	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022420\
Data File : BP001895.D
Acq On : 25 Feb 2020 11:47
Operator : CG/JU
Sample : L1542-21
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBD55

Quant Time: Feb 25 14:20:36 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 07:02:36 2020
Response via : Initial Calibration

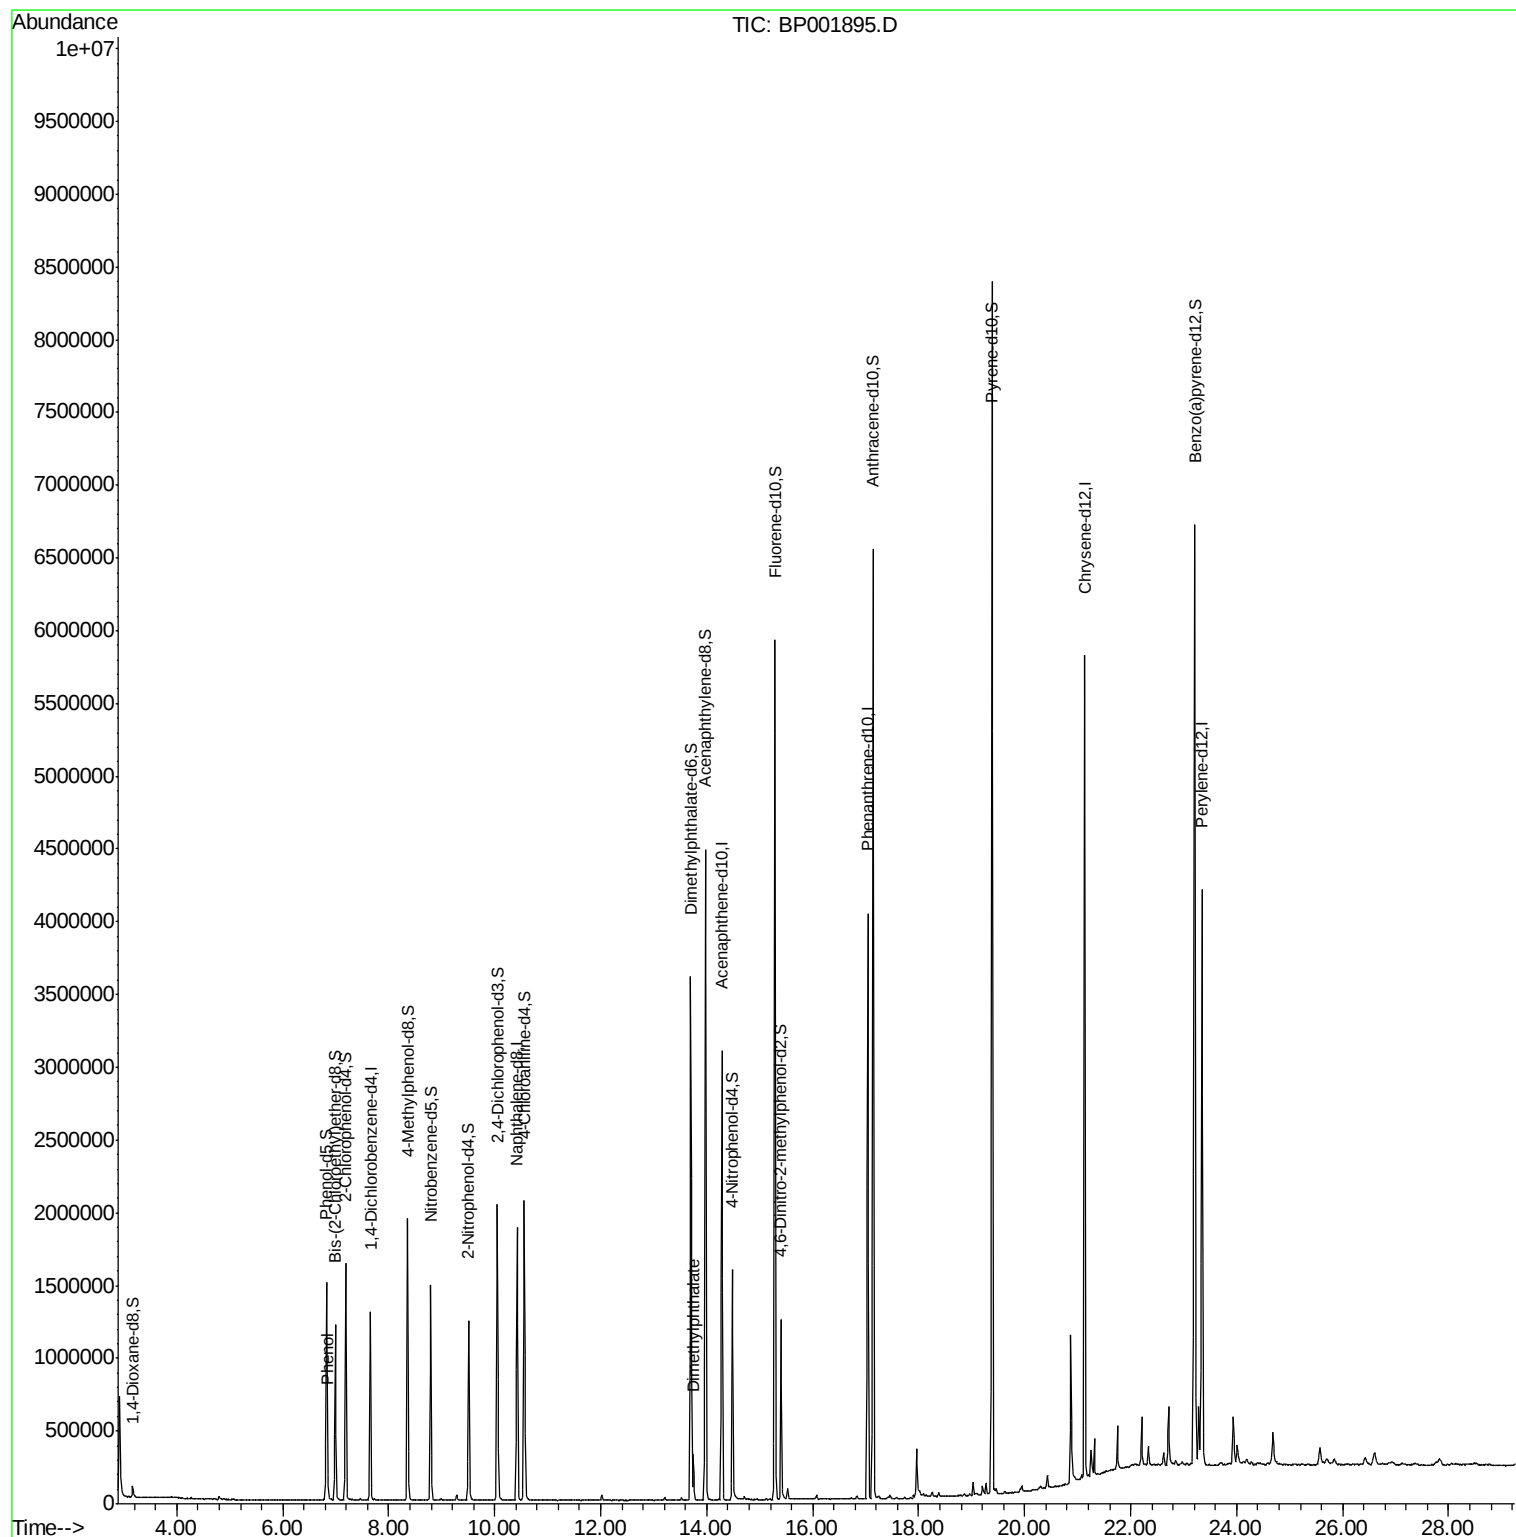

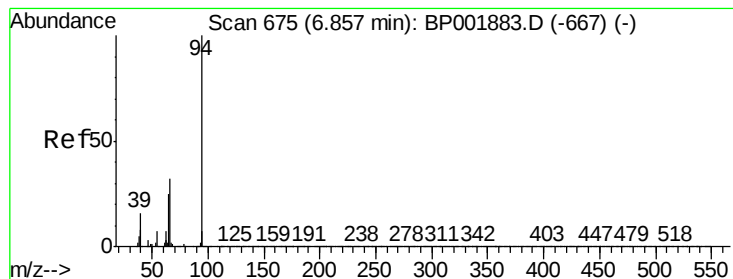





#6

Phenol

Concen: 1.054 ng/ul
 RT: 6.85 min Scan# 674
 Delta R.T. -0.01 min
 Lab File: BP001895.D
 Acq: 25 Feb 2020 11:47

Instrument :
 BNA_P
 ClientSampleId :
 DBD55

Tot Ion: 94 Resp: 31660
 Ion Ratio Lower Upper
 94 100
 65 29.4 19.8 29.6
 66 47.5 26.6 39.8#

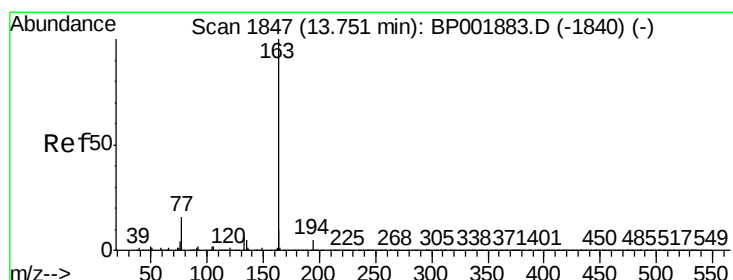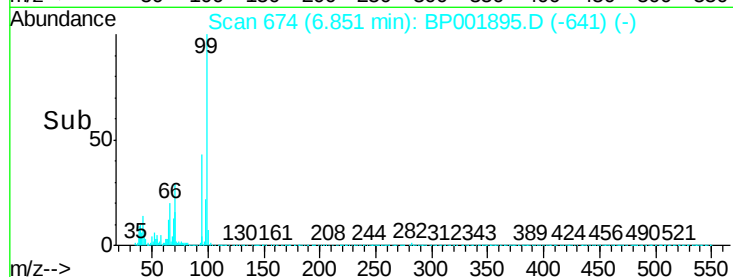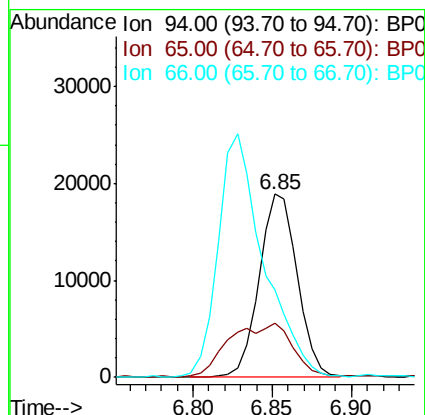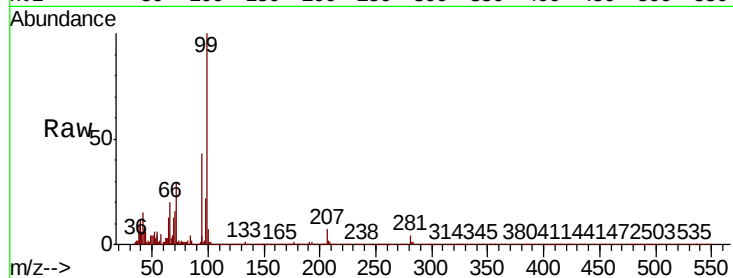

#45

Dimethylphthalate

Concen: 2.668 ng/ul
 RT: 13.75 min Scan# 1846
 Delta R.T. -0.01 min
 Lab File: BP001895.D
 Acq: 25 Feb 2020 11:47

Tgt Ion: 163 Resp: 208624
 Ion Ratio Lower Upper
 163 100
 194 4.8 3.5 5.3
 164 10.0 8.0 12.0

