

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022420\
 Data File : BP001897.D
 Acq On : 25 Feb 2020 13:02
 Operator : CG/JU
 Sample : L1542-15
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBD51

Quant Time: Feb 25 14:24:07 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 25 07:02:36 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	362292	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	1571012	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1049836	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	2451834	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2705613	20.00	ng/ul	0.00
86) Perylene-d12	23.35	264	2625797	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.17	96	37916	4.35	ng/uL	0.00
5) Phenol-d5	6.83	99	739788	27.02	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	421723	26.52	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	653551	29.54	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	622567	28.67	ng/ul	-0.01
19) Nitrobenzene-d5	8.79	128	320168	30.11	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	357367	37.16	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	679503	29.71	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	943095	34.86	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	2122303	28.81	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	2612697	28.80	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	345990	26.97	ng/ul	0.00
58) Fluorene-d10	15.29	176	1940001	29.28	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	219213	22.68	ng/ul	0.00
71) Anthracene-d10	17.14	188	3033417	28.08	ng/ul	0.00
79) Pyrene-d10	19.39	212	3609616	26.00	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	3722042	29.35	ng/ul	0.00
Target Compounds						
6) Phenol	6.85	94	30498	1.051	ng/ul	92
45) Dimethylphthalate	13.75	163	248151	3.200	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022420\
Data File : BP001897.D
Acq On : 25 Feb 2020 13:02
Operator : CG/JU
Sample : L1542-15
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBD51

Quant Time: Feb 25 14:24:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 07:02:36 2020
Response via : Initial Calibration

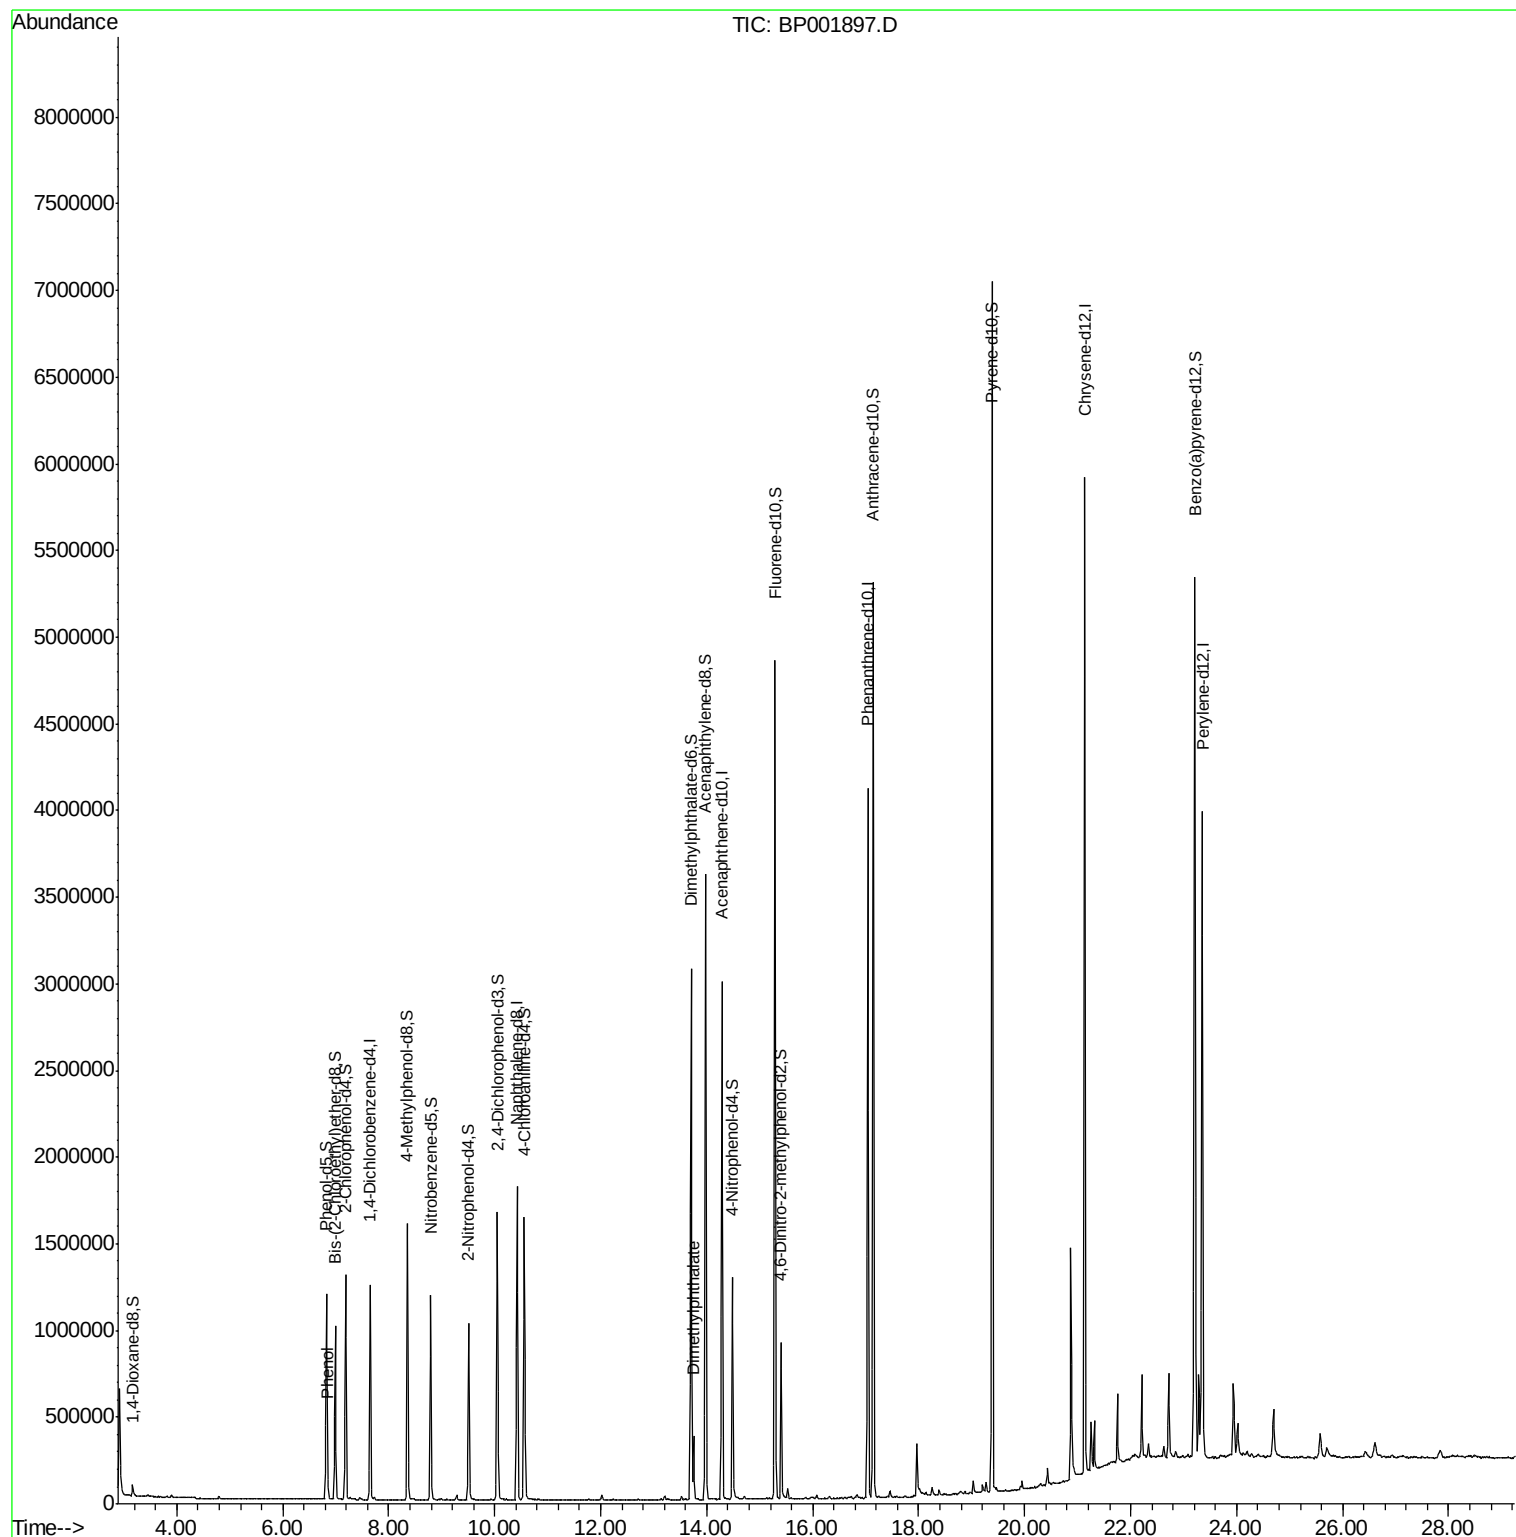

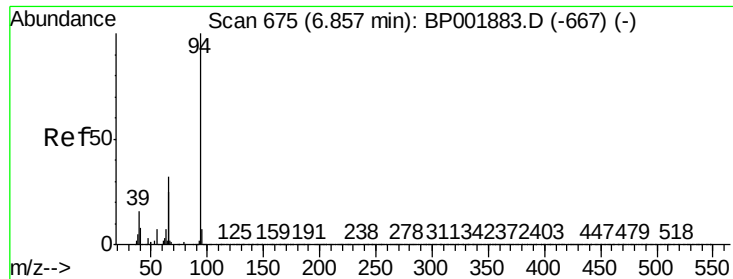





#6

Phenol

Concen: 1.051 ng/ul
 RT: 6.85 min Scan# 674
 Delta R.T. -0.01 min
 Lab File: BP001897.D
 Acq: 25 Feb 2020 13:02

Instrument :
 BNA_P
 ClientSampleId :
 DBD51

Tot Ion	Ratio	Lower	Upper
94	100		
65	27.4	19.8	29.6
66	39.2	26.6	39.8

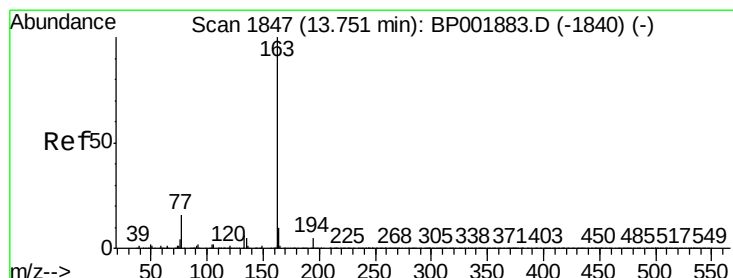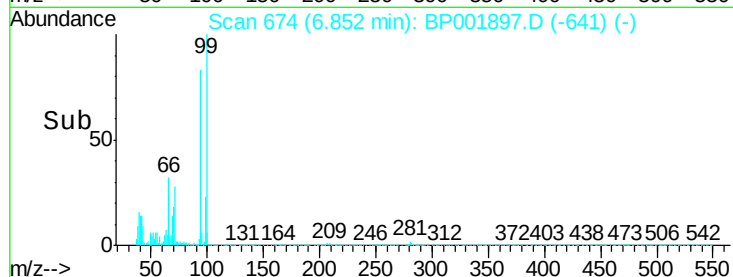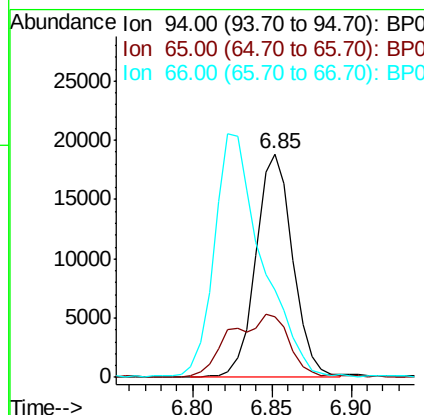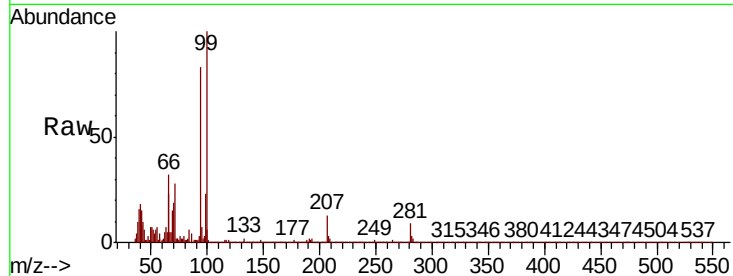

#45

Dimethylphthalate

Concen: 3.200 ng/ul
 RT: 13.75 min Scan# 1847
 Delta R.T. 0.00 min
 Lab File: BP001897.D
 Acq: 25 Feb 2020 13:02

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.4	3.5	5.3
164	9.8	8.0	12.0

