

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022420\
 Data File : BP001908.D
 Acq On : 25 Feb 2020 21:04
 Operator : CG/JU
 Sample : L1543-02
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBD58

Quant Time: Feb 26 04:41:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 26 04:37:11 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	510222	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	2200168	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1426058	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	3249741	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	3403478	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	3359441	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.17	96	48327	3.93	ng/uL	0.00
5) Phenol-d5	6.83	99	934154	24.23	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	527281	23.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	807967	25.93	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	785871	25.70	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	410716	27.58	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	453438	33.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	852770	26.62	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	1028121	27.14	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	2583047	25.81	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	3171126	25.73	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	395333	22.69	ng/ul	0.00
58) Fluorene-d10	15.29	176	2329034	25.88	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	280228	21.87	ng/ul	0.00
71) Anthracene-d10	17.13	188	3558525	24.86	ng/ul	0.00
79) Pyrene-d10	19.38	212	4139919	23.70	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.20	264	4195606	25.86	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.75	163	197872	1.879	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022420\
Data File : BP001908.D
Acq On : 25 Feb 2020 21:04
Operator : CG/JU
Sample : L1543-02
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBD58

Quant Time: Feb 26 04:41:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 26 04:37:11 2020
Response via : Initial Calibration

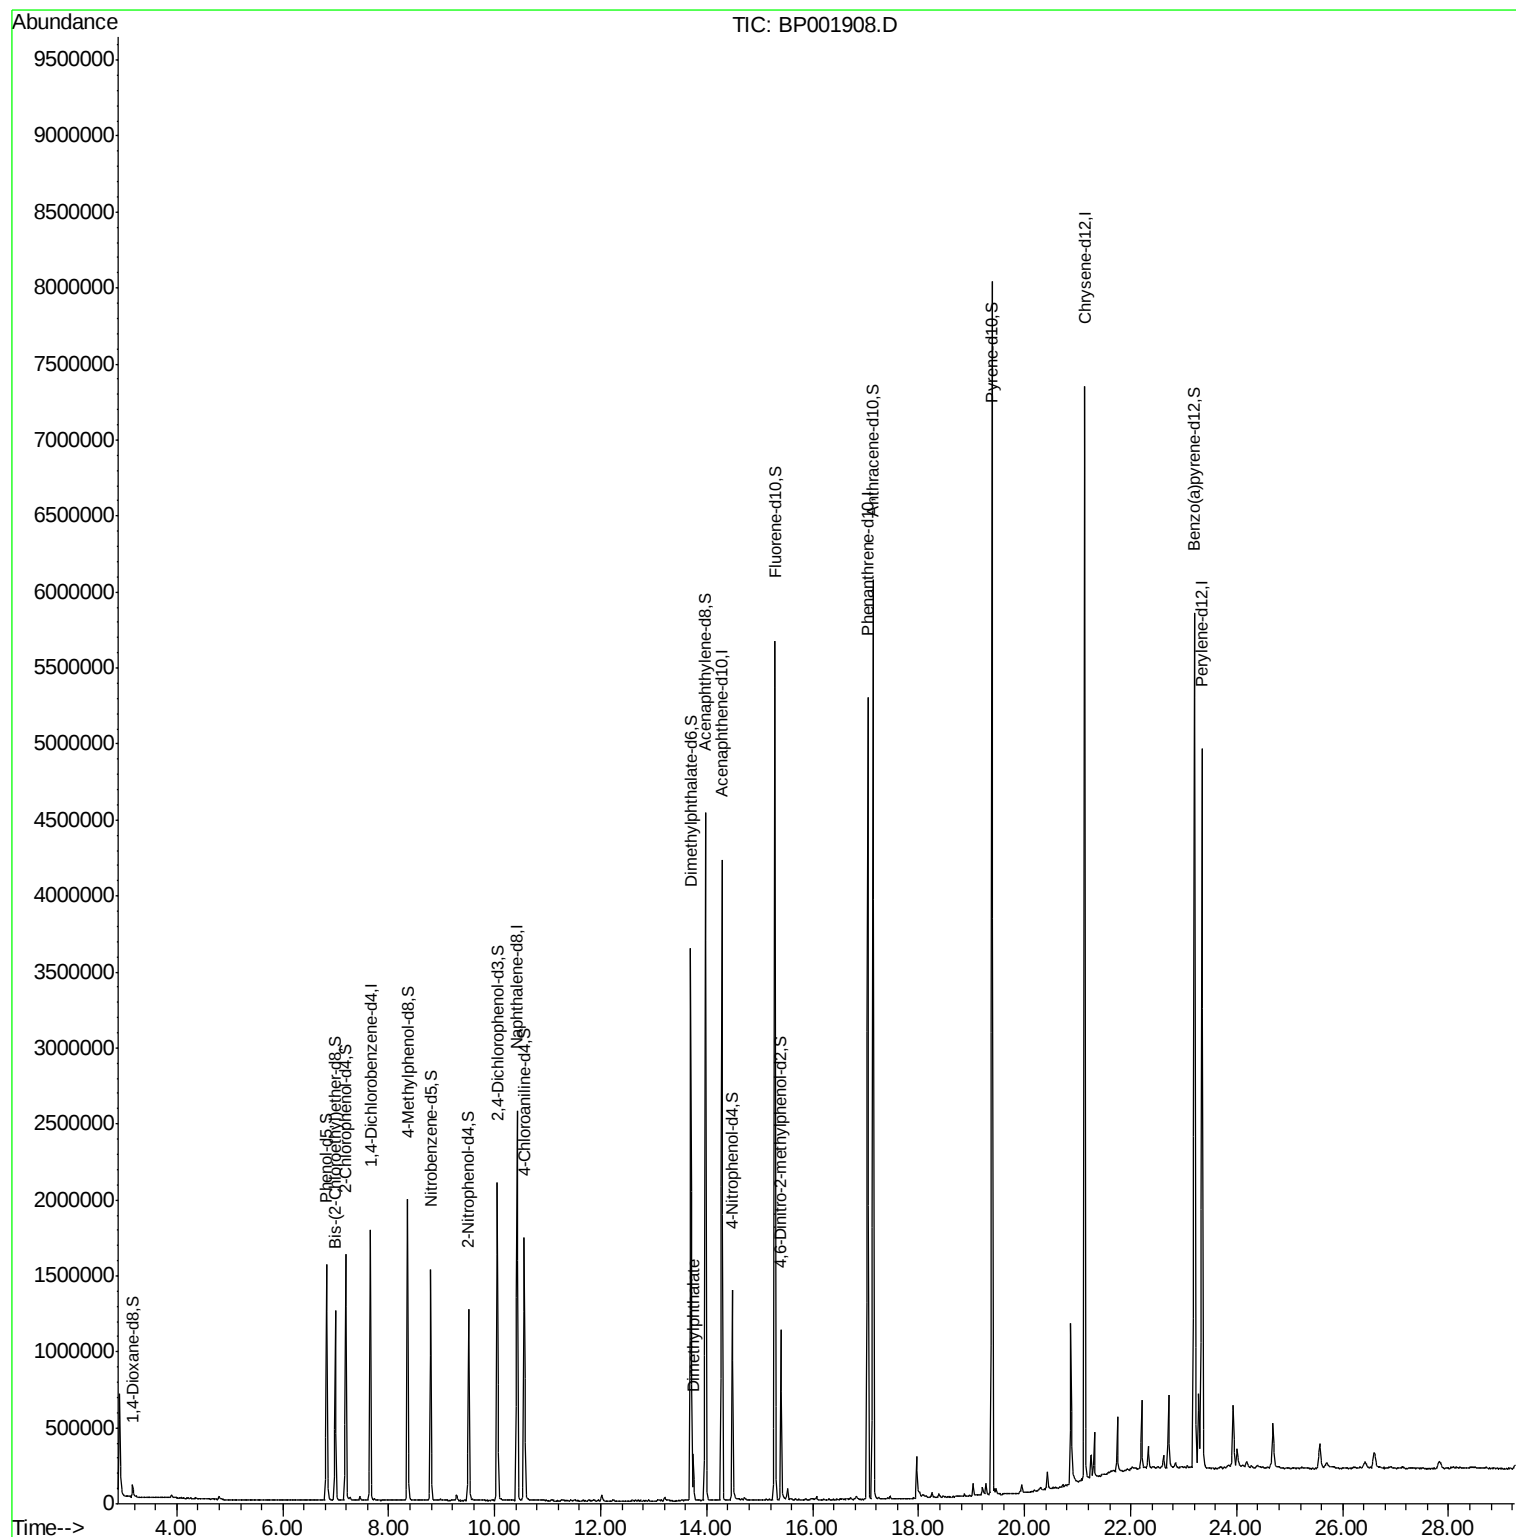

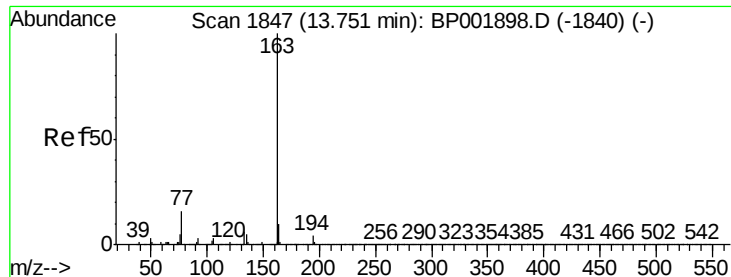

#45

Dimethylphthalate

Concen: 1.879 ng/ul

RT: 13.75 min Scan# 1846

Delta R.T. -0.01 min

Lab File: BP001908.D

Acq: 25 Feb 2020 21:04

Instrument :

BNA_P

ClientSampleId :

DBD58


Tot Ion:163 Resp: 197872

Ion Ratio Lower Upper

163 100

194 4.1 3.5 5.3

164 10.0 8.0 12.0

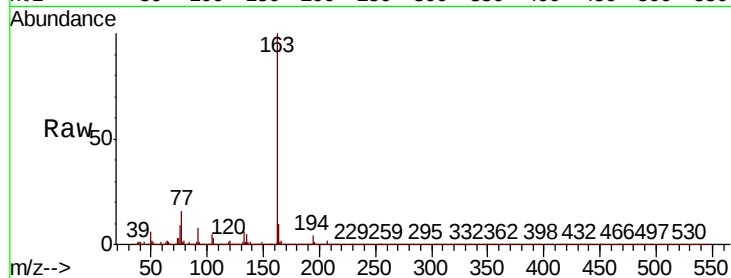

Abundance Ion 163.00 (162.70 to 163.70): E

200000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

