

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022420\
 Data File : BP001921.D
 Acq On : 26 Feb 2020 11:11
 Operator : CG/JU
 Sample : L1543-13
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBD95

Quant Time: Feb 27 03:37:01 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 26 05:53:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	311505	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	1344055	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	866409	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	1998494	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2167021	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	2134196	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.17	96	33396	4.45	ng/uL	0.00
5) Phenol-d5	6.83	99	688447	29.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	389327	28.47	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	612535	32.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	561108	30.05	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	306226	33.66	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	341068	41.45	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	637148	32.56	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	816014	35.26	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	2066363	33.99	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	2433057	32.50	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	360989	34.10	ng/ul	0.00
58) Fluorene-d10	15.28	176	1811956	33.14	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	249114	31.62	ng/ul	0.00
71) Anthracene-d10	17.13	188	3122120	35.46	ng/ul	0.00
79) Pyrene-d10	19.38	212	3828261	34.43	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.20	264	3966989	38.49	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	6.85	94	36561	1.466	ng/ul	92
45) Dimethylphthalate	13.75	163	261484	4.086	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022420\
Data File : BP001921.D
Acq On : 26 Feb 2020 11:11
Operator : CG/JU
Sample : L1543-13
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBD95

Quant Time: Feb 27 03:37:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 26 05:53:41 2020
Response via : Initial Calibration

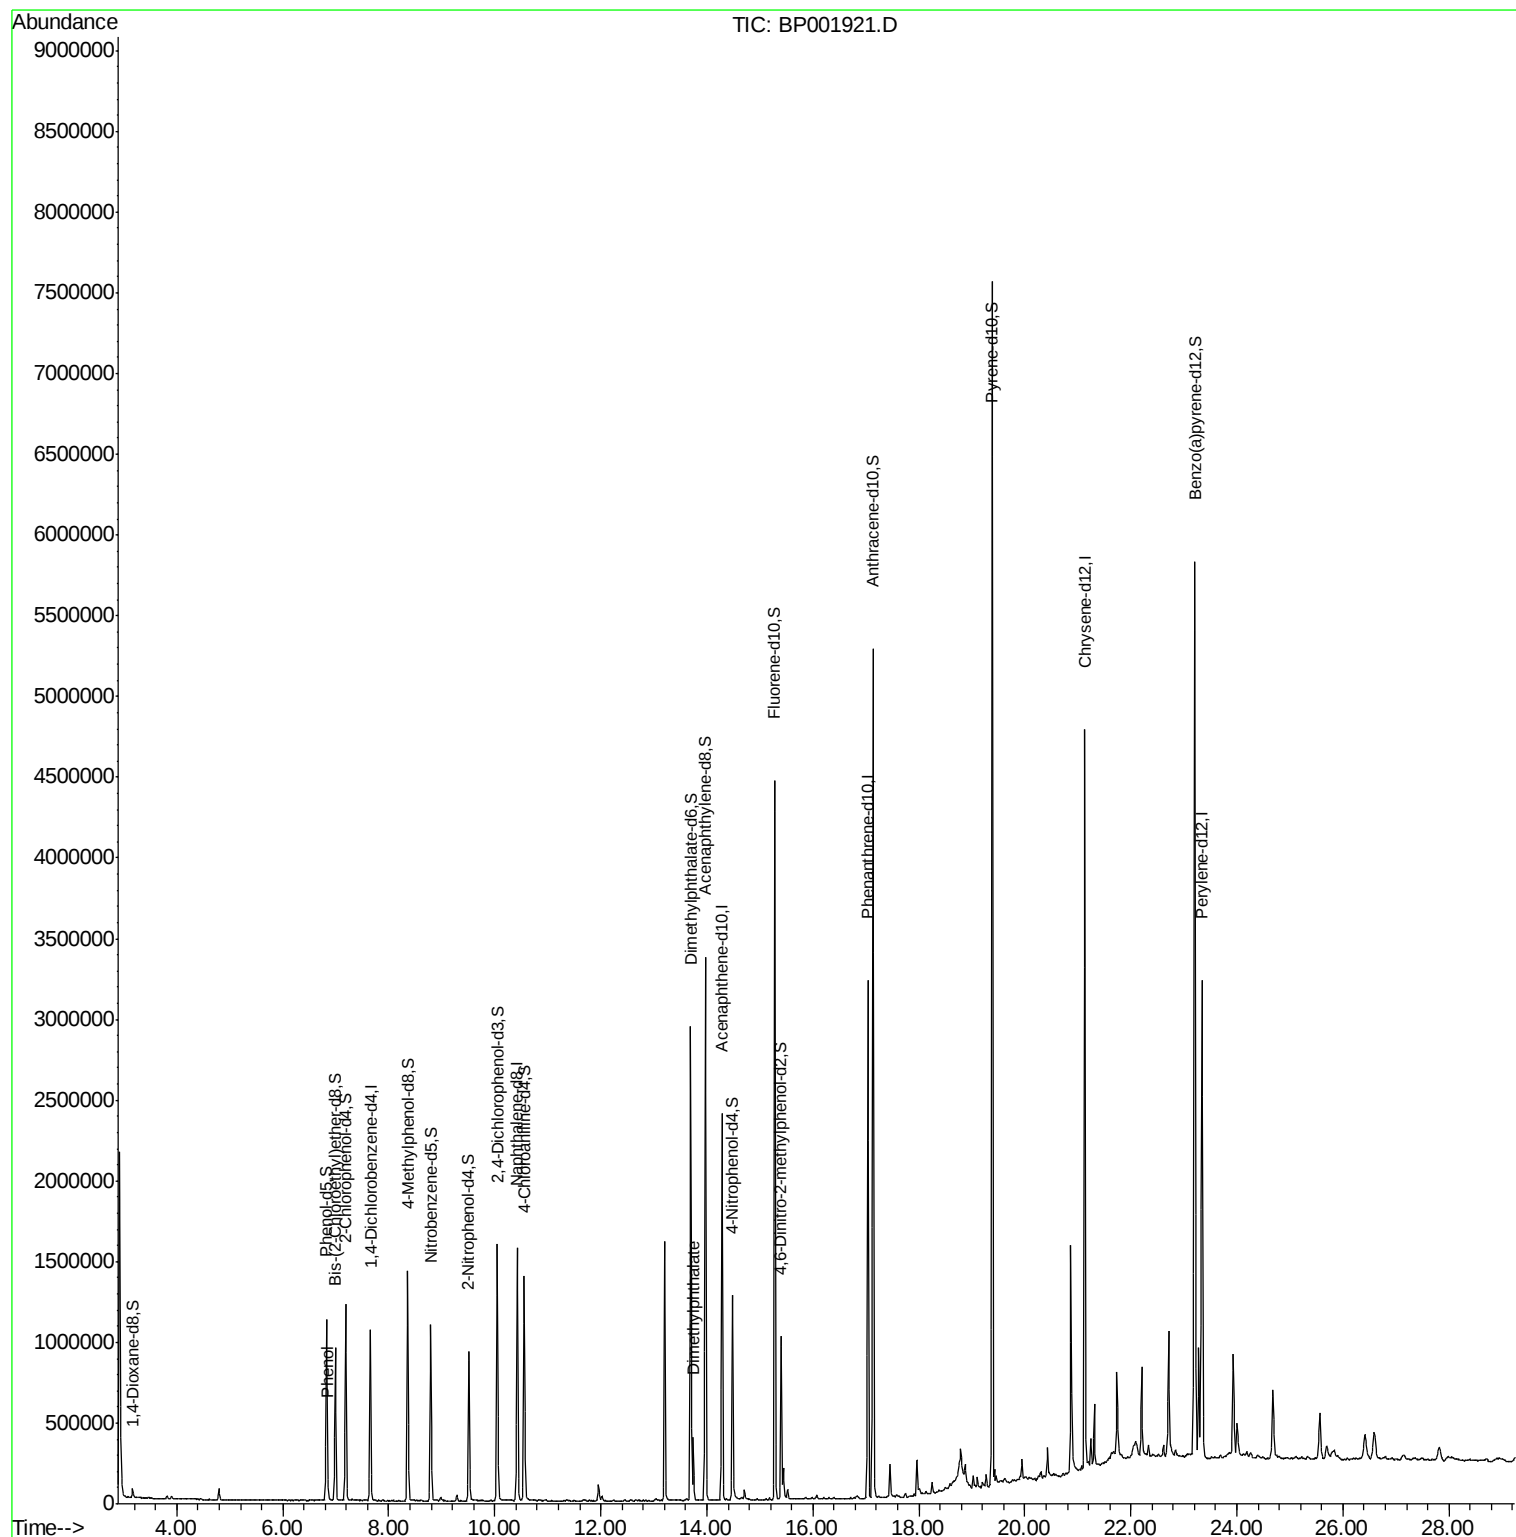

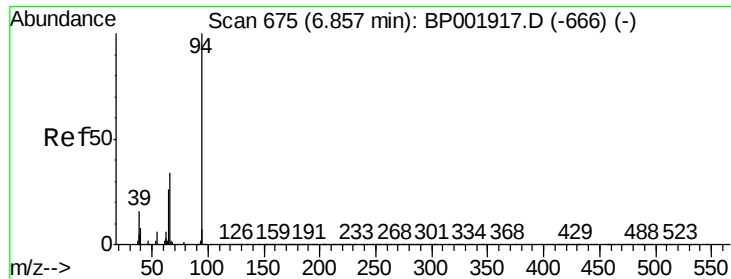

#6

Phenol

Concen: 1.466 ng/ul

RT: 6.85 min Scan# 674

Delta R.T. 0.00 min

Lab File: BP001921.D

Acq: 26 Feb 2020 11:11

Instrument :

BNA_P

ClientSampleId :

DBD95


Tot Ion: 94 Resp: 36561

Ion Ratio Lower Upper

94 100

65 26.8 19.8 29.6




66 39.2 26.6 39.8

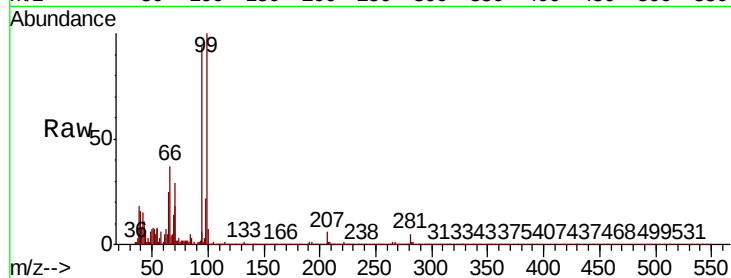

Abundance Ion 94.00 (93.70 to 94.70): BP0

Ion 65.00 (64.70 to 65.70): BP0

Ion 66.00 (65.70 to 66.70): BP0

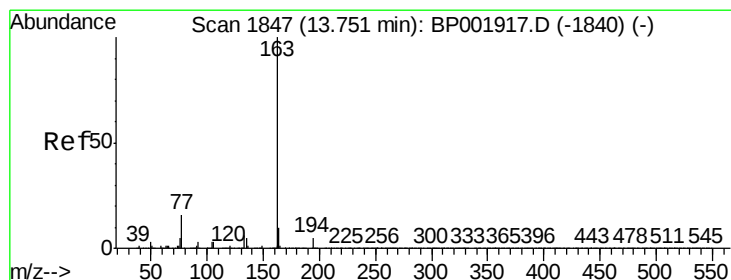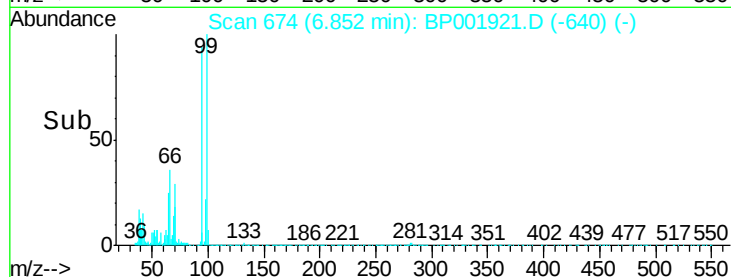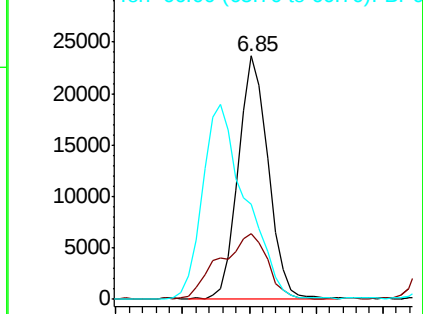

#45

Dimethylphthalate

Concen: 4.086 ng/ul

RT: 13.75 min Scan# 1846

Delta R.T. -0.01 min

Lab File: BP001921.D

Acq: 26 Feb 2020 11:11


Tgt Ion: 163 Resp: 261484

Ion Ratio Lower Upper

163 100

194 4.2 3.5 5.3

164 9.7 8.0 12.0

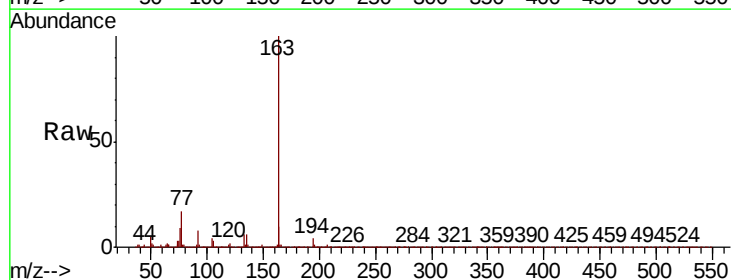

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

