

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022420\
 Data File : BP001930.D
 Acq On : 26 Feb 2020 18:36
 Operator : CG/JU
 Sample : L1543-20
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBDA2

Quant Time: Feb 27 04:21:11 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 27 04:02:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	337757	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	1418682	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	931020	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	2096964	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2156163	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	2149099	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.18	96	12675	1.56	ng/uL	0.00
5) Phenol-d5	6.83	99	235453	9.23	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	140479	9.47	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	210734	10.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	183642	9.07	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	98789	10.29	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	100614	11.58	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	204100	9.88	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	262847	10.76	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	701772	10.74	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	816605	10.15	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	67136	5.90	ng/ul	0.00
58) Fluorene-d10	15.28	176	624306	10.63	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	52623	6.37	ng/ul	0.00
71) Anthracene-d10	17.13	188	984297	10.66	ng/ul	0.00
79) Pyrene-d10	19.38	212	1203211	10.87	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.20	264	1121364	10.80	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.75	163	152438	2.217	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022420\
Data File : BP001930.D
Acq On : 26 Feb 2020 18:36
Operator : CG/JU
Sample : L1543-20
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBDA2

Quant Time: Feb 27 04:21:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 27 04:02:08 2020
Response via : Initial Calibration

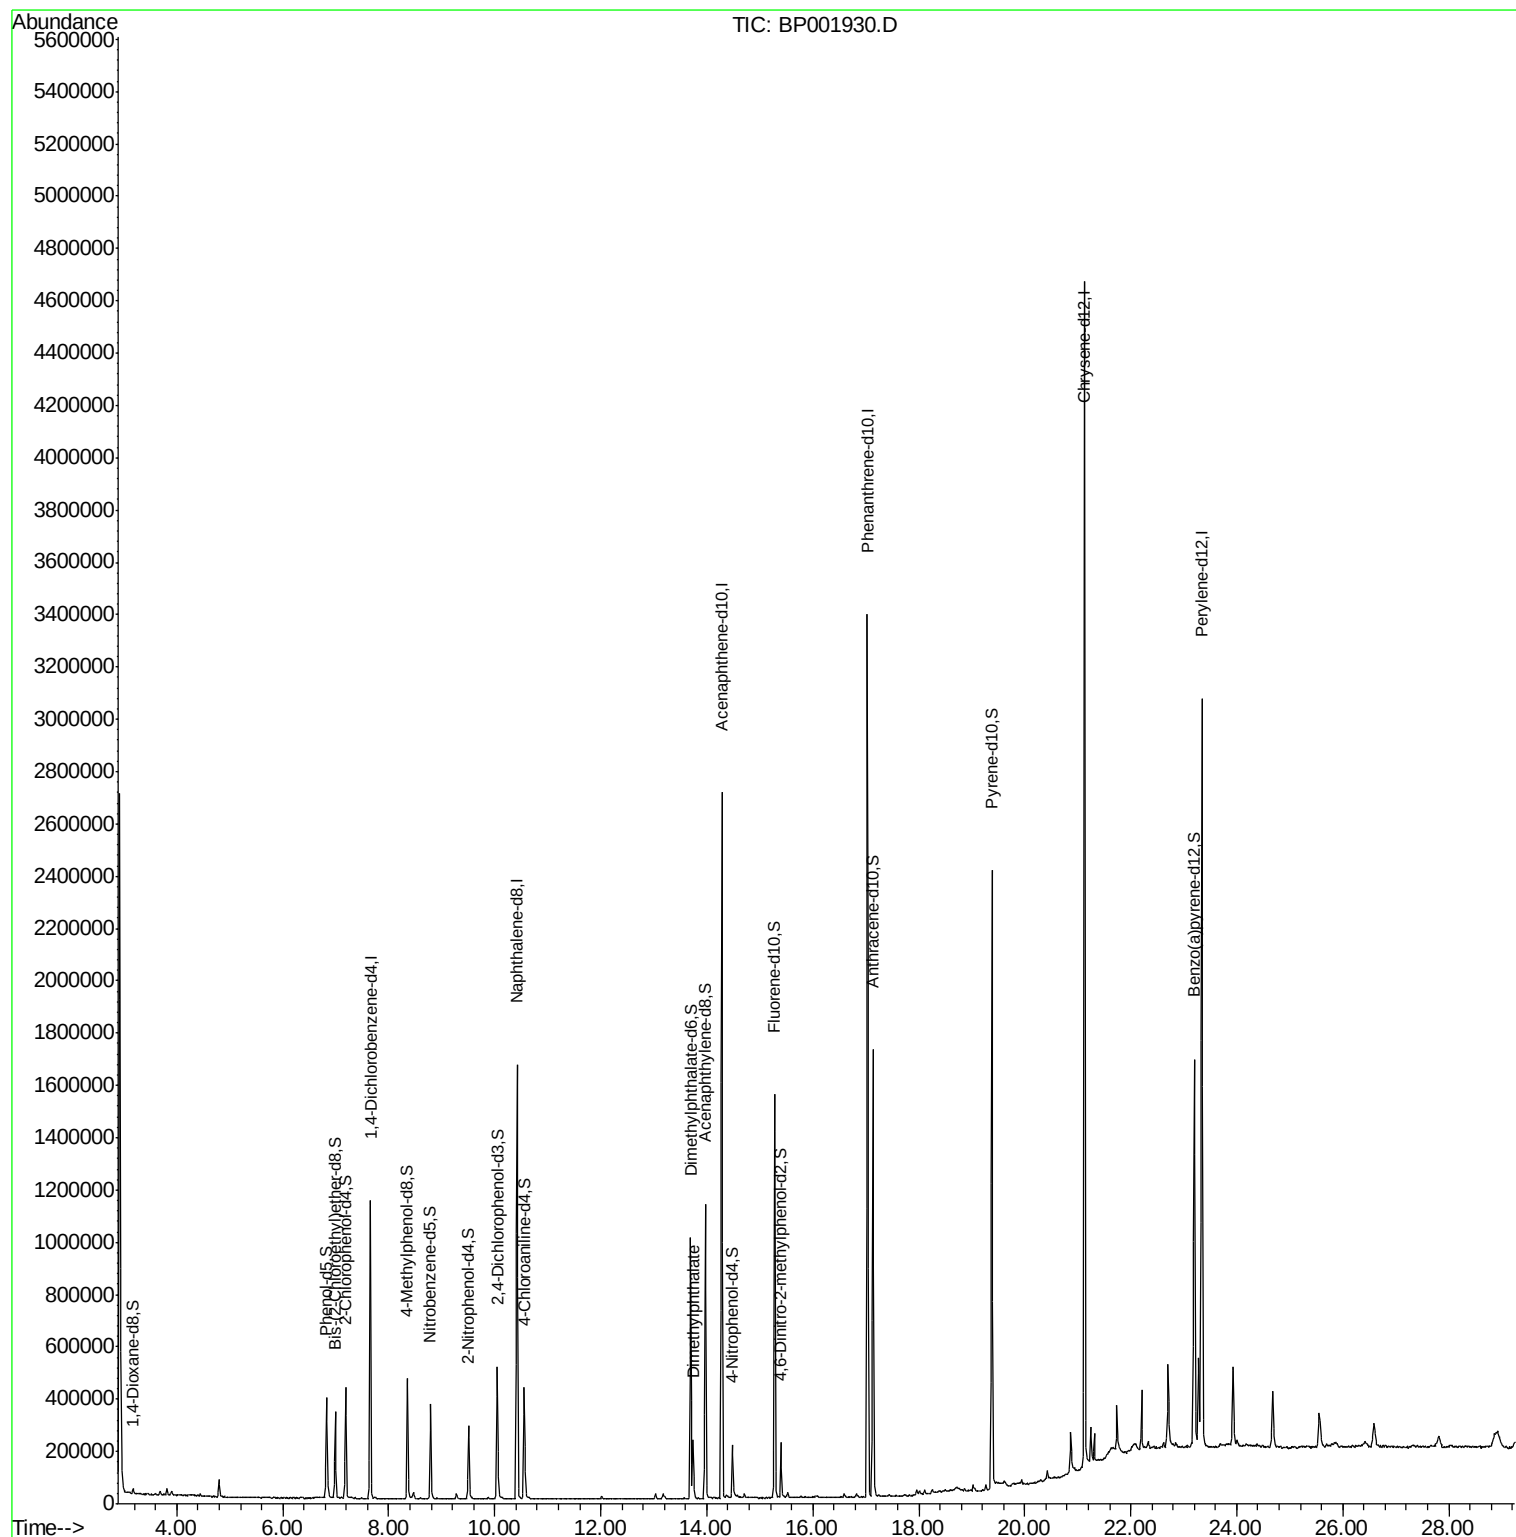

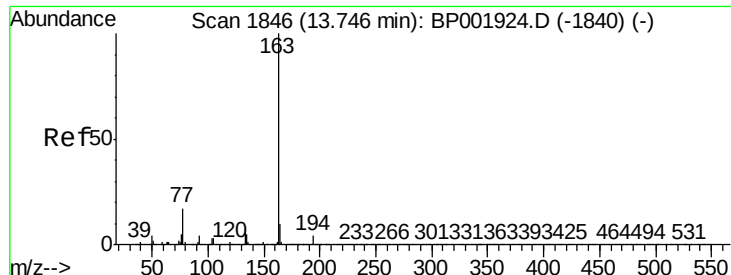

#45

Dimethylphthalate

Concen: 2.217 ng/ul

RT: 13.75 min Scan# 1846

Delta R.T. -0.01 min

Lab File: BP001930.D

Acq: 26 Feb 2020 18:36

Instrument :

BNA_P

ClientSampleId :

DBDA2


Tot Ion:163 Resp: 152438

Ion Ratio Lower Upper

163 100

194 4.6 3.5 5.3

164 9.8 8.0 12.0

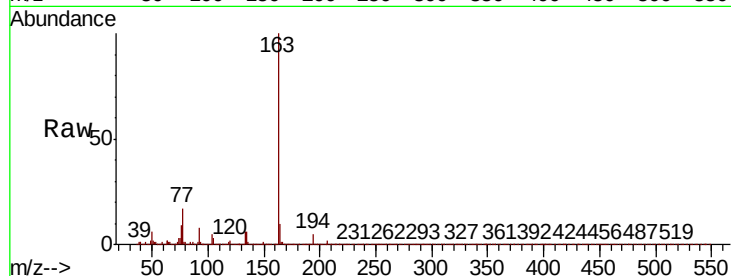

Abundance Ion 163.00 (162.70 to 163.70): E

150000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

