
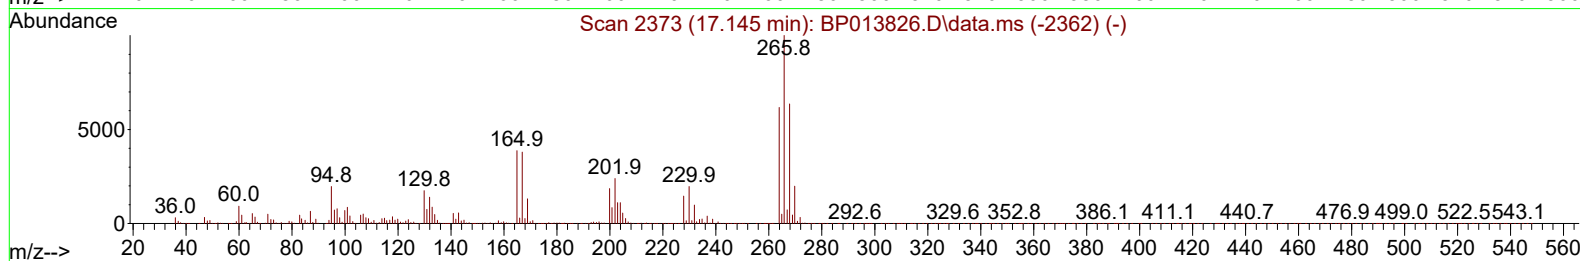
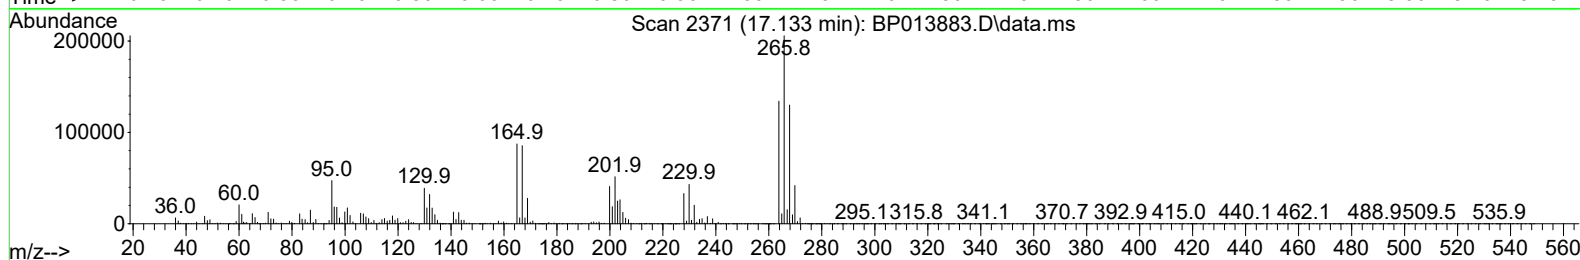


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022423\
Data File : BP013883.D
Acq On : 24 Feb 2023 12:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 25 00:16:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 16:57:00 2023
Response via : Initial Calibration

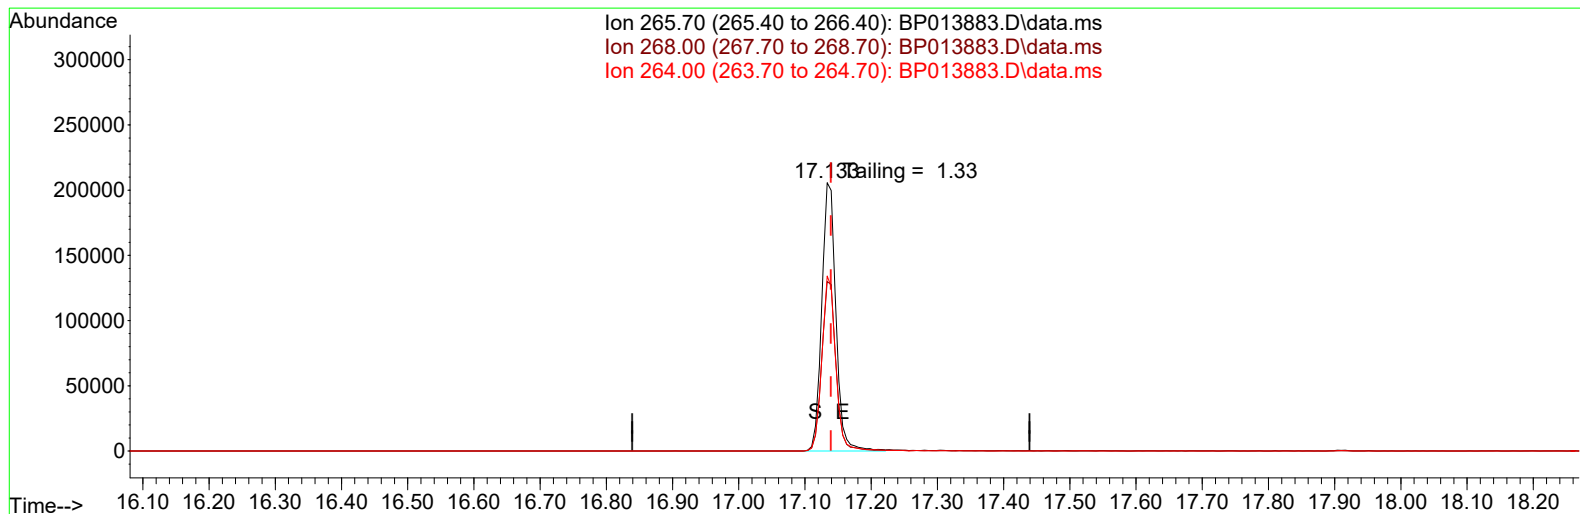

TIC: BP013883.D\data.ms

(70) Pentachlorophenol (C)




17.133min (-0.006) 256002.40 ng

response 306407

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.17
264.00	61.70	65.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022423\
Data File : BP013883.D
Acq On : 24 Feb 2023 12:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 25 00:16:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 16:57:00 2023
Response via : Initial Calibration

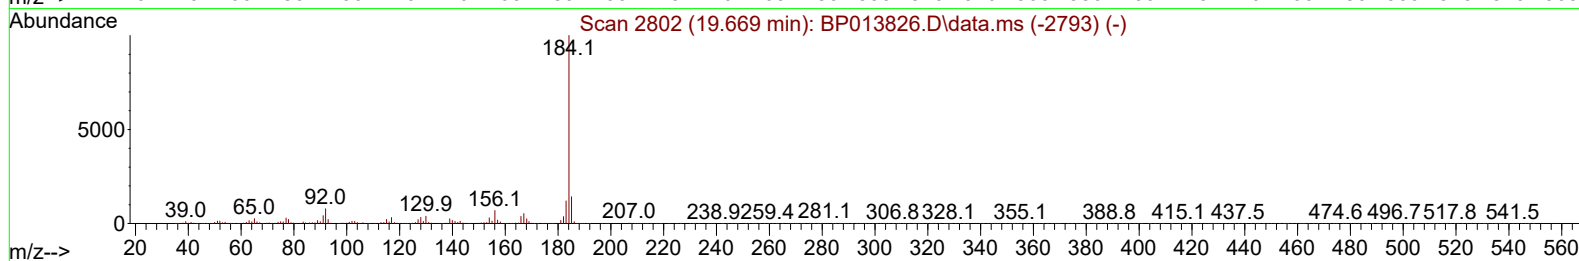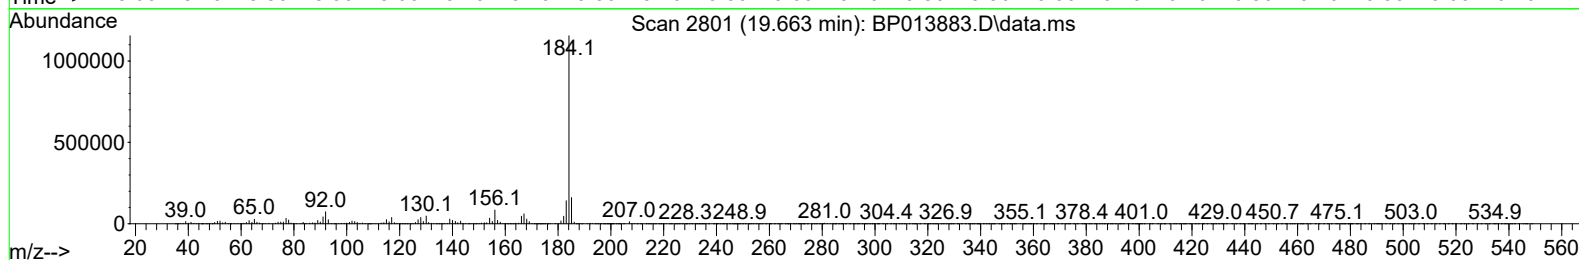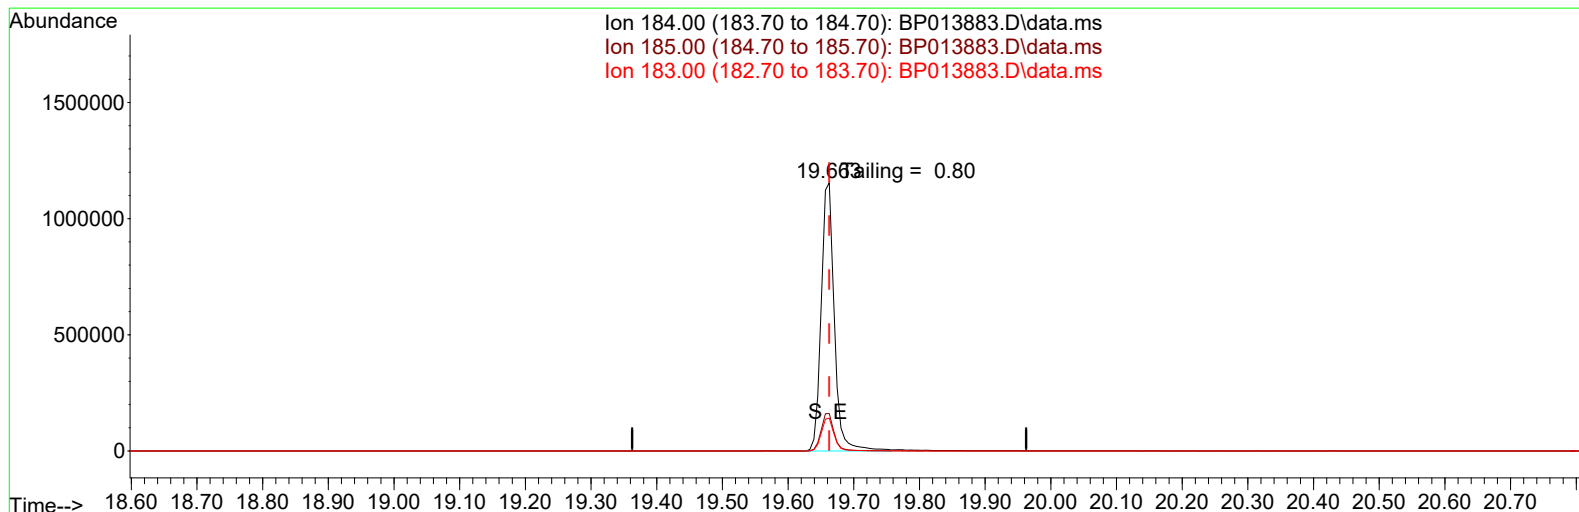

TIC: BP013883.D\data.ms

(77) Benzidine**19.663min (+ 0.000) 73088.87 ng****response 1612099**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.98
183.00	12.00	12.22
0.00	0.00	0.00