
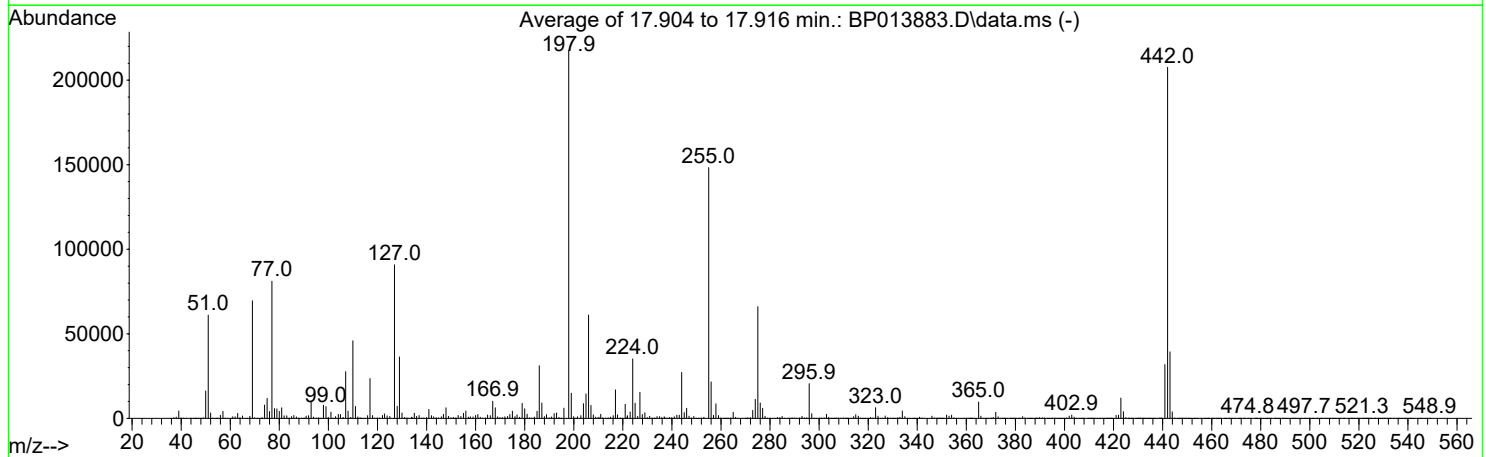


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022423\
Data File : BP013883.D
Acq On : 24 Feb 2023 12:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 24 16:57:00 2023

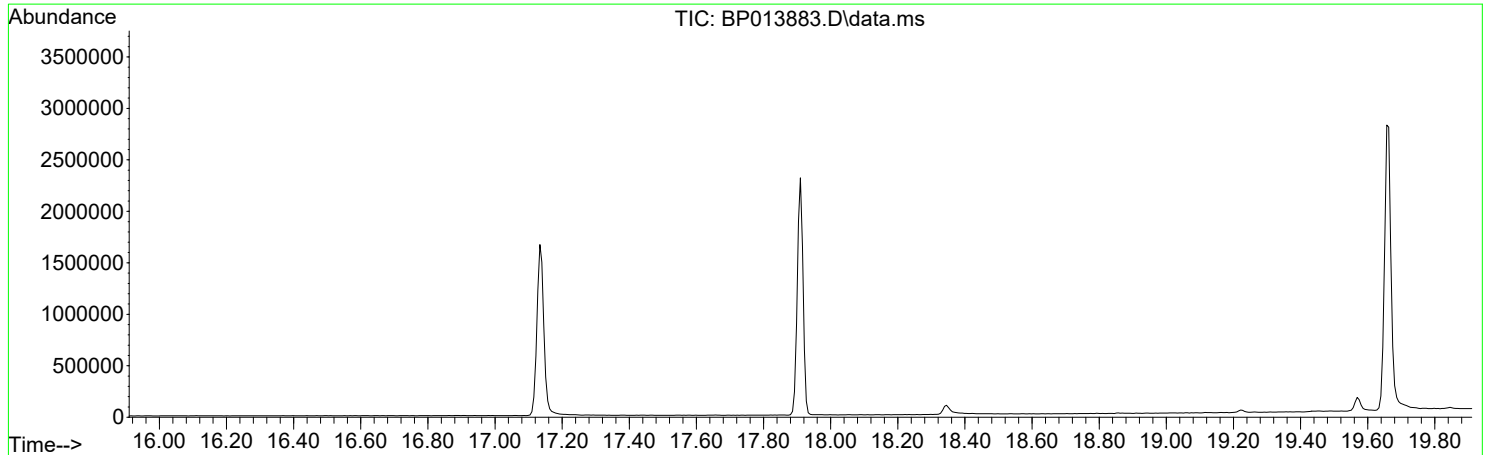

AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.0	60996	PASS
68	69	0.00	2	1.8	1225	PASS
69	198	0.00	100	32.0	69550	PASS
70	69	0.00	2	0.5	350	PASS
127	198	10	80	41.7	90797	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	217534	PASS
199	198	5	9	6.8	14899	PASS
275	198	10	60	30.4	66053	PASS
365	198	1	100	4.4	9666	PASS
441	198	0.01	100	14.6	31782	PASS
442	442	100	100	100.0	207552	PASS
443	442	15	24	19.0	39336	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/24/2023	BNA_P	<u>BP013883.D</u>
Compound Name	Response	Retention Time
DDT	853429	20.857
DDD	13792	20.474
DDE	561	19.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14353	867782	1.65

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022423\
 Data File : BP013883.D
 Acq On : 24 Feb 2023 12:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Feb 25 00:16:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 24 16:57:00 2023
 Response via : Initial Calibration

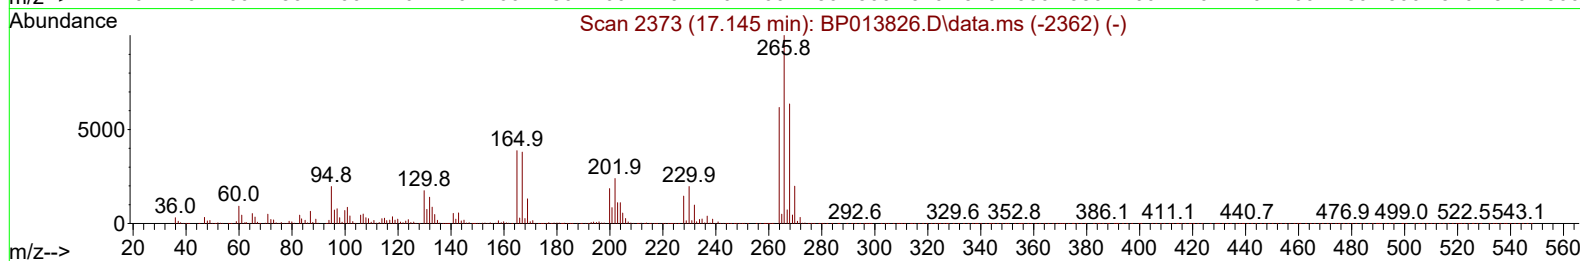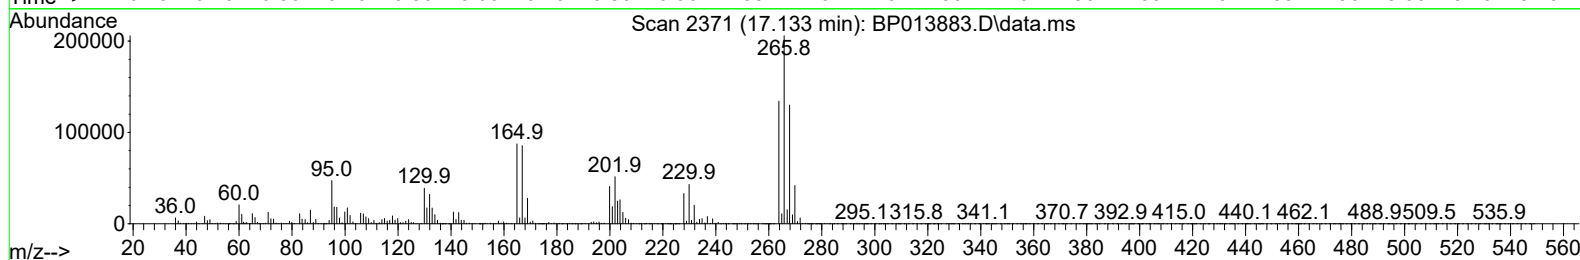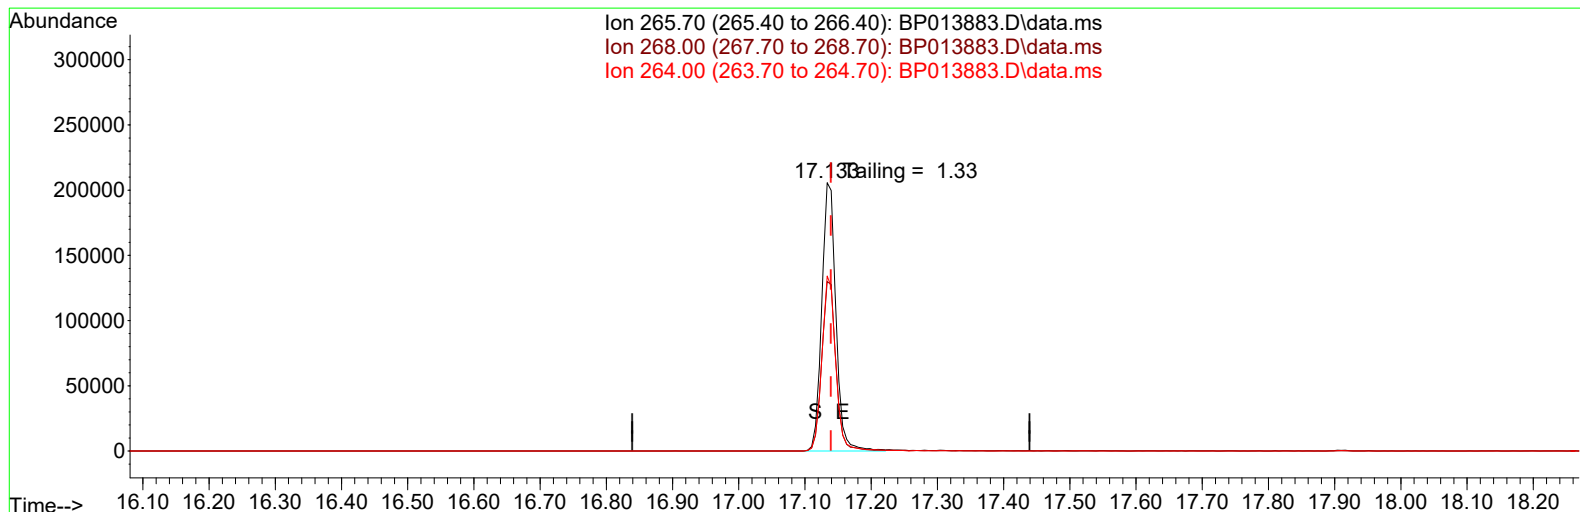

TIC: BP013883.D\data.ms

(70) Pentachlorophenol (C)

17.133min (-0.006) 256002.40 ng




response 306407

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.17
264.00	61.70	65.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022423\
Data File : BP013883.D
Acq On : 24 Feb 2023 12:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 25 00:16:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 16:57:00 2023
Response via : Initial Calibration

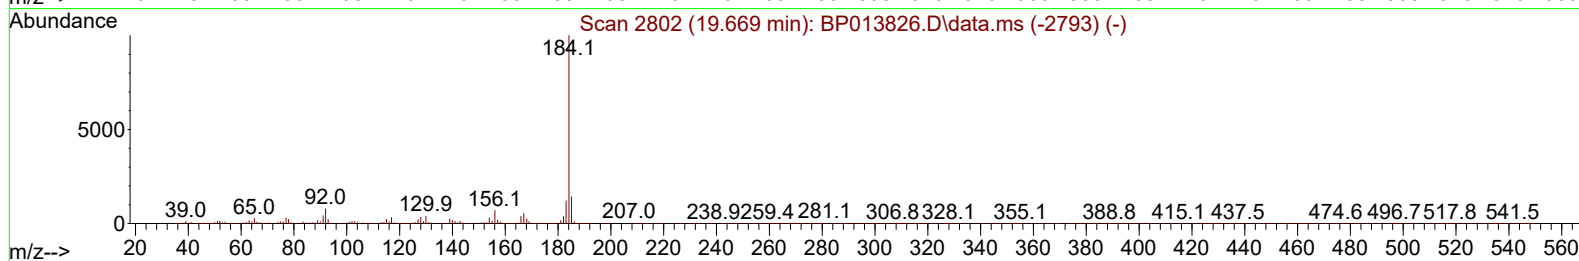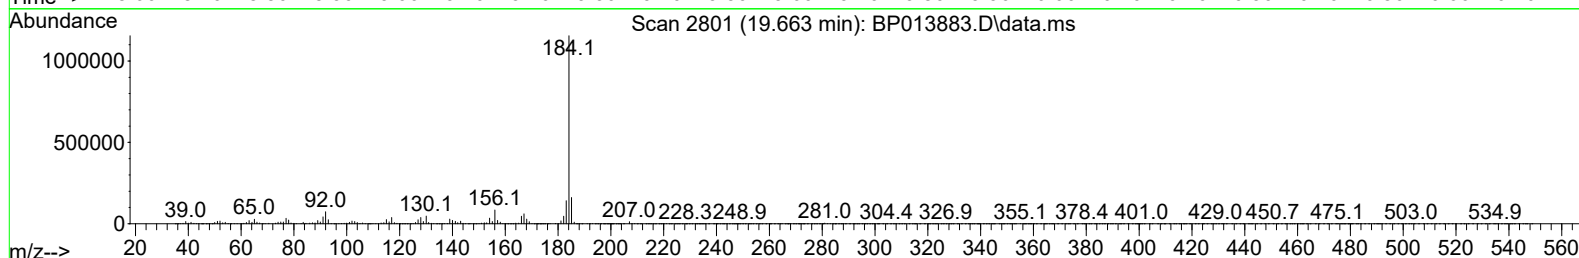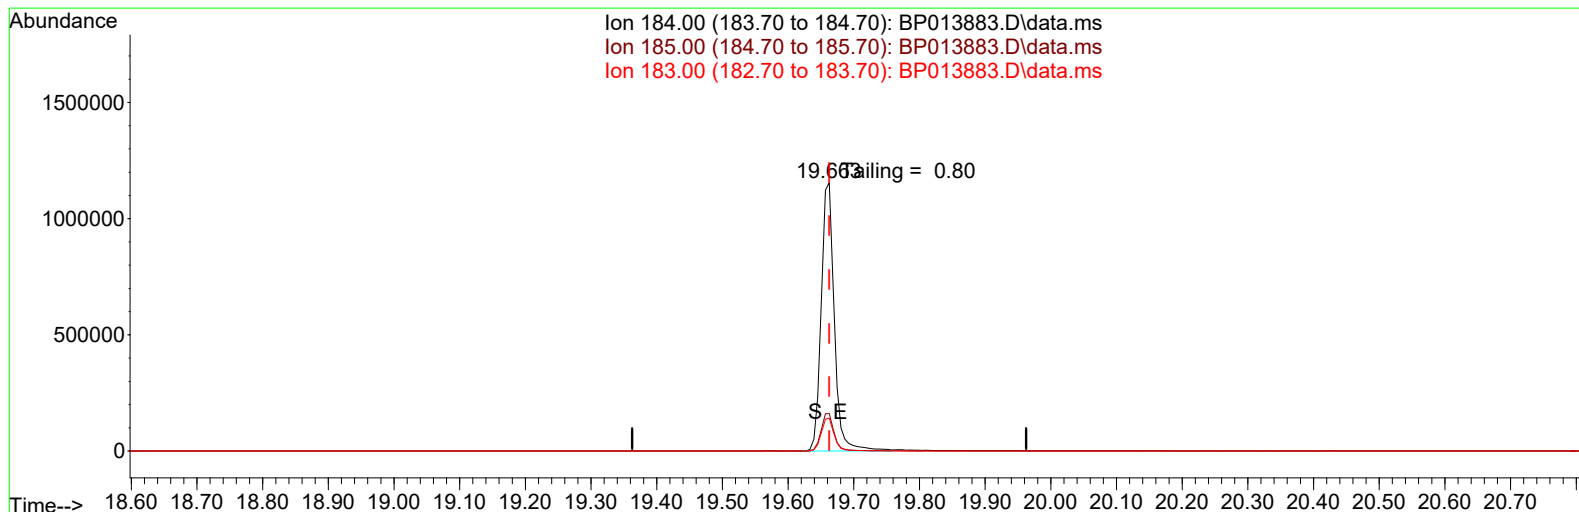

TIC: BP013883.D\data.ms

(77) Benzidine

19.663min (+ 0.000) 73088.87 ng

response 1612099

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.98
183.00	12.00	12.22
0.00	0.00	0.00