

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
 Data File : BP019871.D
 Acq On : 24 Feb 2024 20:21
 Operator : MA/JU
 Sample : P1564-17
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 LKWD-BACKFILL-17

Quant Time: Feb 26 00:15:25 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 23 13:10:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	66898	20.000	ng	0.00
21) Naphthalene-d8	10.698	136	243416	20.000	ng	0.00
39) Acenaphthene-d10	14.539	164	163553	20.000	ng	0.00
64) Phenanthrene-d10	17.304	188	378207	20.000	ng	0.00
76) Chrysene-d12	21.410	240	414427	20.000	ng	-0.02
86) Perylene-d12	23.839	264	487328	20.000	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.475	112	329758	79.456	ng	0.00
7) Phenol-d6	7.075	99	428309	76.539	ng	0.00
23) Nitrobenzene-d5	9.069	82	301231	53.623	ng	0.00
42) 2,4,6-Tribromophenol	16.039	330	246406	103.186	ng	0.00
45) 2-Fluorobiphenyl	13.163	172	690712	52.208	ng	0.00
79) Terphenyl-d14	19.874	244	1469170	58.300	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019871.D
Acq On : 24 Feb 2024 20:21
Operator : MA/JU
Sample : P1564-17
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-17

Quant Time: Feb 26 00:15:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 23 13:10:49 2024
Response via : Initial Calibration




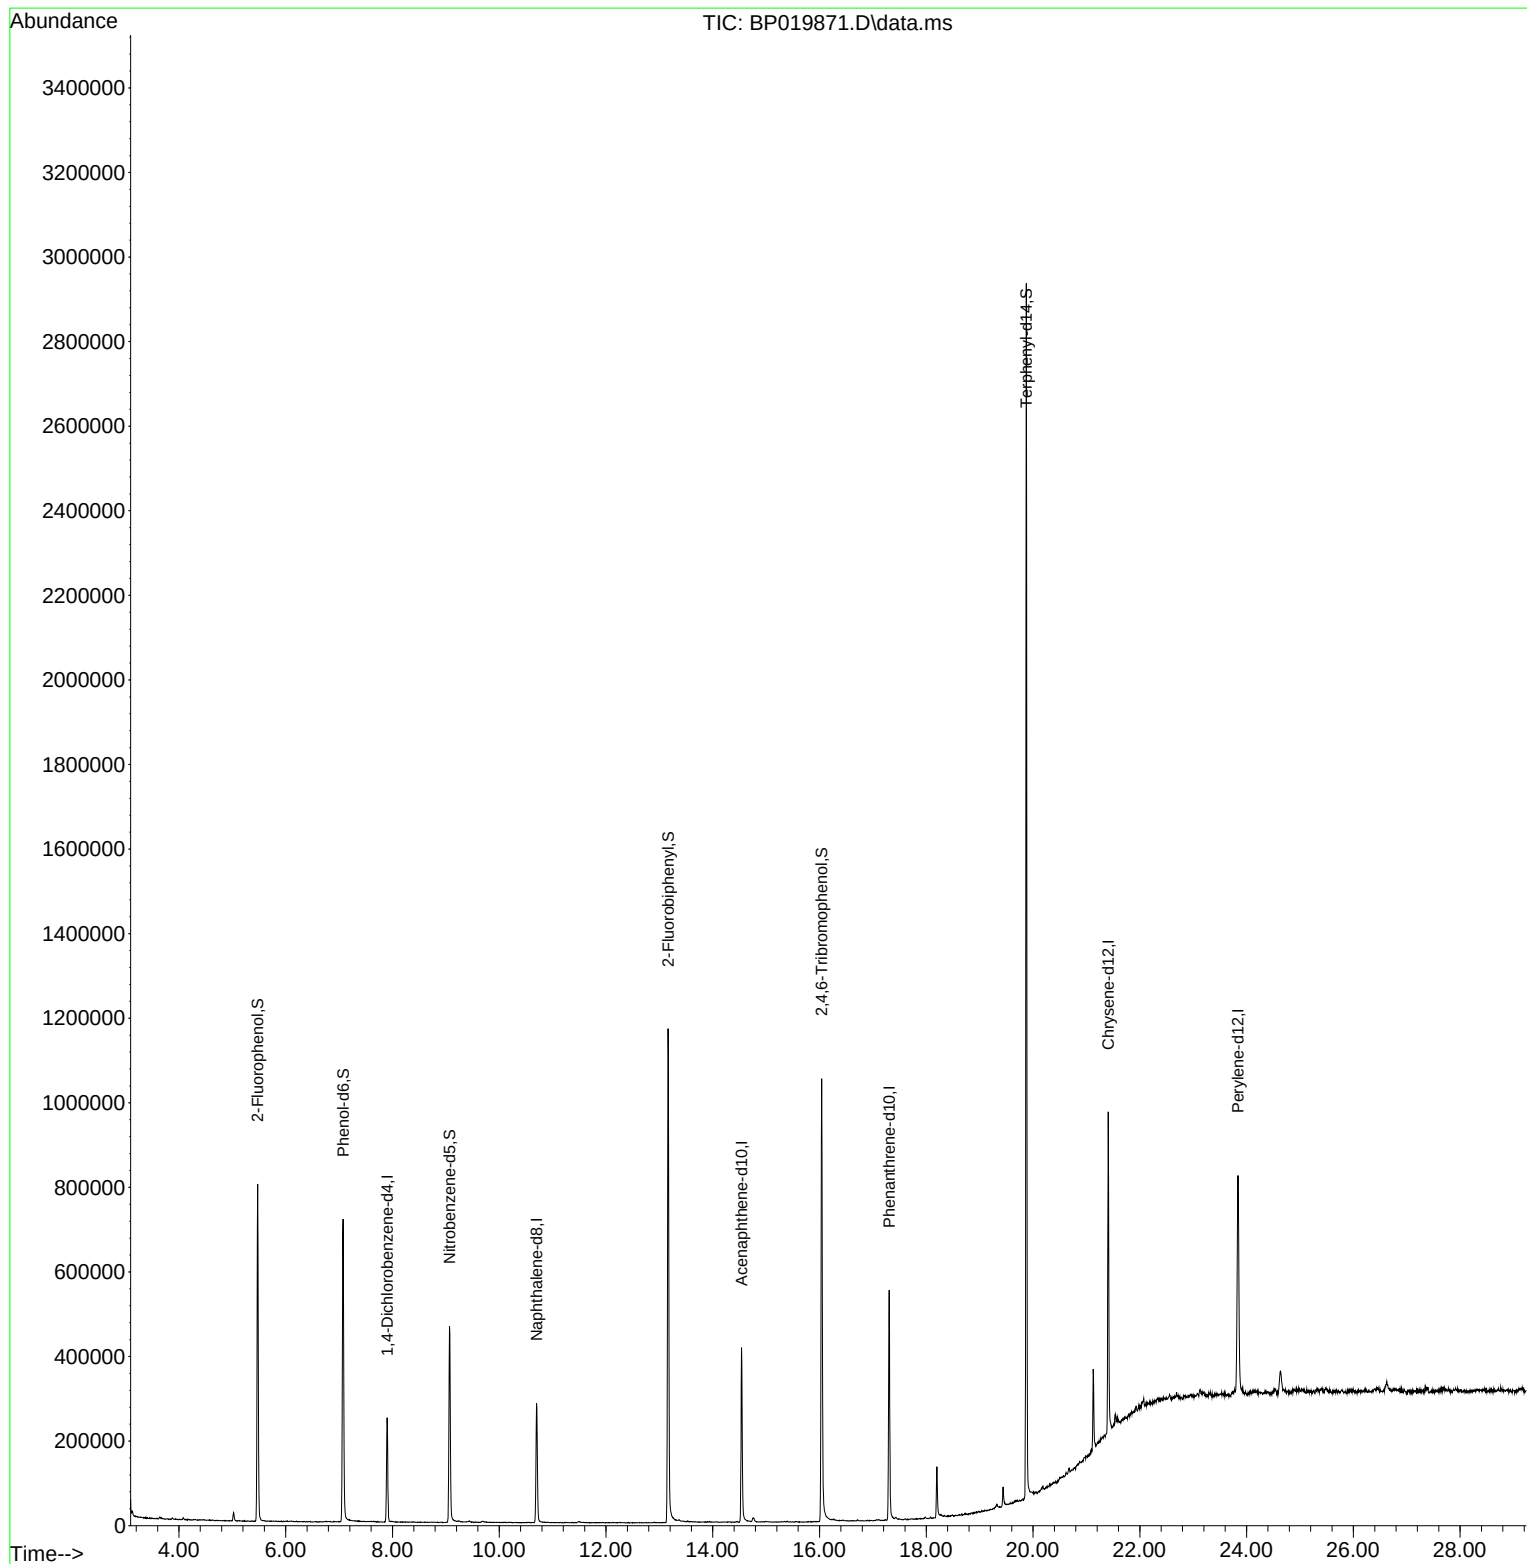




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.899 min Scan# 81
Delta R.T. -0.000 min
Lab File: BP019871.D
Acq: 24 Feb 2024 20:21




Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-17


Tgt Ion:152 Resp: 66898
Ion Ratio Lower Upper
152 100
150 158.1 121.8 182.8
115 66.7 49.9 74.9

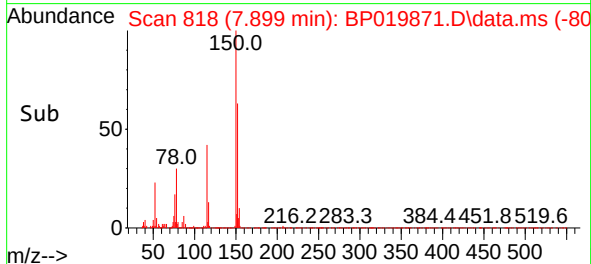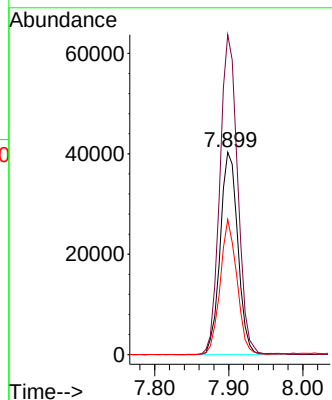

#5
2-Fluorophenol
Concen: 79.456 ng
RT: 5.475 min Scan# 406
Delta R.T. -0.000 min
Lab File: BP019871.D
Acq: 24 Feb 2024 20:21

Tgt Ion:112 Resp: 329758
Ion Ratio Lower Upper
112 100
64 59.4 47.4 71.0
63 32.8 27.0 40.6


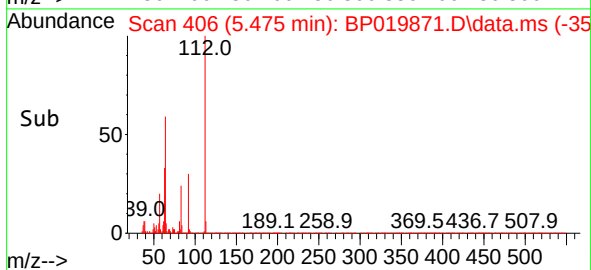
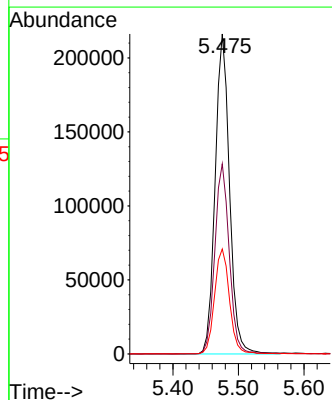
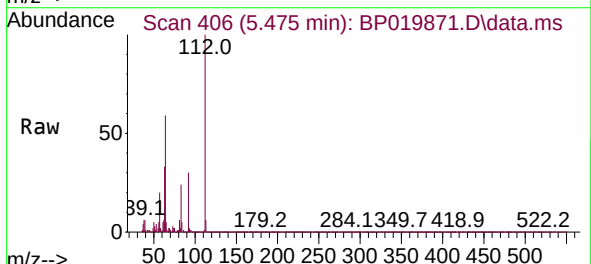




#7
Phenol-d6
Concen: 76.539 ng
RT: 7.075 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP019871.D
Acq: 24 Feb 2024 20:21




Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-17


Tgt Ion: 99 Resp: 428309
Ion Ratio Lower Upper
99 100
42 16.8 14.7 22.1
71 44.1 34.8 52.2

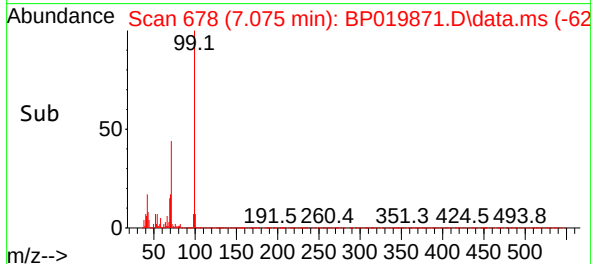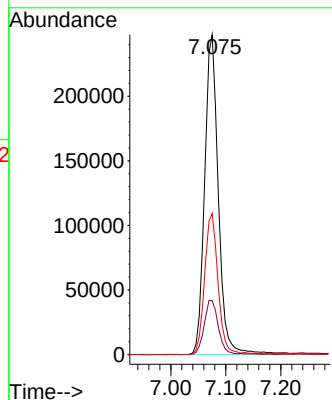

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.698 min Scan# 1294
Delta R.T. -0.006 min
Lab File: BP019871.D
Acq: 24 Feb 2024 20:21

Tgt Ion: 136 Resp: 243416
Ion Ratio Lower Upper
136 100
137 10.8 8.8 13.2
54 6.9 5.3 7.9
68 5.0 4.1 6.1


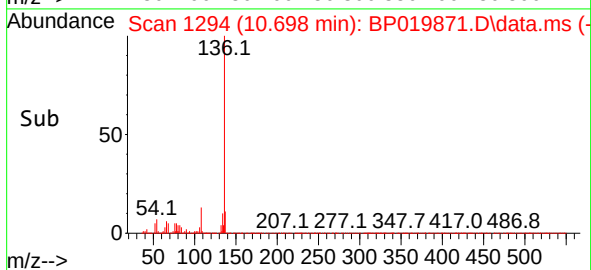
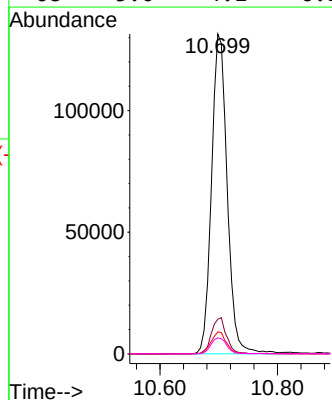
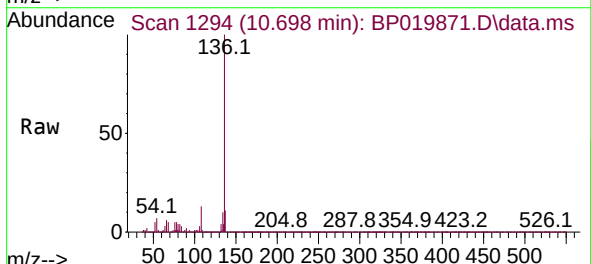




#23
Nitrobenzene-d5
Concen: 53.623 ng
RT: 9.069 min Scan# 10
Delta R.T. -0.006 min
Lab File: BP019871.D
Acq: 24 Feb 2024 20:21




Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-17


Tgt Ion: 82 Resp: 301231
Ion Ratio Lower Upper
82 100
128 38.0 29.7 44.5
54 47.2 36.8 55.2

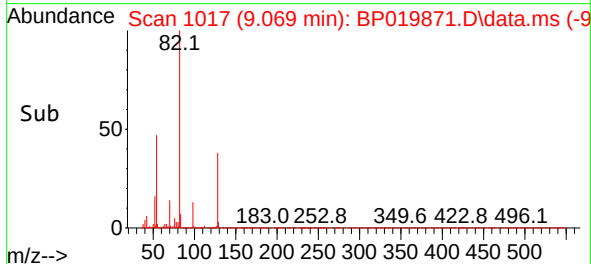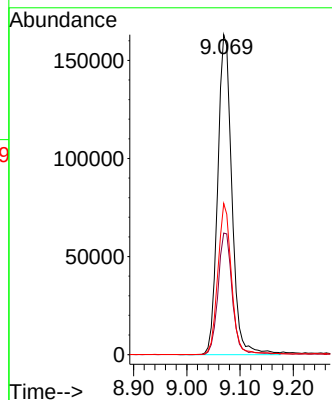

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.539 min Scan# 1947
Delta R.T. -0.006 min
Lab File: BP019871.D
Acq: 24 Feb 2024 20:21

Tgt Ion:164 Resp: 163553
Ion Ratio Lower Upper
164 100
162 99.7 81.2 121.8
160 43.8 35.1 52.7

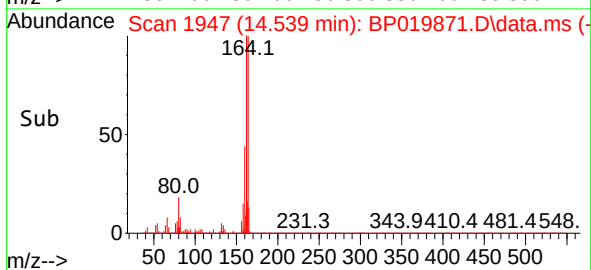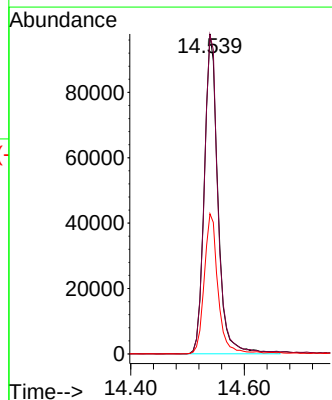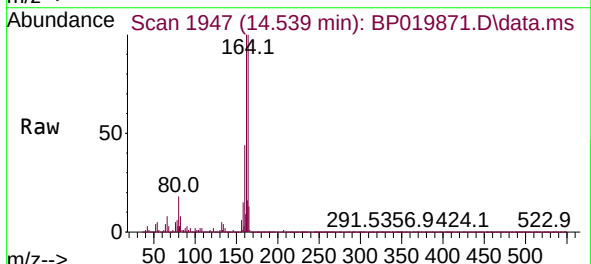

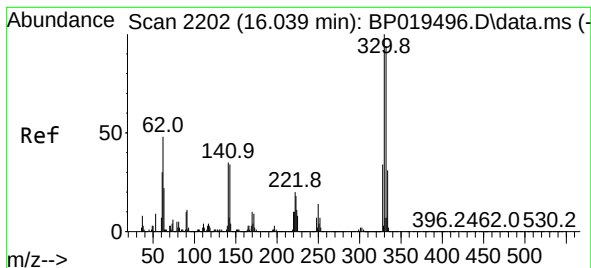

#42

2,4,6-Tribromophenol

Concen: 103.186 ng

RT: 16.039 min Scan# 21

Delta R.T. -0.006 min

Lab File: BP019871.D

Acq: 24 Feb 2024 20:21

Instrument :

BNA_P

ClientSampleId :

LKWD-BACKFILL-17





Tgt Ion:330 Resp: 246406

Ion Ratio Lower Upper

330 100

332 98.1 77.2 115.8

141 29.3 27.0 40.4

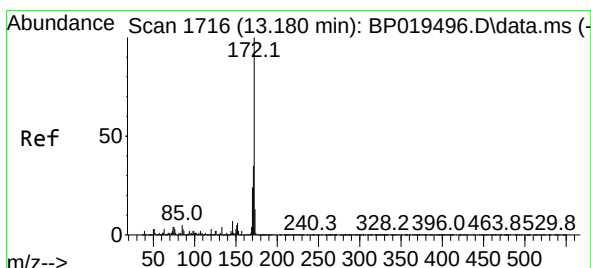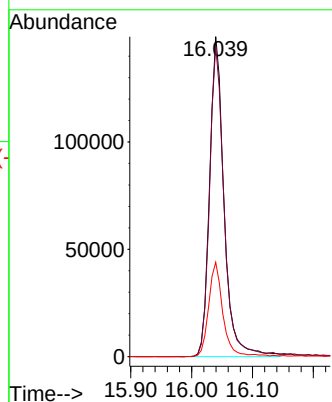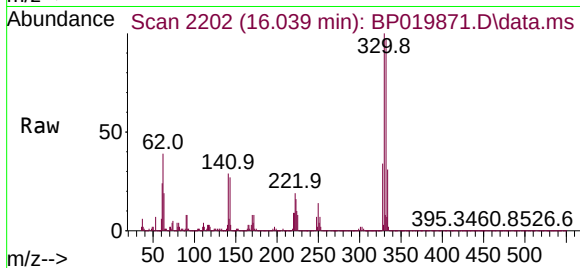

#45

2-Fluorobiphenyl

Concen: 52.208 ng

RT: 13.163 min Scan# 1713

Delta R.T. -0.006 min

Lab File: BP019871.D

Acq: 24 Feb 2024 20:21




Tgt Ion:172 Resp: 690712


Ion Ratio Lower Upper

172 100

171 34.7 28.2 42.4

170 22.8 18.9 28.3

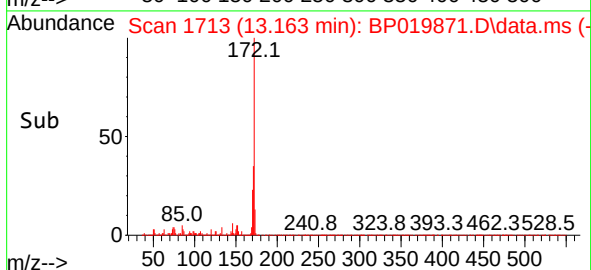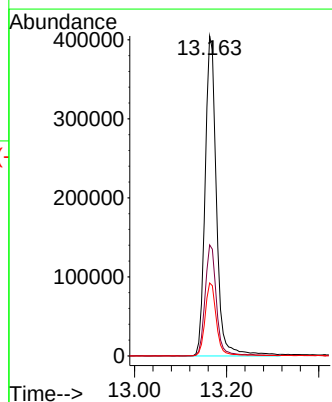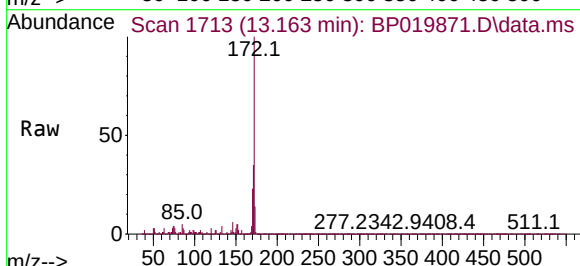

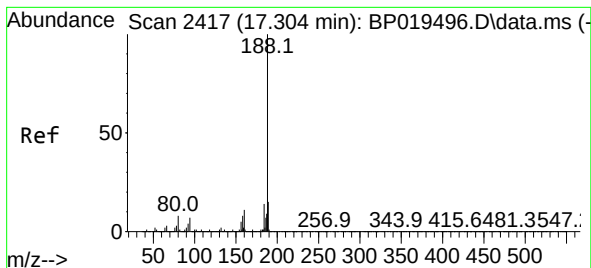

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.304 min Scan# 2417

Delta R.T. -0.006 min

Lab File: BP019871.D

Acq: 24 Feb 2024 20:21

Instrument :

BNA_P

ClientSampleId :

LKWD-BACKFILL-17





Tgt Ion:188 Resp: 378207

Ion Ratio Lower Upper

188 100

94 6.3 5.4 8.2

80 7.3 6.3 9.5

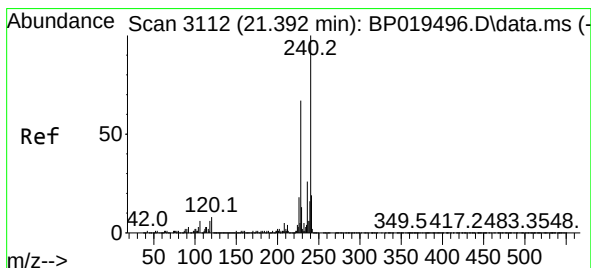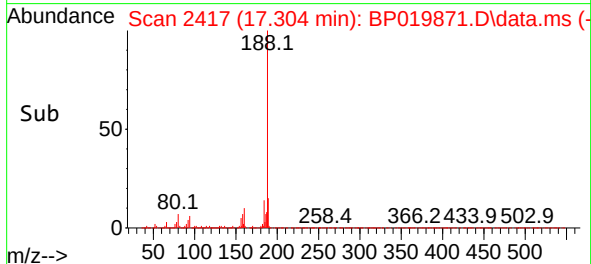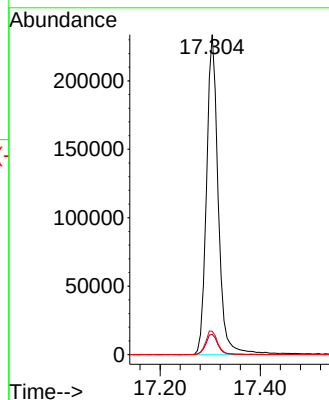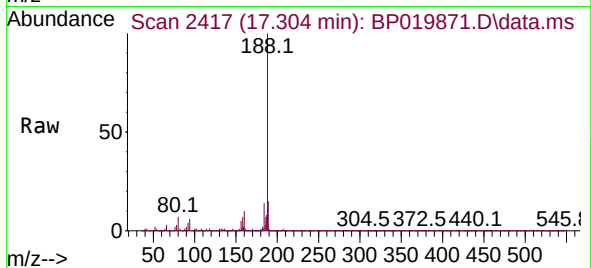

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.410 min Scan# 3115

Delta R.T. -0.018 min

Lab File: BP019871.D

Acq: 24 Feb 2024 20:21




Tgt Ion:240 Resp: 414427


Ion Ratio Lower Upper

240 100

120 6.2 6.1 9.1

236 25.5 20.7 31.1


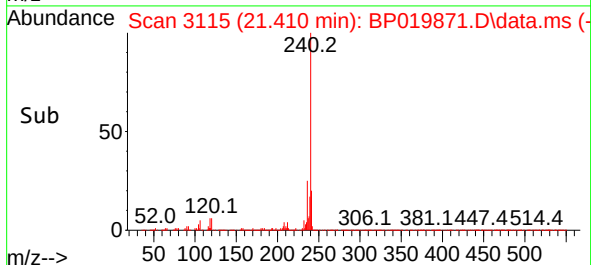
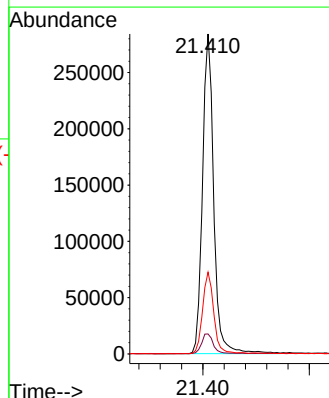
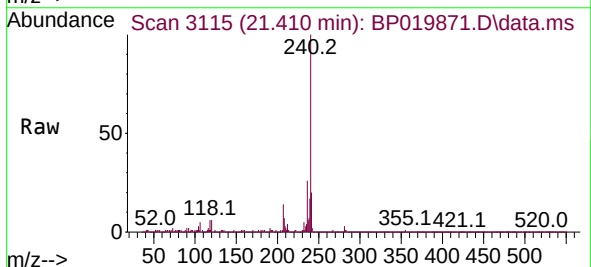




#79
 Terphenyl-d14
 Concen: 58.300 ng
 RT: 19.874 min Scan# 2854
 Delta R.T. -0.018 min
 Lab File: BP019871.D
 Acq: 24 Feb 2024 20:21

Instrument :
 BNA_P
 ClientSampleId :
 LKWD-BACKFILL-17

Tgt Ion:244 Resp: 1469170
 Ion Ratio Lower Upper
 244 100
 212 7.2 6.1 9.1
 122 6.7 5.9 8.9

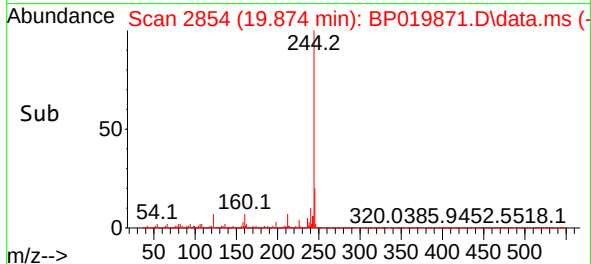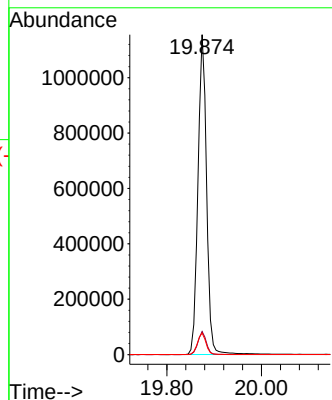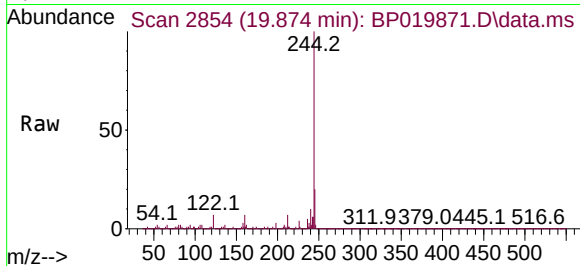

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.839 min Scan# 3528
 Delta R.T. -0.030 min
 Lab File: BP019871.D
 Acq: 24 Feb 2024 20:21

Tgt Ion:264 Resp: 487328
 Ion Ratio Lower Upper
 264 100
 260 23.4 19.2 28.8
 265 22.9 17.0 25.4

