

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
 Data File : BP019856.D
 Acq On : 24 Feb 2024 11:56
 Operator : MA/JU
 Sample : PB159229BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB159229BL

Quant Time: Feb 26 00:07:45 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 23 13:10:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.904	152	106691	20.000	ng	0.00
21) Naphthalene-d8	10.704	136	355494	20.000	ng	0.00
39) Acenaphthene-d10	14.545	164	232170	20.000	ng	0.00
64) Phenanthrene-d10	17.310	188	555060	20.000	ng	0.00
76) Chrysene-d12	21.416	240	545267	20.000	ng	-0.01
86) Perylene-d12	23.851	264	649589	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.481	112	809403	122.287	ng	0.00
7) Phenol-d6	7.081	99	1011087	113.292	ng	0.00
23) Nitrobenzene-d5	9.075	82	697634	85.035	ng	0.00
42) 2,4,6-Tribromophenol	16.045	330	501746	148.014	ng	0.00
45) 2-Fluorobiphenyl	13.169	172	1429406	76.111	ng	0.00
79) Terphenyl-d14	19.880	244	2856777	86.161	ng	-0.01


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019856.D
Acq On : 24 Feb 2024 11:56
Operator : MA/JU
Sample : PB159229BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159229BL

Quant Time: Feb 26 00:07:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 23 13:10:49 2024
Response via : Initial Calibration




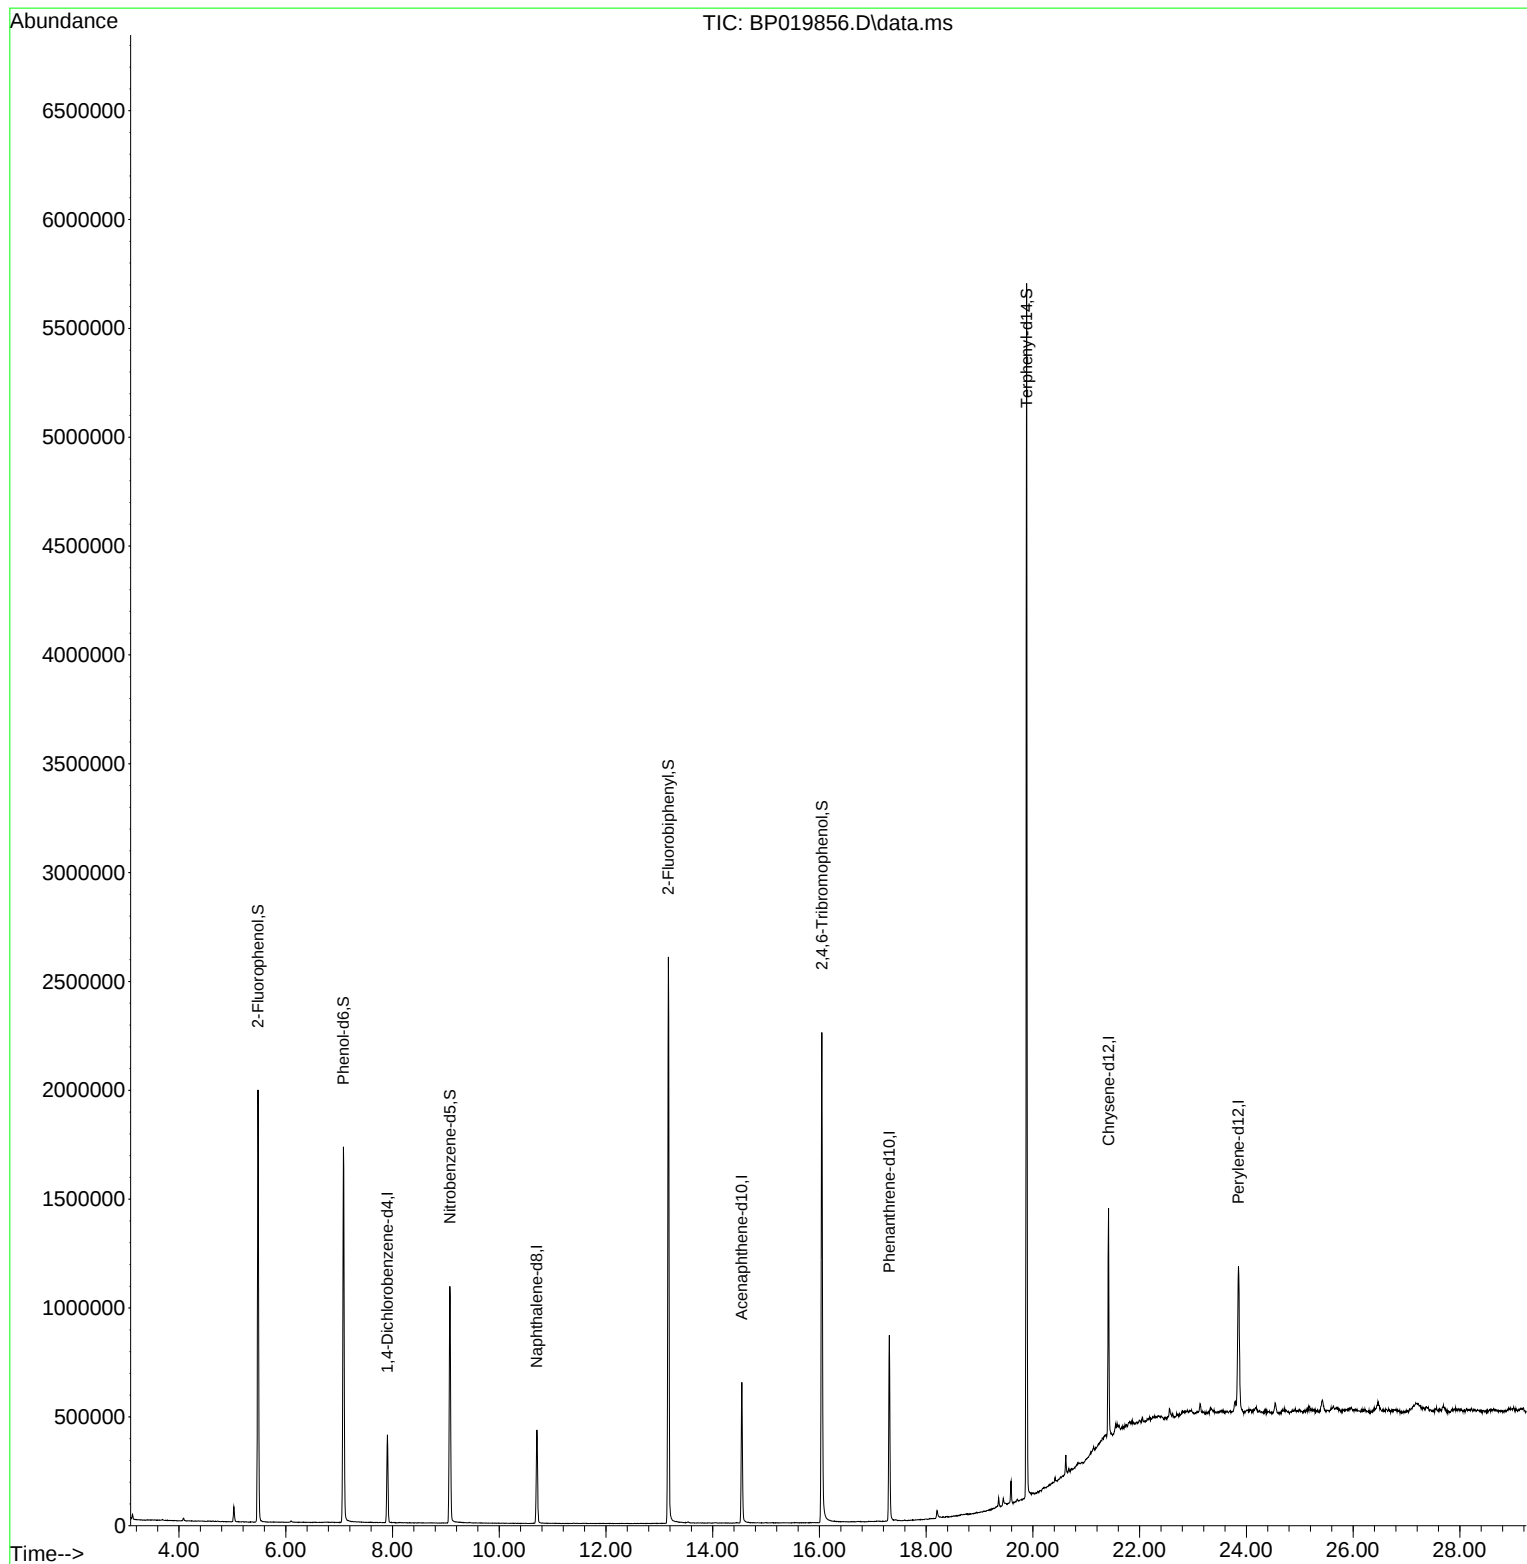


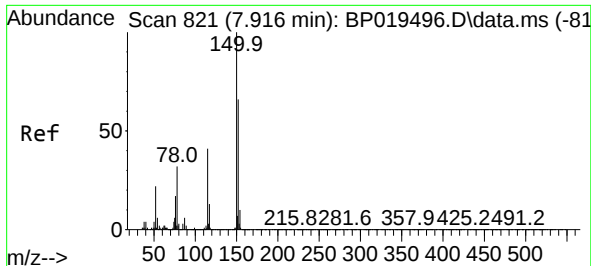

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.904 min Scan# 81
Delta R.T. 0.005 min
Lab File: BP019856.D
Acq: 24 Feb 2024 11:56




Instrument :
BNA_P
ClientSampleId :
PB159229BL

Tgt Ion:152 Resp: 106691
Ion Ratio Lower Upper
152 100
150 150.2 121.8 182.8
115 63.3 49.9 74.9

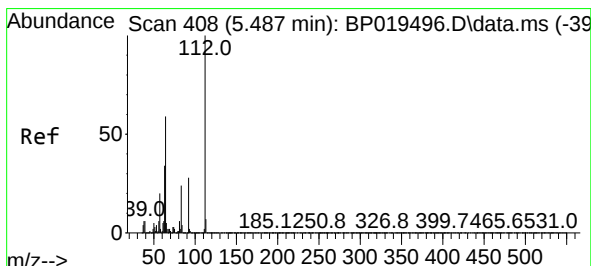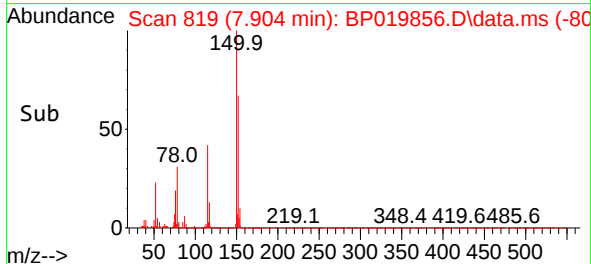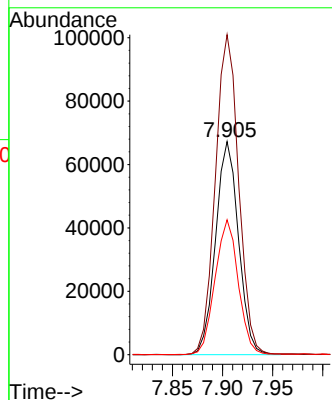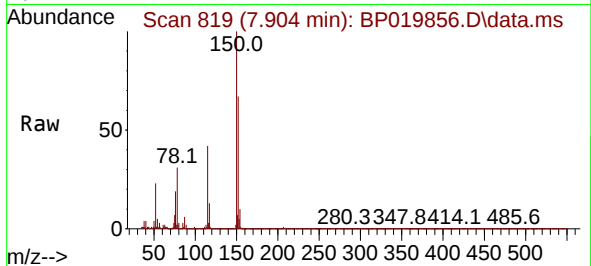

#5
2-Fluorophenol
Concen: 122.287 ng
RT: 5.481 min Scan# 407
Delta R.T. 0.006 min
Lab File: BP019856.D
Acq: 24 Feb 2024 11:56

Tgt Ion:112 Resp: 809403
Ion Ratio Lower Upper
112 100
64 61.2 47.4 71.0
63 32.9 27.0 40.6

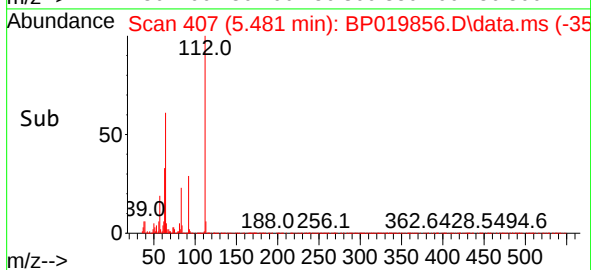
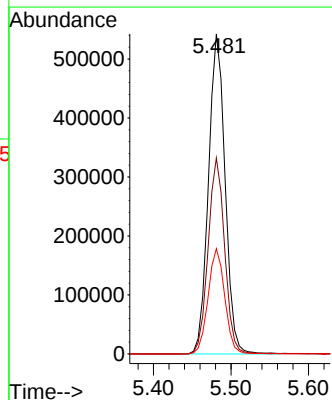
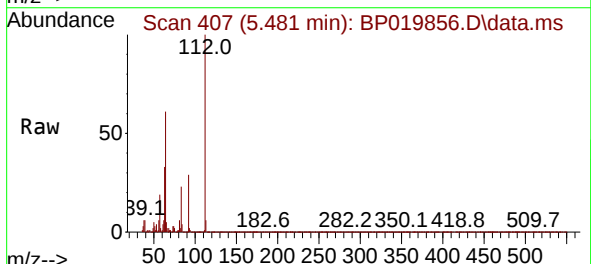




#7
Phenol-d6
Concen: 113.292 ng
RT: 7.081 min Scan# 61
Delta R.T. 0.006 min
Lab File: BP019856.D
Acq: 24 Feb 2024 11:56




Instrument :
BNA_P
ClientSampleId :
PB159229BL

Tgt Ion: 99 Resp: 1011087
Ion Ratio Lower Upper
99 100
42 17.2 14.7 22.1
71 41.6 34.8 52.2

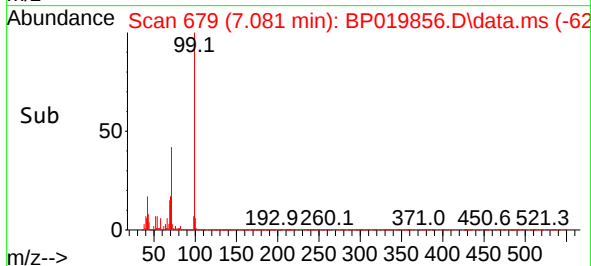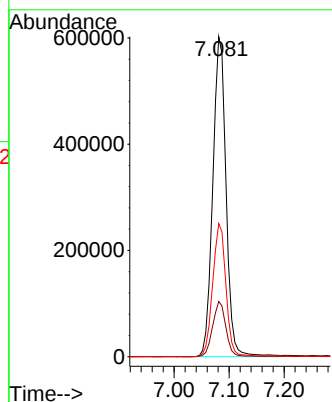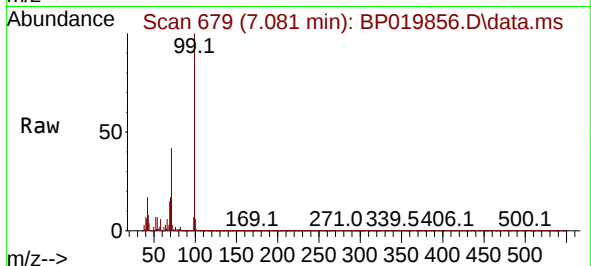

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.704 min Scan# 1295
Delta R.T. -0.000 min
Lab File: BP019856.D
Acq: 24 Feb 2024 11:56

Tgt Ion: 136 Resp: 355494
Ion Ratio Lower Upper
136 100
137 11.1 8.8 13.2
54 7.3 5.3 7.9
68 5.9 4.1 6.1


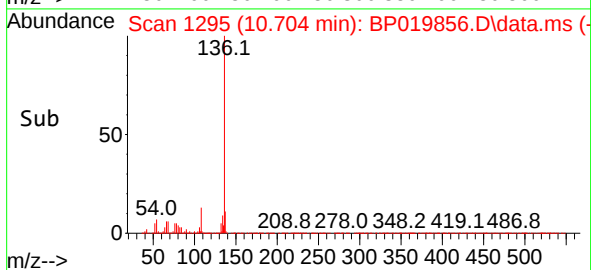
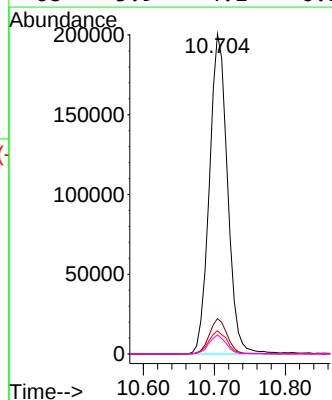
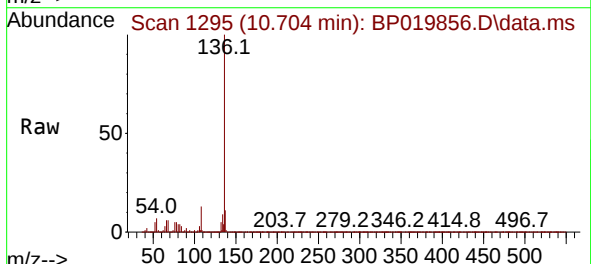




#23
Nitrobenzene-d5
Concen: 85.035 ng
RT: 9.075 min Scan# 1018
Delta R.T. -0.000 min
Lab File: BP019856.D
Acq: 24 Feb 2024 11:56




Instrument :
BNA_P
ClientSampleId :
PB159229BL


Tgt Ion: 82 Resp: 697634
Ion Ratio Lower Upper
82 100
128 37.7 29.7 44.5
54 44.9 36.8 55.2

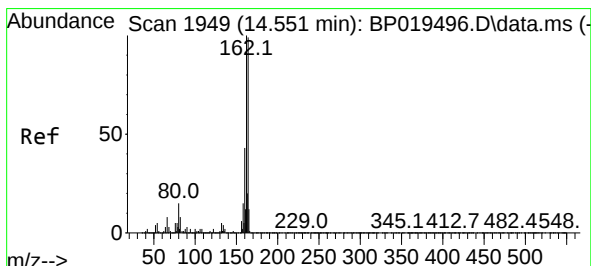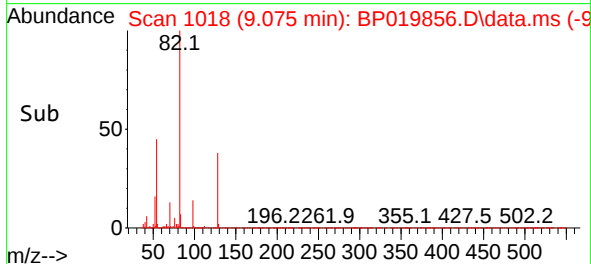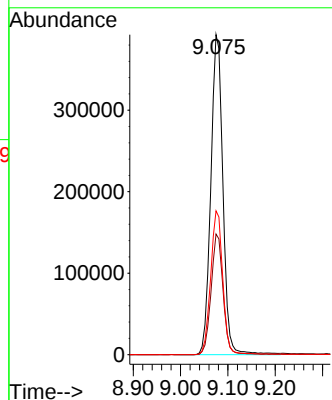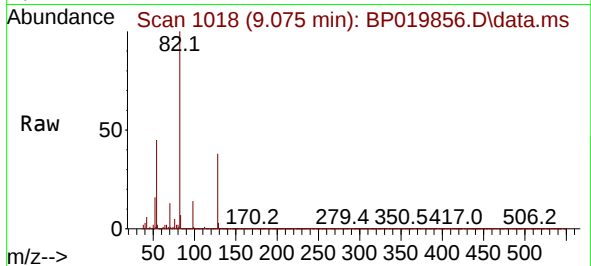

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.545 min Scan# 1948
Delta R.T. -0.000 min
Lab File: BP019856.D
Acq: 24 Feb 2024 11:56

Tgt Ion: 164 Resp: 232170
Ion Ratio Lower Upper
164 100
162 105.3 81.2 121.8
160 45.0 35.1 52.7

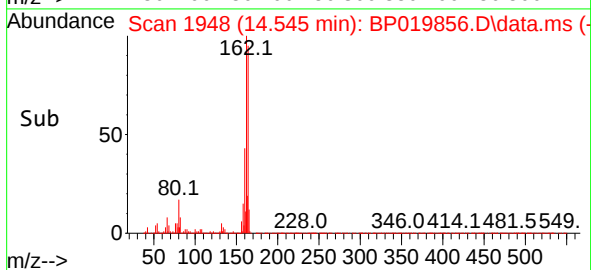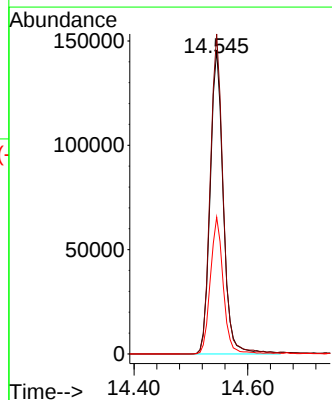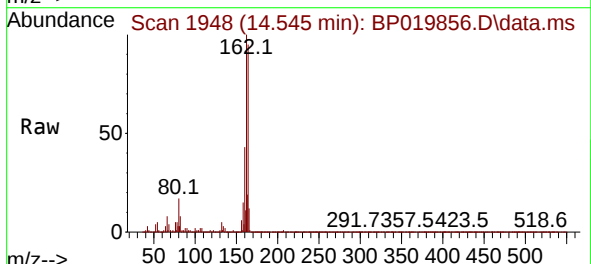

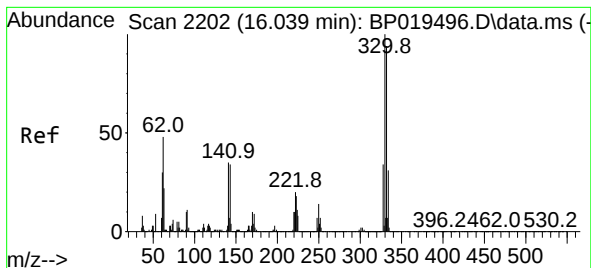

#42

2,4,6-Tribromophenol

Concen: 148.014 ng

RT: 16.045 min Scan# 21

Delta R.T. -0.000 min

Lab File: BP019856.D

Acq: 24 Feb 2024 11:56

Instrument :

BNA_P

ClientSampleId :

PB159229BL





Tgt Ion:330 Resp: 501746

Ion Ratio Lower Upper

330 100

332 96.9 77.2 115.8

141 30.0 27.0 40.4

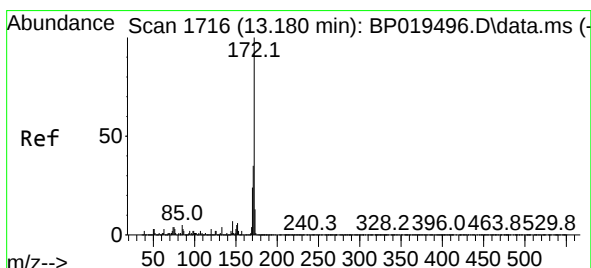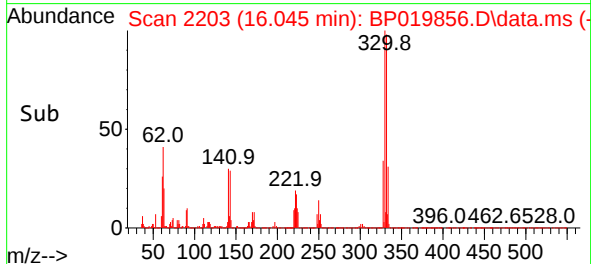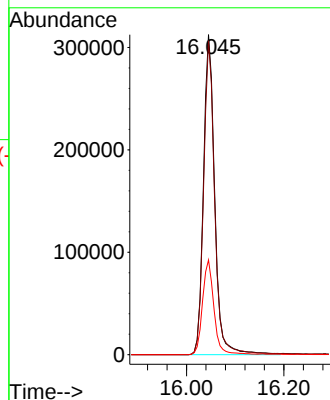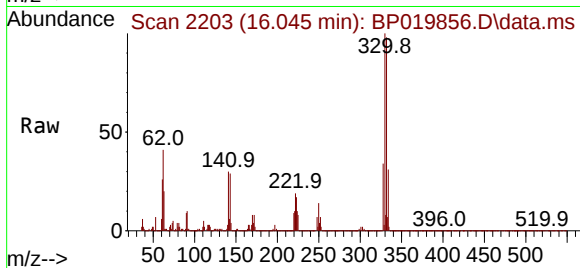

#45

2-Fluorobiphenyl

Concen: 76.111 ng

RT: 13.169 min Scan# 1714

Delta R.T. -0.000 min

Lab File: BP019856.D

Acq: 24 Feb 2024 11:56




Tgt Ion:172 Resp: 1429406


Ion Ratio Lower Upper

172 100

171 34.9 28.2 42.4

170 23.2 18.9 28.3

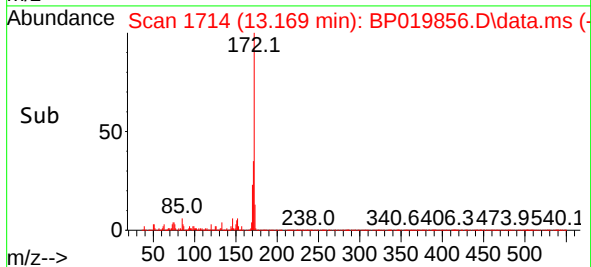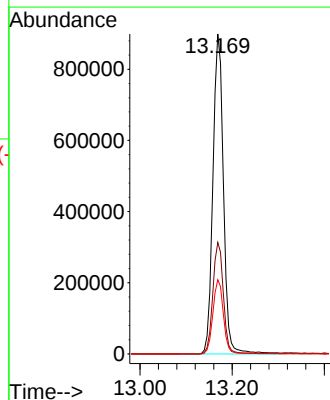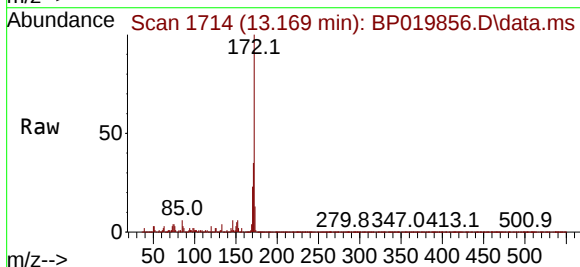

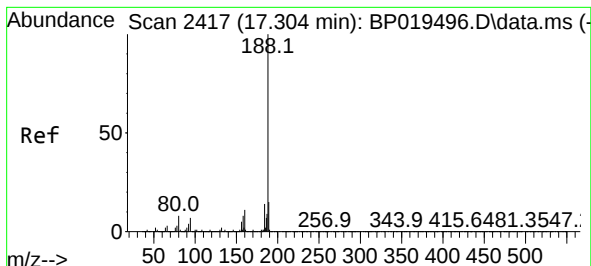

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.310 min Scan# 2417

Delta R.T. -0.000 min

Lab File: BP019856.D

Acq: 24 Feb 2024 11:56

Instrument :

BNA_P

ClientSampleId :

PB159229BL





Tgt Ion:188 Resp: 555060

Ion Ratio Lower Upper

188 100

94 7.4 5.4 8.2

80 8.6 6.3 9.5

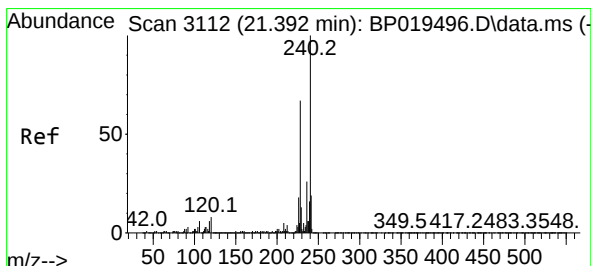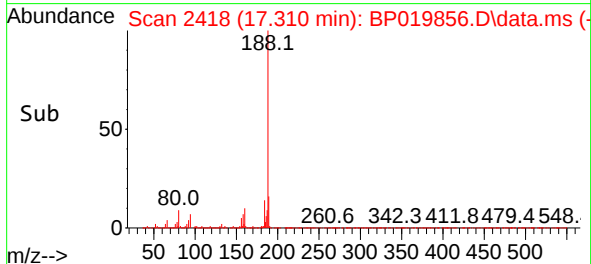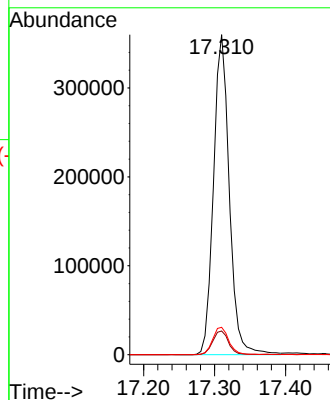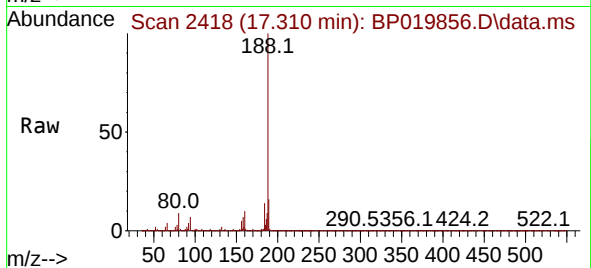

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.416 min Scan# 3116

Delta R.T. -0.012 min

Lab File: BP019856.D

Acq: 24 Feb 2024 11:56




Tgt Ion:240 Resp: 545267

Ion Ratio Lower Upper

240 100

120 6.8 6.1 9.1

236 25.3 20.7 31.1

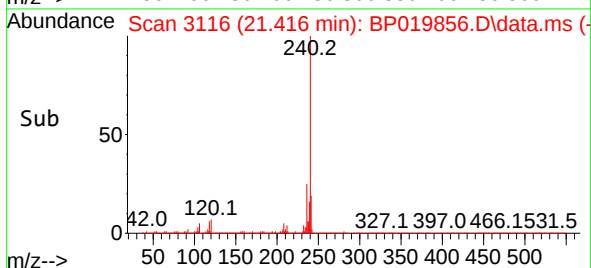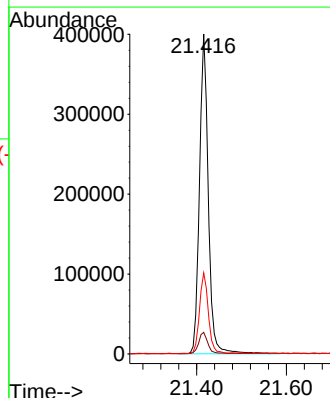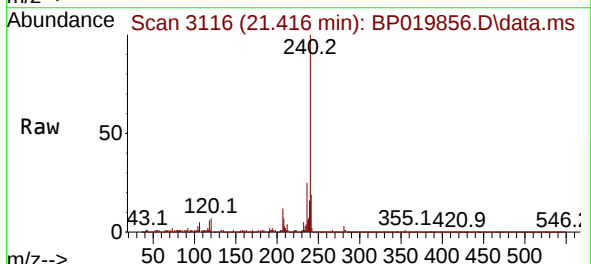



#79

Terphenyl-d14

Concen: 86.161 ng

RT: 19.880 min Scan# 21

Delta R.T. -0.012 min

Lab File: BP019856.D

Acq: 24 Feb 2024 11:56

Instrument :

BNA_P

ClientSampleId :

PB159229BL





Tgt Ion:244 Resp: 2856777

Ion Ratio Lower Upper

244 100

212 7.3 6.1 9.1

122 7.3 5.9 8.9

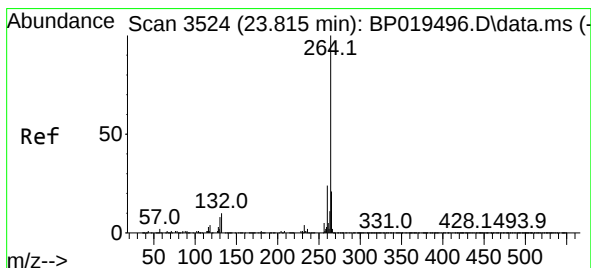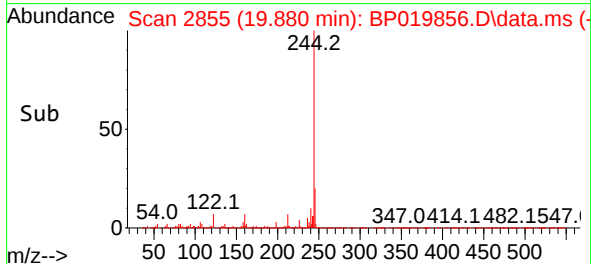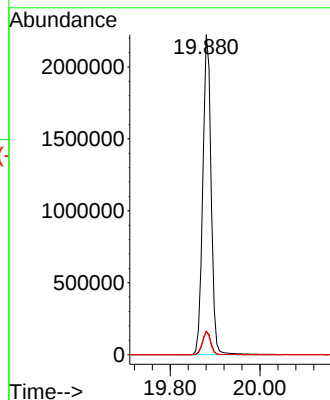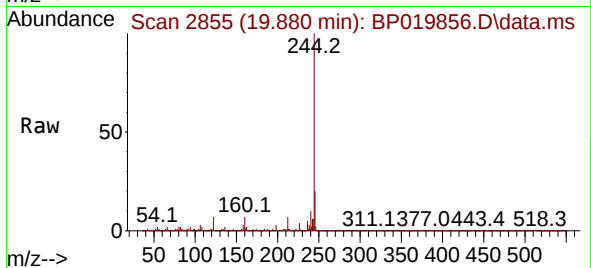

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.851 min Scan# 3530

Delta R.T. -0.018 min

Lab File: BP019856.D

Acq: 24 Feb 2024 11:56

Tgt Ion:264 Resp: 649589

Ion Ratio Lower Upper

264 100

260 22.7 19.2 28.8

265 21.6 17.0 25.4

