

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019856.D
Acq On : 24 Feb 2024 11:56
Operator : MA/JU
Sample : PB159229BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159229BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP019856.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.028	325	330	340	rVB	69457	101985	1.44%	0.342%
2	5.481	400	407	422	rBV	1983873	2956632	41.63%	9.905%
3	7.081	670	679	700	rBV	1726023	2935156	41.33%	9.833%
4	7.905	812	819	828	rBV	403367	643061	9.05%	2.154%
5	9.075	1010	1018	1037	rBV	1087334	1937119	27.27%	6.489%
6	10.704	1288	1295	1310	rBV	429223	760344	10.71%	2.547%
7	13.169	1706	1714	1737	rBV	2602181	4161976	58.60%	13.943%
8	14.545	1940	1948	1966	rBV	646412	1037924	14.61%	3.477%
9	16.045	2193	2203	2228	rBV	2252457	3700418	52.10%	12.396%
10	17.310	2411	2418	2430	rBV	853004	1319527	18.58%	4.420%
11	18.204	2565	2570	2578	rBV4	36738	72893	1.03%	0.244%
12	19.592	2802	2806	2812	rVB	104246	129288	1.82%	0.433%
13	19.880	2850	2855	2864	rBV	5571711	7102455	100.00%	23.793%
14	20.616	2977	2980	2986	rVB3	82722	91980	1.30%	0.308%
15	21.416	3111	3116	3124	rBV	1041480	1392462	19.61%	4.665%
16	23.851	3524	3530	3542	rVB	661134	1507477	21.22%	5.050%




Sum of corrected areas: 29850697

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019856.D
Acq On : 24 Feb 2024 11:56
Operator : MA/JU
Sample : PB159229BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159229BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

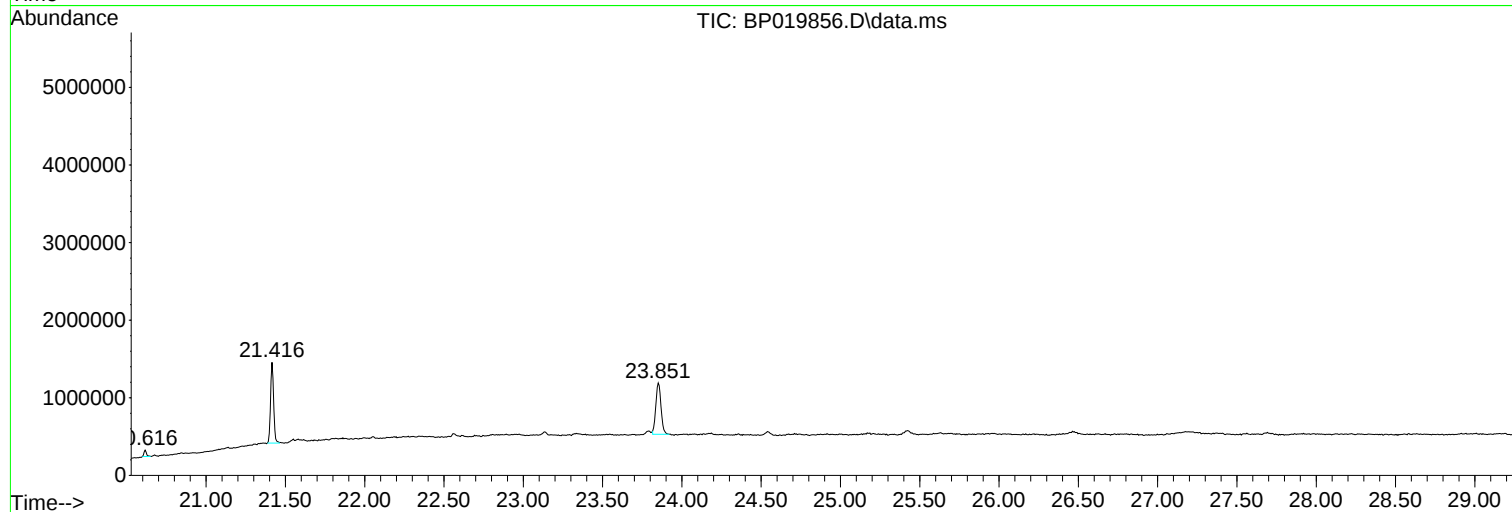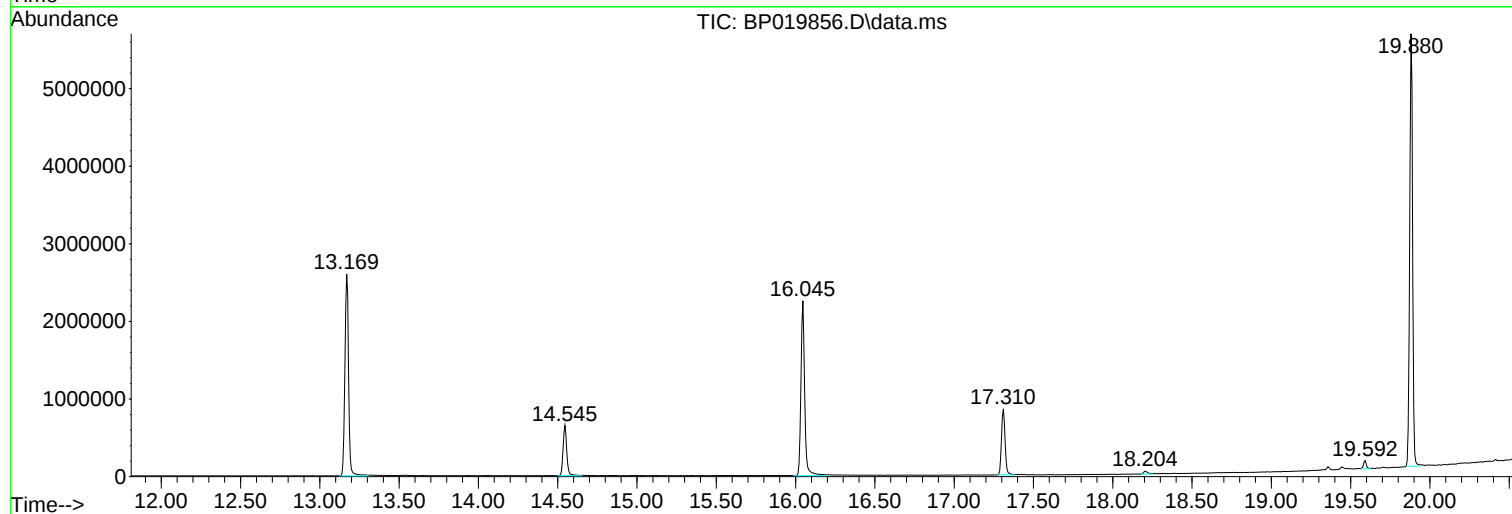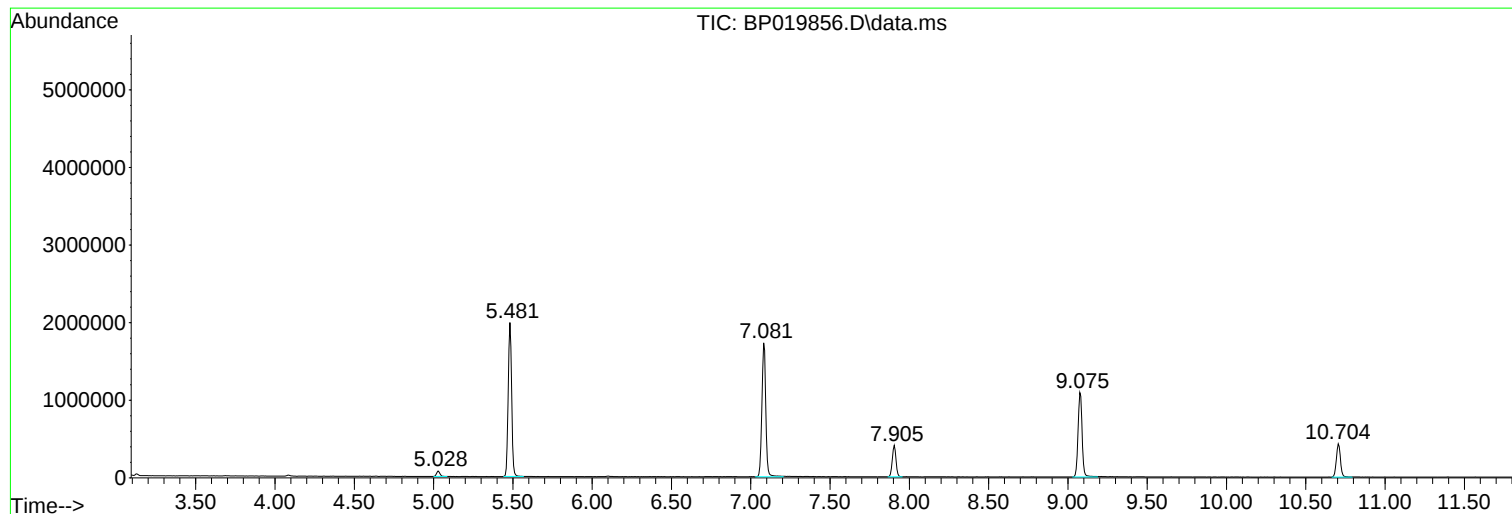

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019856.D
Acq On : 24 Feb 2024 11:56
Operator : MA/JU
Sample : PB159229BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159229BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019856.D
Acq On : 24 Feb 2024 11:56
Operator : MA/JU
Sample : PB159229BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159229BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------