

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019858.D
Acq On : 24 Feb 2024 13:03
Operator : MA/JU
Sample : PB159213BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159213BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP019858.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.481	400	407	422	rBV	1440438	2182059	39.99%	10.263%
2	7.081	671	679	692	rBV	1193147	1989312	36.46%	9.356%
3	7.904	812	819	830	rBV	268411	430610	7.89%	2.025%
4	9.075	1007	1018	1032	rBV	793080	1391180	25.50%	6.543%
5	10.704	1287	1295	1307	rBV	314920	547502	10.03%	2.575%
6	13.169	1707	1714	1737	rBV	2070440	3162518	57.96%	14.874%
7	14.545	1941	1948	1964	rBV	455457	756330	13.86%	3.557%
8	16.045	2196	2203	2230	rBV	1459179	2467526	45.23%	11.605%
9	17.310	2411	2418	2431	rBV	555078	896033	16.42%	4.214%
10	19.880	2849	2855	2867	rBV	4289349	5456109	100.00%	25.662%
11	21.416	3111	3116	3126	rBV	663445	997393	18.28%	4.691%
12	23.851	3524	3530	3542	rVB	421099	985227	18.06%	4.634%




Sum of corrected areas: 21261799

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019858.D
Acq On : 24 Feb 2024 13:03
Operator : MA/JU
Sample : PB159213BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159213BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

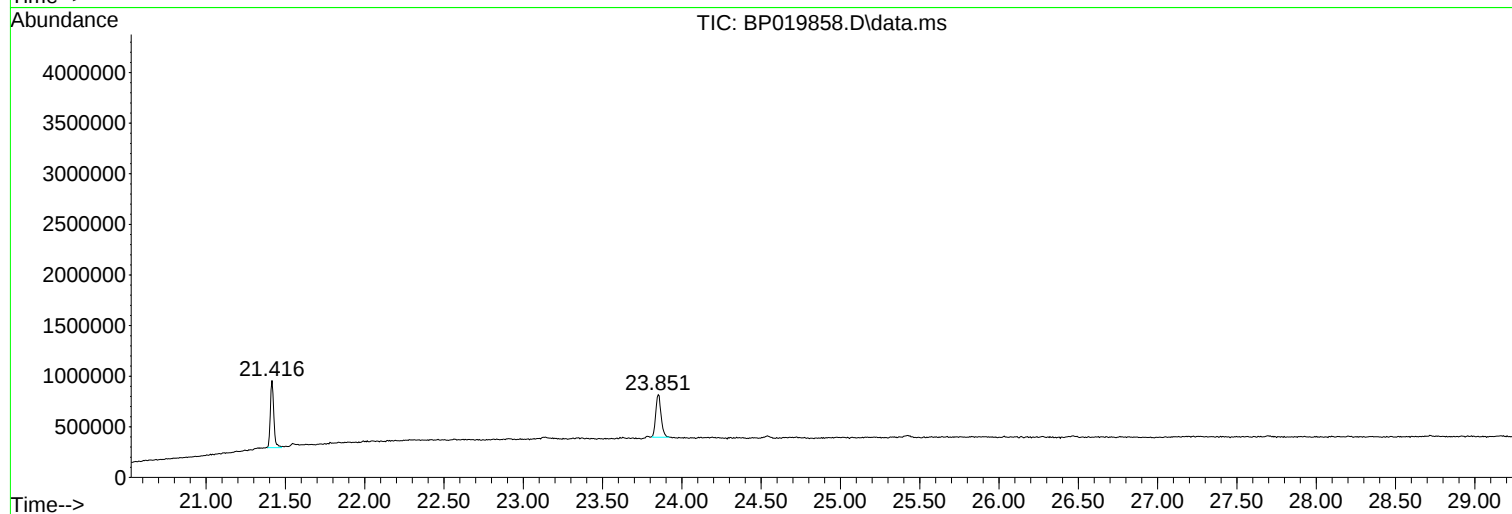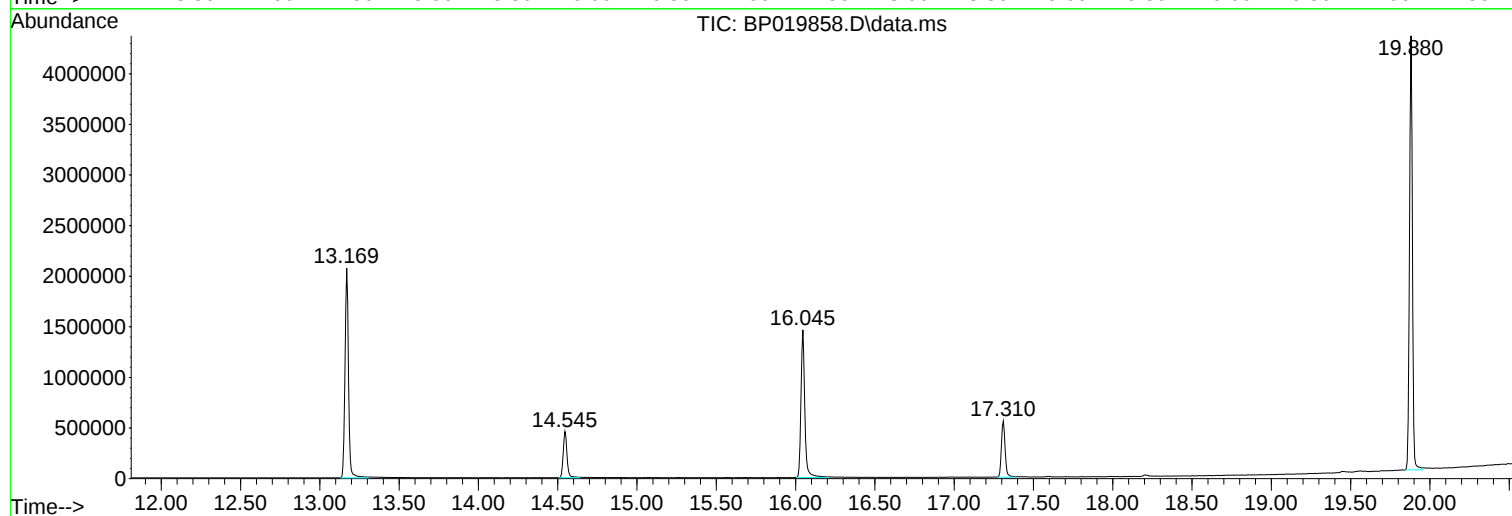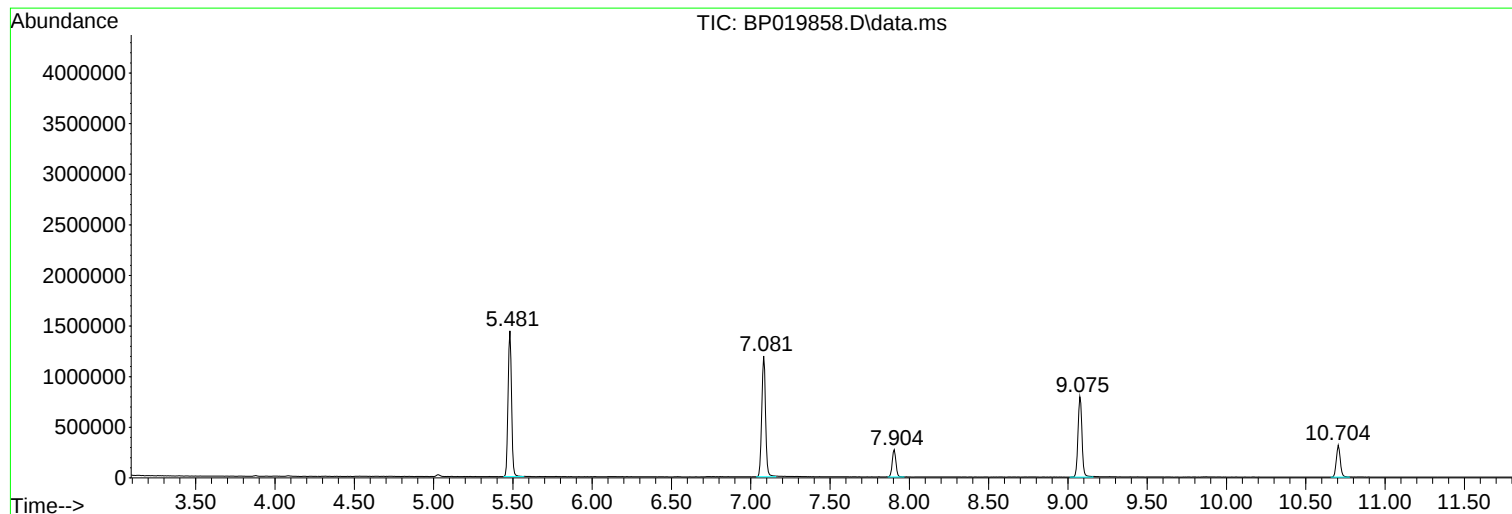

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019858.D
Acq On : 24 Feb 2024 13:03
Operator : MA/JU
Sample : PB159213BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159213BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019858.D
Acq On : 24 Feb 2024 13:03
Operator : MA/JU
Sample : PB159213BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159213BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------