

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
 Data File : BP019861.D
 Acq On : 24 Feb 2024 14:44
 Operator : MA/JU
 Sample : P1564-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 LKWD-BACKFILL-09

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP019861.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	39	rVB	35909	54746	1.63%	0.348%
2	5.022	324	329	335	rVB	39197	55114	1.64%	0.350%
3	5.475	399	406	421	rBV	721169	1108796	33.03%	7.043%
4	7.075	671	678	690	rBV	865834	1499157	44.66%	9.523%
5	7.905	811	819	826	rBV	324842	542081	16.15%	3.443%
6	9.075	1010	1018	1036	rBV	539686	981904	29.25%	6.237%
7	10.704	1287	1295	1306	rBV	293376	522400	15.56%	3.318%
8	13.169	1706	1714	1734	rBV	1096766	1809575	53.91%	11.495%
9	14.545	1941	1948	1964	rBV	409123	705824	21.03%	4.484%
10	16.045	2195	2203	2222	rBV	913242	1587758	47.30%	10.086%
11	17.304	2410	2417	2430	rBV	540569	909001	27.08%	5.774%
12	18.198	2565	2569	2579	rBV2	64140	104500	3.11%	0.664%
13	19.439	2777	2780	2784	rBV4	29361	41264	1.23%	0.262%
14	19.874	2849	2854	2866	rBV	2512452	3356687	100.00%	21.322%
15	21.133	3064	3068	3074	rBV	178322	241509	7.19%	1.534%
16	21.410	3111	3115	3126	rBV	765655	1096327	32.66%	6.964%
17	23.845	3523	3529	3539	rVB	527024	1126009	33.55%	7.153%




Sum of corrected areas: 15742652

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019861.D
Acq On : 24 Feb 2024 14:44
Operator : MA/JU
Sample : P1564-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

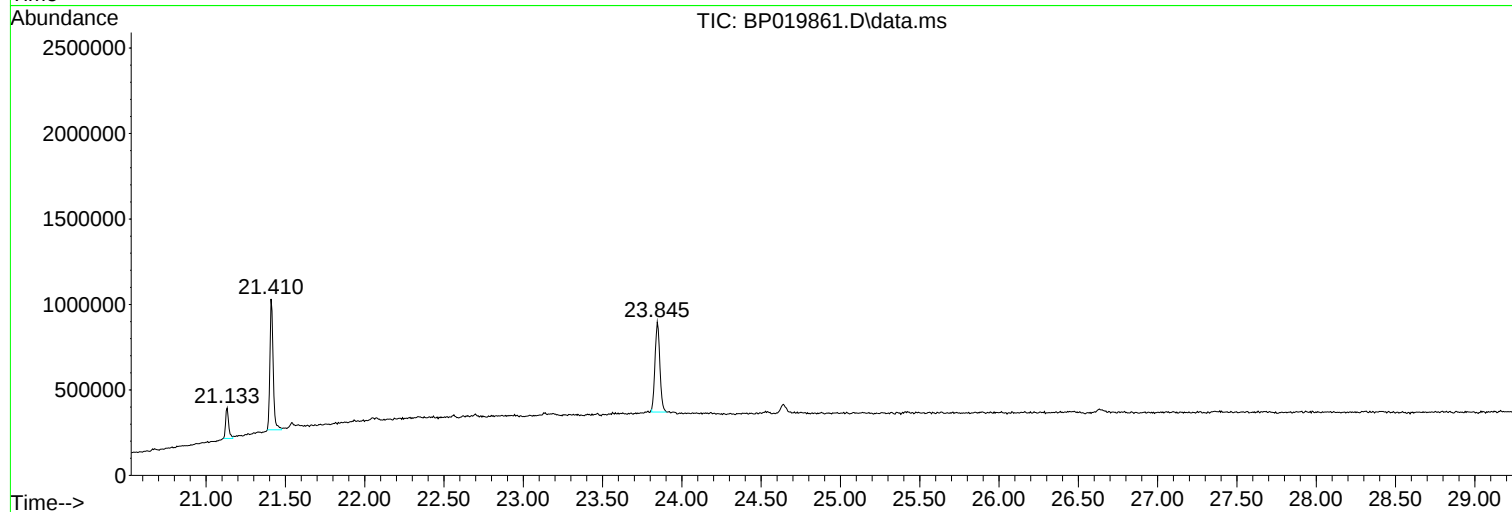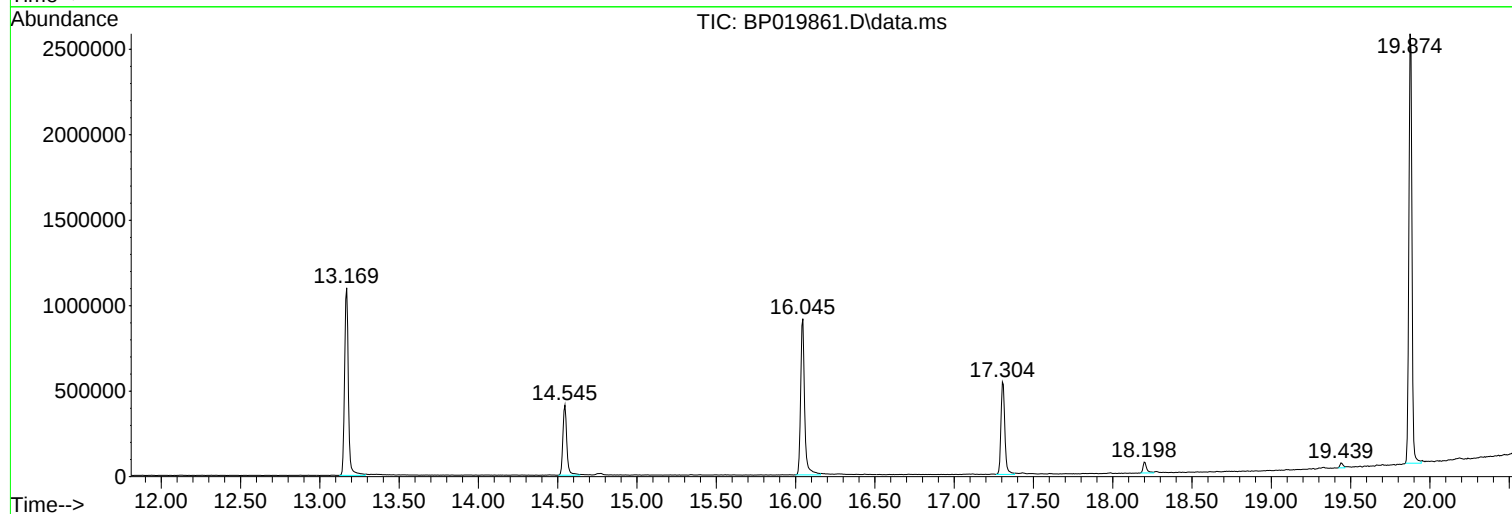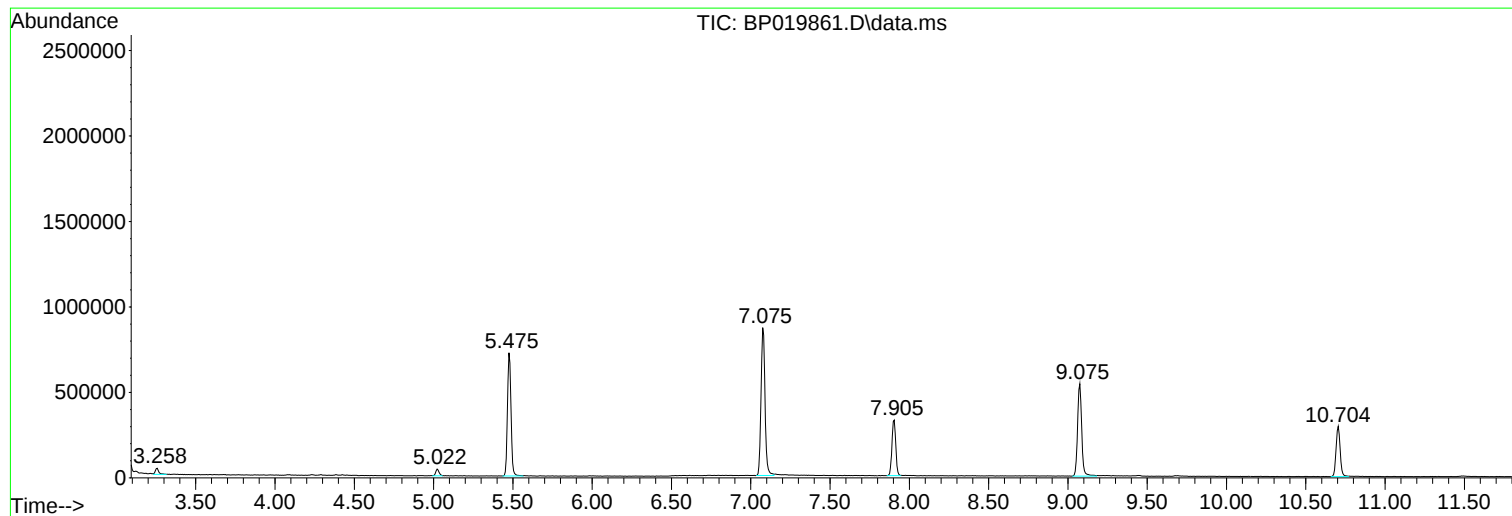

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019861.D
Acq On : 24 Feb 2024 14:44
Operator : MA/JU
Sample : P1564-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019861.D
Acq On : 24 Feb 2024 14:44
Operator : MA/JU
Sample : P1564-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------