

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
 Data File : BP019862.D
 Acq On : 24 Feb 2024 15:18
 Operator : MA/JU
 Sample : P1564-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 LKWD-BACKFILL-10

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP019862.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.475	400	406	421	rBV	717621	1111190	28.06%	7.343%
2	7.075	670	678	697	rBV	630162	1123480	28.37%	7.425%
3	7.905	811	819	826	rBV	235177	393746	9.94%	2.602%
4	9.075	1008	1018	1031	rBV	423600	754470	19.05%	4.986%
5	10.705	1286	1295	1310	rBV	269927	502562	12.69%	3.321%
6	13.169	1706	1714	1728	rBV	1025299	1732014	43.74%	11.446%
7	14.546	1941	1948	1962	rBV	375596	644731	16.28%	4.261%
8	16.045	2195	2203	2221	rBV	872681	1566224	39.55%	10.351%
9	17.304	2411	2417	2433	rBV	500457	838999	21.19%	5.545%
10	18.198	2564	2569	2577	rBV	106953	169380	4.28%	1.119%
11	19.439	2777	2780	2787	rBV3	37911	57352	1.45%	0.379%
12	19.792	2834	2840	2843	rBV8	21836	56347	1.42%	0.372%
13	19.875	2849	2854	2867	rBV	2976963	3959958	100.00%	26.170%
14	21.133	3064	3068	3072	rBV	163372	208016	5.25%	1.375%
15	21.410	3110	3115	3128	rBV	661515	1002917	25.33%	6.628%
16	23.845	3523	3529	3539	rVB	469324	1010236	25.51%	6.676%




Sum of corrected areas: 15131622

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019862.D
Acq On : 24 Feb 2024 15:18
Operator : MA/JU
Sample : P1564-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

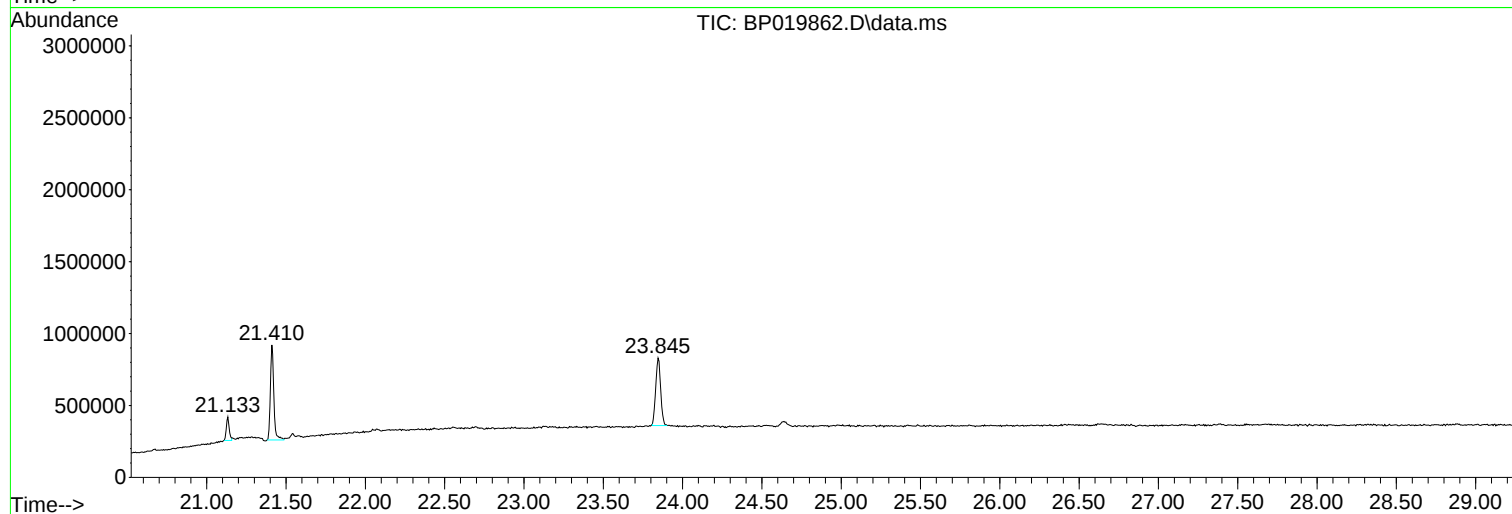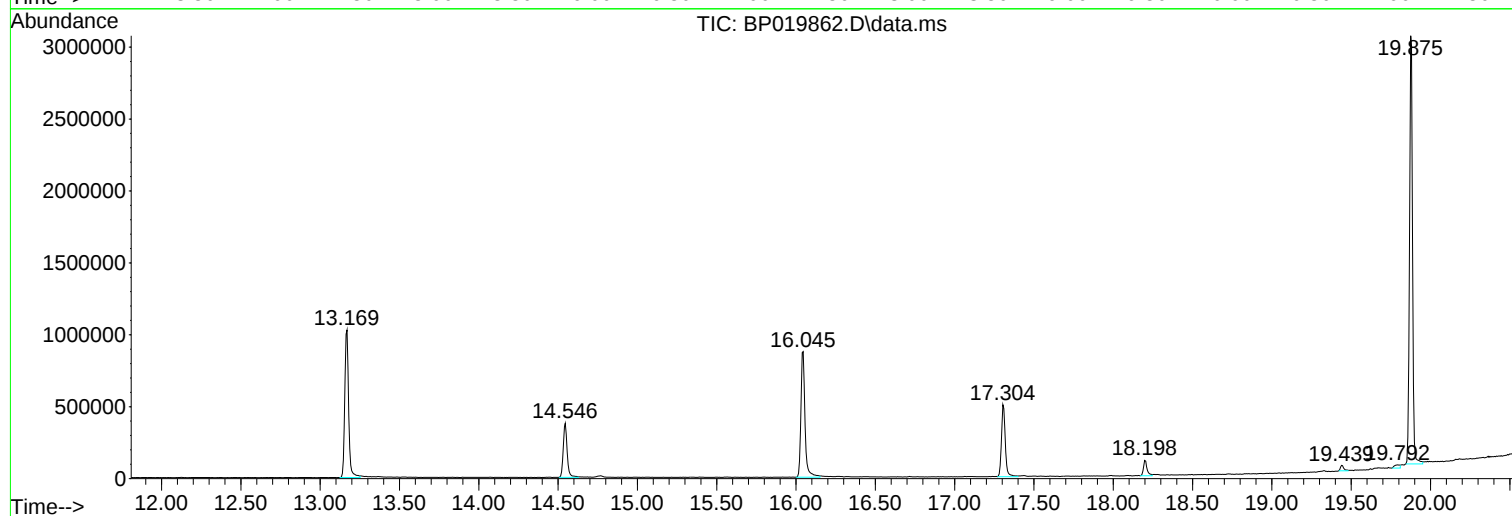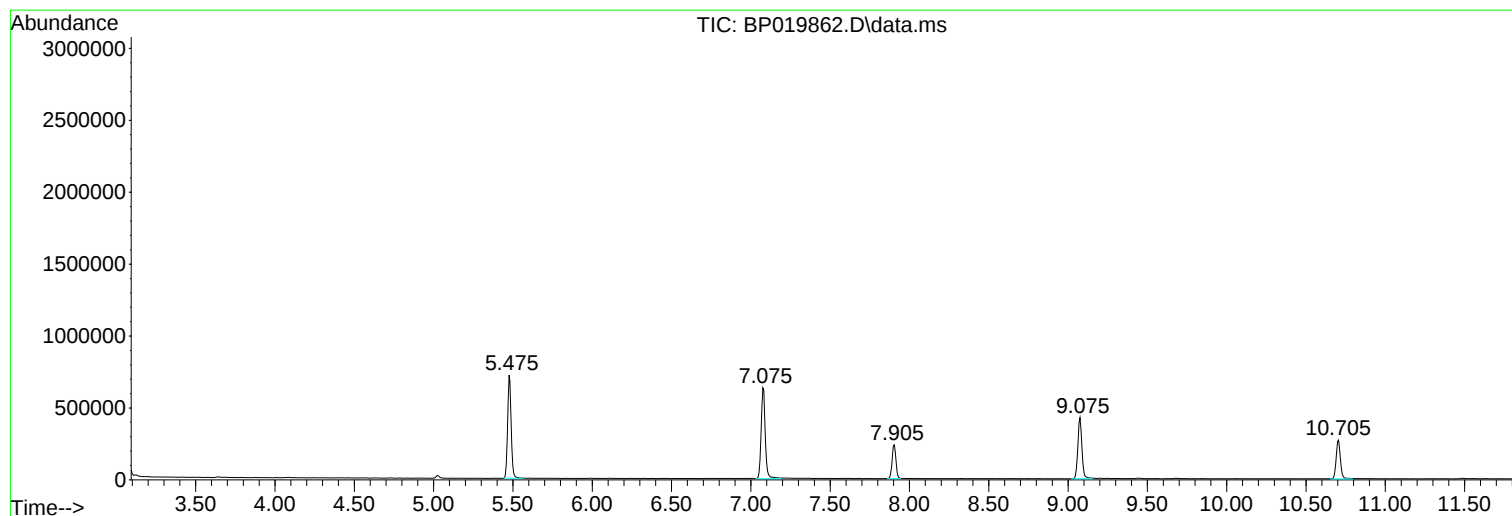

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019862.D
Acq On : 24 Feb 2024 15:18
Operator : MA/JU
Sample : P1564-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019862.D
Acq On : 24 Feb 2024 15:18
Operator : MA/JU
Sample : P1564-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------