

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
 Data File : BP019865.D
 Acq On : 24 Feb 2024 16:59
 Operator : MA/JU
 Sample : P1564-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 LKWD-BACKFILL-11

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP019865.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.028	325	330	336	rVB	24011	36181	1.14%	0.230%
2	5.475	399	406	415	rBV	887132	1339934	42.14%	8.509%
3	7.075	671	678	698	rBV	885879	1483202	46.64%	9.419%
4	7.899	811	818	828	rBV	313265	510150	16.04%	3.240%
5	9.069	1008	1017	1030	rBV	486240	879185	27.65%	5.583%
6	10.704	1286	1295	1309	rBV	310625	561439	17.65%	3.565%
7	13.169	1706	1714	1730	rBV	1157310	1943157	61.10%	12.340%
8	14.539	1941	1947	1962	rBV	397174	699950	22.01%	4.445%
9	16.039	2195	2202	2227	rBV	906670	1629340	51.24%	10.347%
10	17.304	2410	2417	2429	rBV	522266	853199	26.83%	5.418%
11	18.198	2565	2569	2577	rBV	95433	145778	4.58%	0.926%
12	19.439	2776	2780	2788	rBV3	36752	64218	2.02%	0.408%
13	19.875	2849	2854	2863	rBV	2471921	3180092	100.00%	20.195%
14	21.133	3064	3068	3074	rBV	139130	183777	5.78%	1.167%
15	21.410	3110	3115	3123	rBV	725015	1066910	33.55%	6.775%
16	23.845	3523	3529	3542	rVB	544927	1170287	36.80%	7.432%




Sum of corrected areas: 15746799

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019865.D
Acq On : 24 Feb 2024 16:59
Operator : MA/JU
Sample : P1564-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-11

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

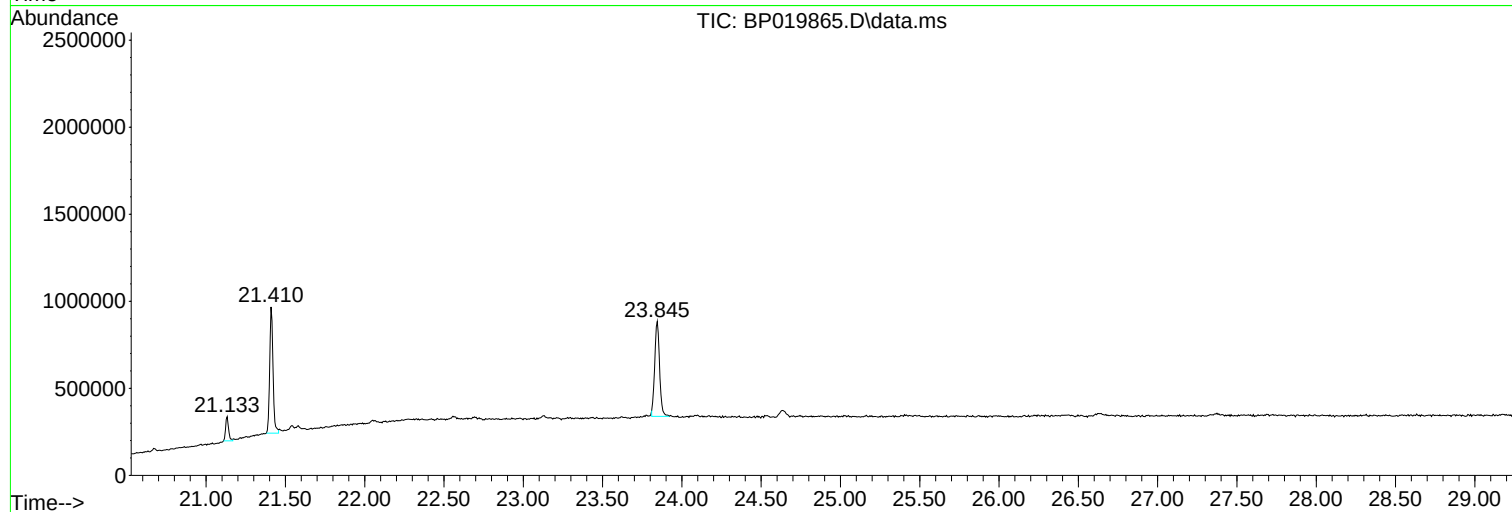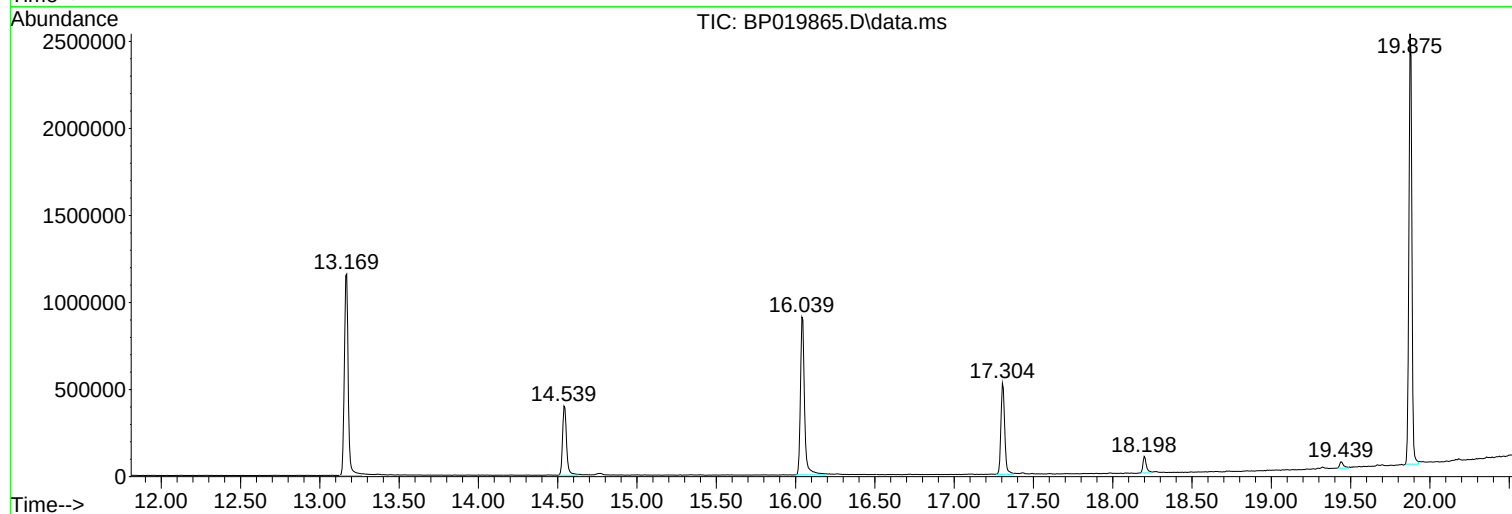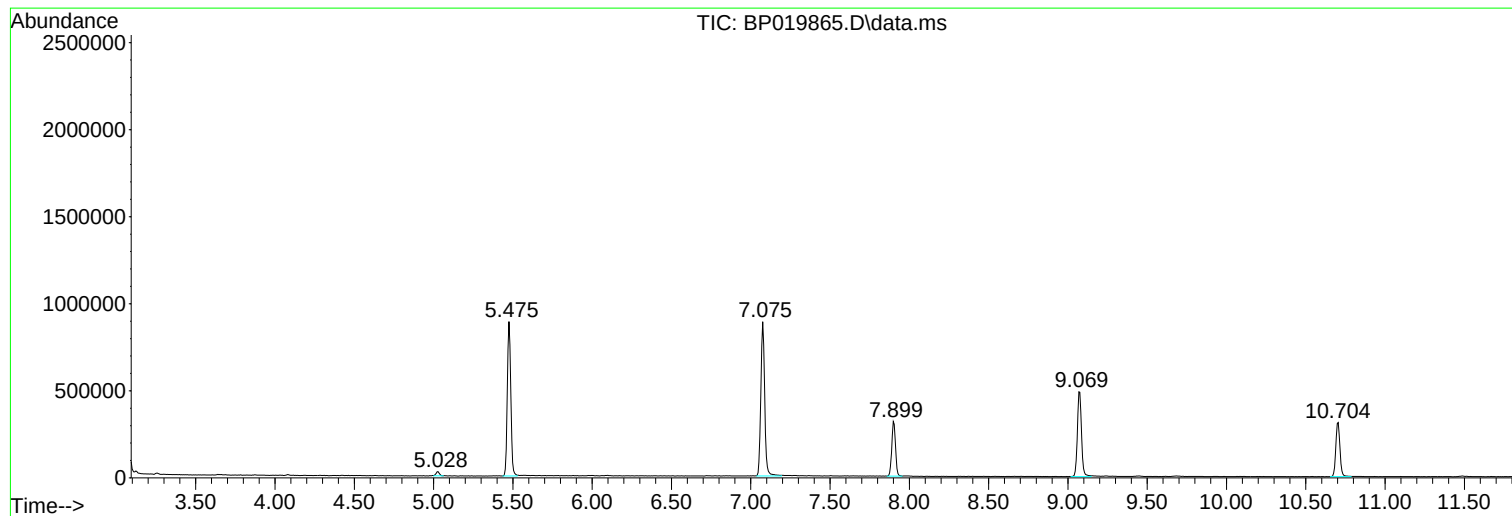

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019865.D
Acq On : 24 Feb 2024 16:59
Operator : MA/JU
Sample : P1564-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-11

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019865.D
Acq On : 24 Feb 2024 16:59
Operator : MA/JU
Sample : P1564-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-11

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------