

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
 Data File : BP019866.D
 Acq On : 24 Feb 2024 17:33
 Operator : MA/JU
 Sample : P1564-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 LKWD-BACKFILL-12

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP019866.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	24	28	39	rVB2	31609	47304	2.06%	0.387%
2	5.022	324	329	335	rVB	24079	34876	1.52%	0.285%
3	5.475	399	406	420	rBV	716960	1070427	46.57%	8.746%
4	7.075	670	678	691	rBV	601063	1021227	44.43%	8.344%
5	7.899	811	818	827	rBV	247645	410756	17.87%	3.356%
6	9.075	1010	1018	1030	rBV	371234	696483	30.30%	5.691%
7	10.699	1286	1294	1312	rBV	271338	506951	22.06%	4.142%
8	13.163	1706	1713	1730	rBV	883999	1510586	65.73%	12.343%
9	14.540	1941	1947	1964	rBV	340058	597742	26.01%	4.884%
10	16.039	2195	2202	2219	rBV	677337	1188937	51.73%	9.715%
11	17.304	2410	2417	2433	rBV	444545	729376	31.74%	5.960%
12	18.198	2564	2569	2579	rBV2	82911	136189	5.93%	1.113%
13	19.439	2776	2780	2788	rBV4	30871	51165	2.23%	0.418%
14	19.875	2849	2854	2864	rBV	1793426	2298291	100.00%	18.779%
15	21.127	3064	3067	3075	rBV2	99956	141262	6.15%	1.154%
16	21.410	3110	3115	3125	rBV	592655	884827	38.50%	7.230%
17	23.839	3522	3528	3537	rVB	425063	911996	39.68%	7.452%




Sum of corrected areas: 12238395

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019866.D
Acq On : 24 Feb 2024 17:33
Operator : MA/JU
Sample : P1564-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

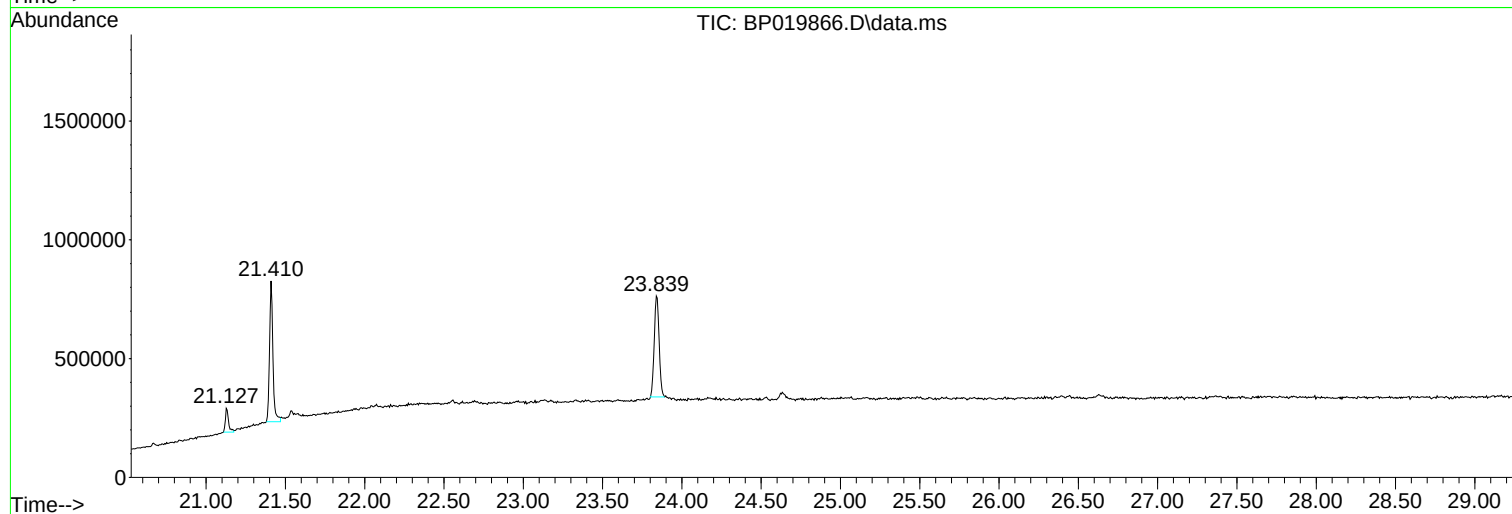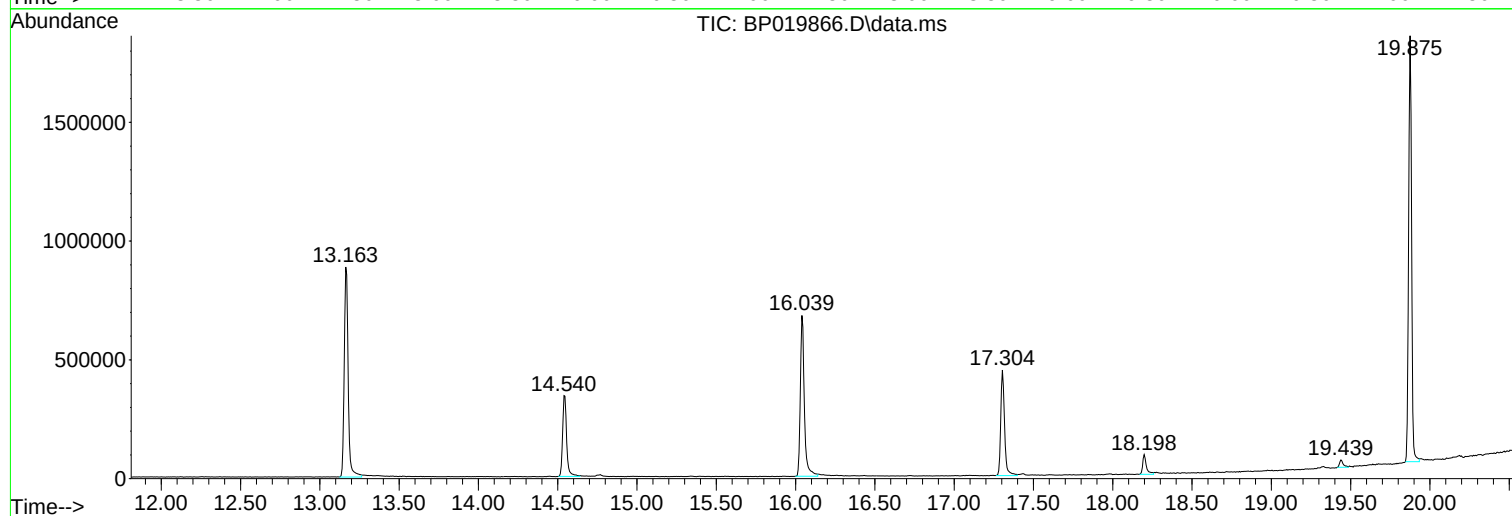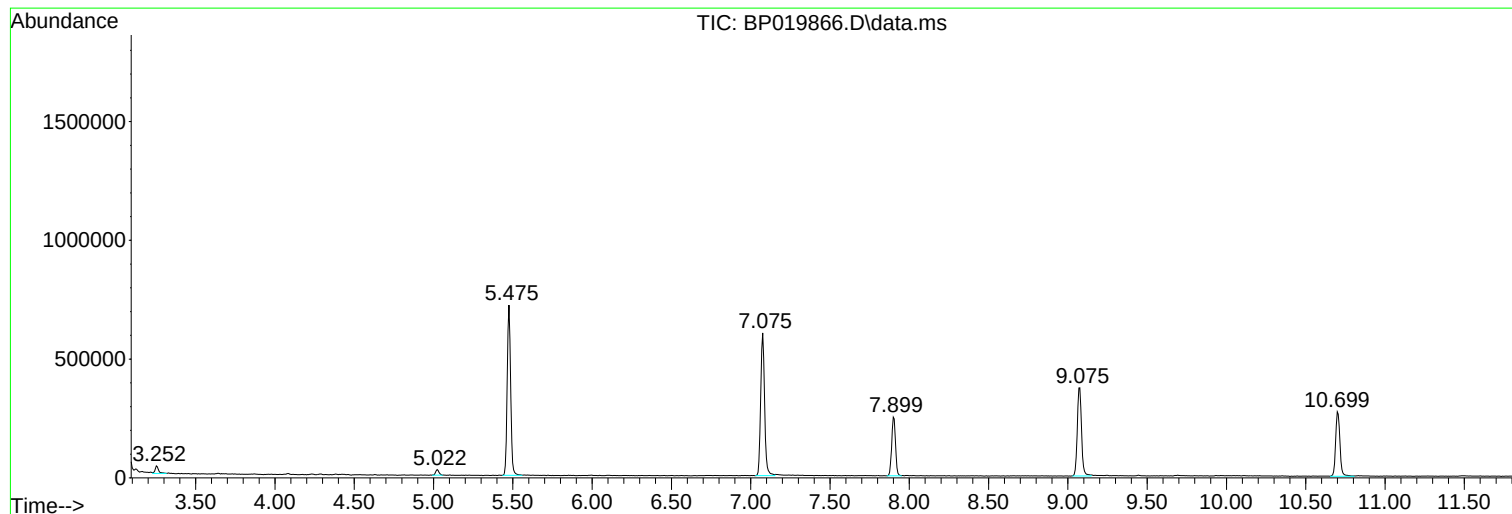

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019866.D
Acq On : 24 Feb 2024 17:33
Operator : MA/JU
Sample : P1564-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019866.D
Acq On : 24 Feb 2024 17:33
Operator : MA/JU
Sample : P1564-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------