

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP022424\  
 Data File : BP019867.D  
 Acq On : 24 Feb 2024 18:06  
 Operator : MA/JU  
 Sample : P1564-09  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 LKWD-BACKFILL-13

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP013124.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP019867.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.475       | 399           | 406         | 417          | rBV      | 1025501        | 1541858       | 33.94%          | 7.832%        |
| 2         | 7.075       | 670           | 678         | 697          | rBV      | 1224799        | 2074121       | 45.66%          | 10.536%       |
| 3         | 7.899       | 810           | 818         | 829          | rBV      | 291396         | 485513        | 10.69%          | 2.466%        |
| 4         | 9.075       | 1010          | 1018        | 1032         | rBV      | 639377         | 1166376       | 25.68%          | 5.925%        |
| 5         | 10.704      | 1287          | 1295        | 1311         | rBV      | 285402         | 526292        | 11.59%          | 2.673%        |
| 6         | 13.163      | 1704          | 1713        | 1731         | rBV      | 1537972        | 2496640       | 54.96%          | 12.682%       |
| 7         | 14.540      | 1940          | 1947        | 1966         | rBV      | 419134         | 702529        | 15.47%          | 3.569%        |
| 8         | 16.040      | 2194          | 2202        | 2221         | rBV      | 1286132        | 2199077       | 48.41%          | 11.171%       |
| 9         | 17.304      | 2410          | 2417        | 2431         | rBV      | 554099         | 905315        | 19.93%          | 4.599%        |
| 10        | 18.198      | 2564          | 2569        | 2580         | rBV      | 187927         | 282697        | 6.22%           | 1.436%        |
| 11        | 19.439      | 2776          | 2780        | 2787         | rBV3     | 66295          | 100609        | 2.21%           | 0.511%        |
| 12        | 19.875      | 2848          | 2854        | 2867         | rBV      | 3586797        | 4542610       | 100.00%         | 23.075%       |
| 13        | 21.127      | 3063          | 3067        | 3074         | rBV2     | 263835         | 348708        | 7.68%           | 1.771%        |
| 14        | 21.410      | 3110          | 3115        | 3127         | rBV      | 792247         | 1113082       | 24.50%          | 5.654%        |
| 15        | 23.839      | 3522          | 3528        | 3538         | rVB      | 551983         | 1200780       | 26.43%          | 6.100%        |




Sum of corrected areas: 19686207

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP022424\  
Data File : BP019867.D  
Acq On : 24 Feb 2024 18:06  
Operator : MA/JU  
Sample : P1564-09  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
LKWD-BACKFILL-13

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP013124.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

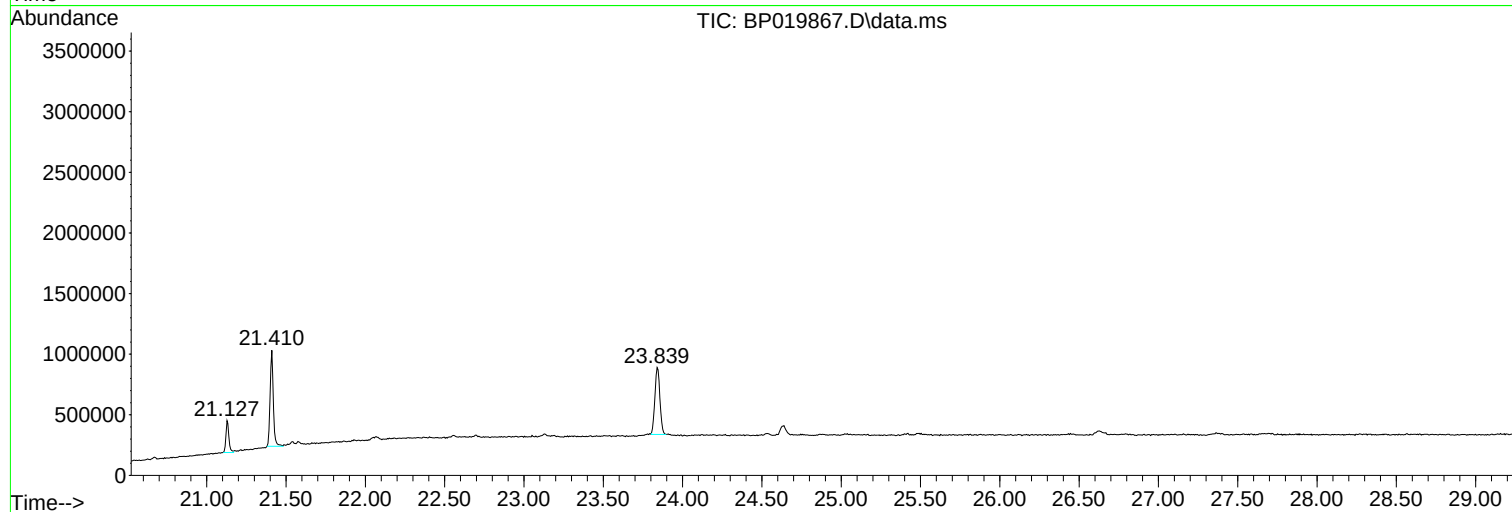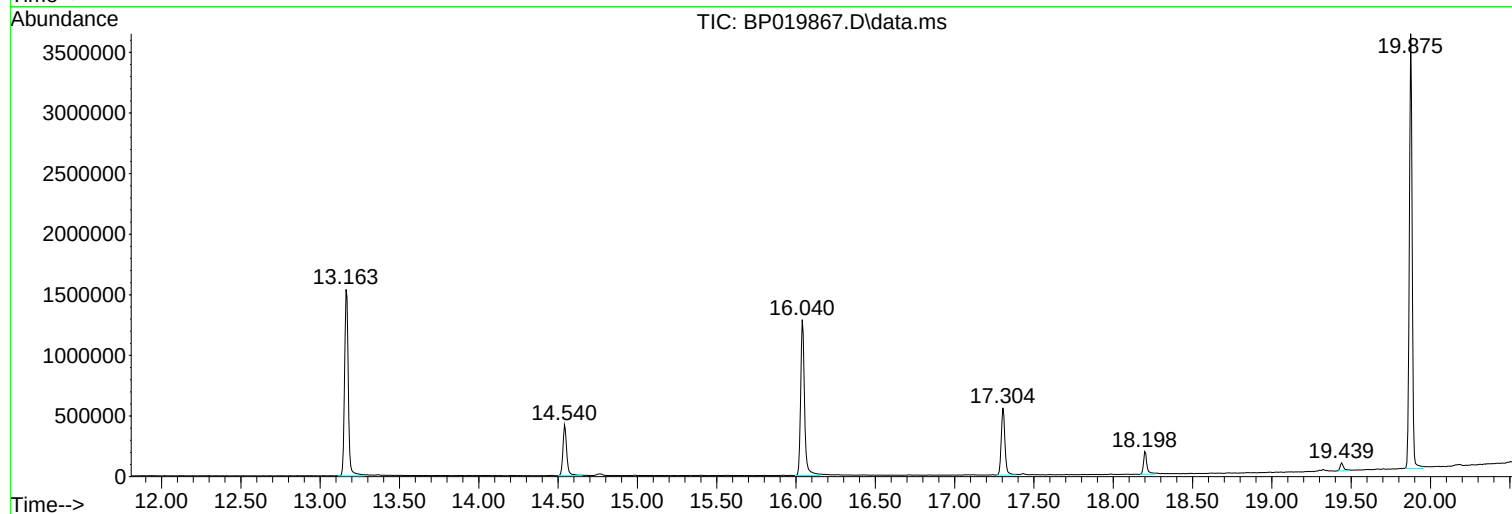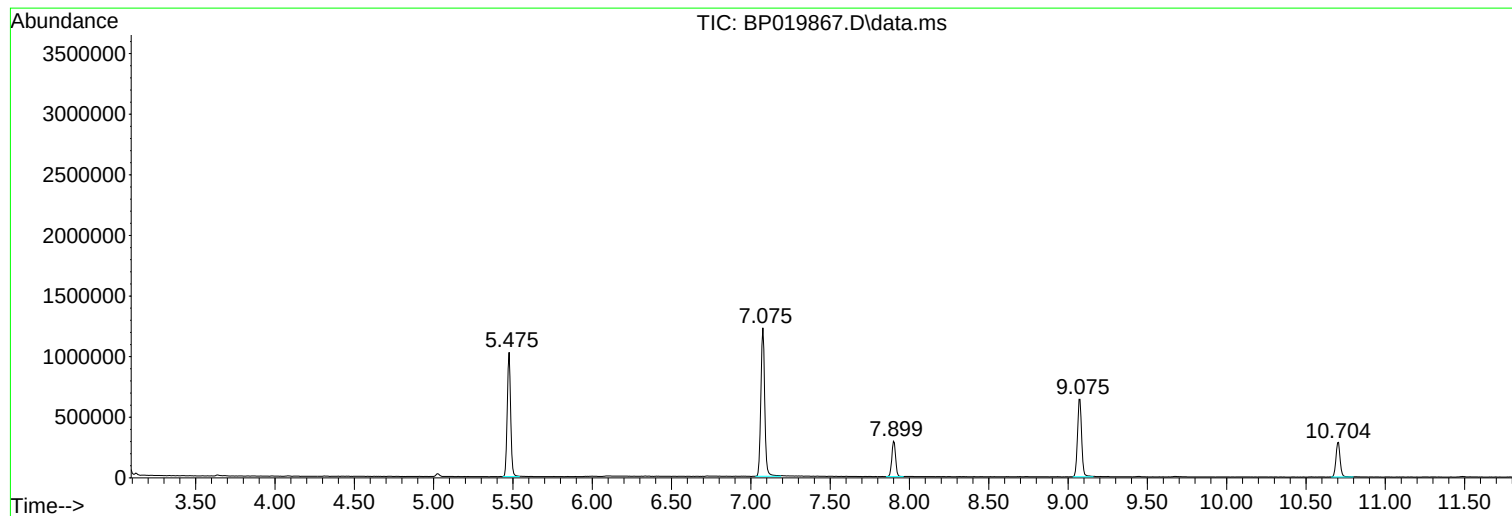

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP022424\  
Data File : BP019867.D  
Acq On : 24 Feb 2024 18:06  
Operator : MA/JU  
Sample : P1564-09  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
LKWD-BACKFILL-13

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP013124.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP022424\  
Data File : BP019867.D  
Acq On : 24 Feb 2024 18:06  
Operator : MA/JU  
Sample : P1564-09  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
LKWD-BACKFILL-13

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP013124.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|