

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
 Data File : BP019868.D
 Acq On : 24 Feb 2024 18:40
 Operator : MA/JU
 Sample : P1564-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 LKWD-BACKFILL-14

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP019868.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.022	323	329	337	rBV	33831	53529	1.43%	0.335%
2	5.475	399	406	418	rBV	863808	1311171	34.93%	8.218%
3	7.075	670	678	696	rBV	757905	1296101	34.53%	8.123%
4	7.899	812	818	829	rVB	229584	375928	10.02%	2.356%
5	9.075	1009	1018	1032	rBV	468702	870986	23.21%	5.459%
6	10.699	1284	1294	1305	rBV	257373	481961	12.84%	3.021%
7	13.163	1704	1713	1736	rBV	1213972	2014505	53.67%	12.626%
8	14.539	1940	1947	1968	rBV	375248	639566	17.04%	4.008%
9	16.039	2195	2202	2222	rBV	1070702	1802298	48.02%	11.296%
10	17.304	2410	2417	2431	rBV	519194	836924	22.30%	5.245%
11	18.198	2564	2569	2579	rBV	121603	193253	5.15%	1.211%
12	19.439	2776	2780	2786	rBV2	46820	70496	1.88%	0.442%
13	19.875	2848	2854	2863	rBV	2978021	3753222	100.00%	23.523%
14	21.127	3064	3067	3074	rBV	153364	211787	5.64%	1.327%
15	21.410	3110	3115	3124	rBV	699860	1026786	27.36%	6.435%
16	23.839	3522	3528	3539	rVB	468554	1016861	27.09%	6.373%




Sum of corrected areas: 15955374

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019868.D
Acq On : 24 Feb 2024 18:40
Operator : MA/JU
Sample : P1564-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

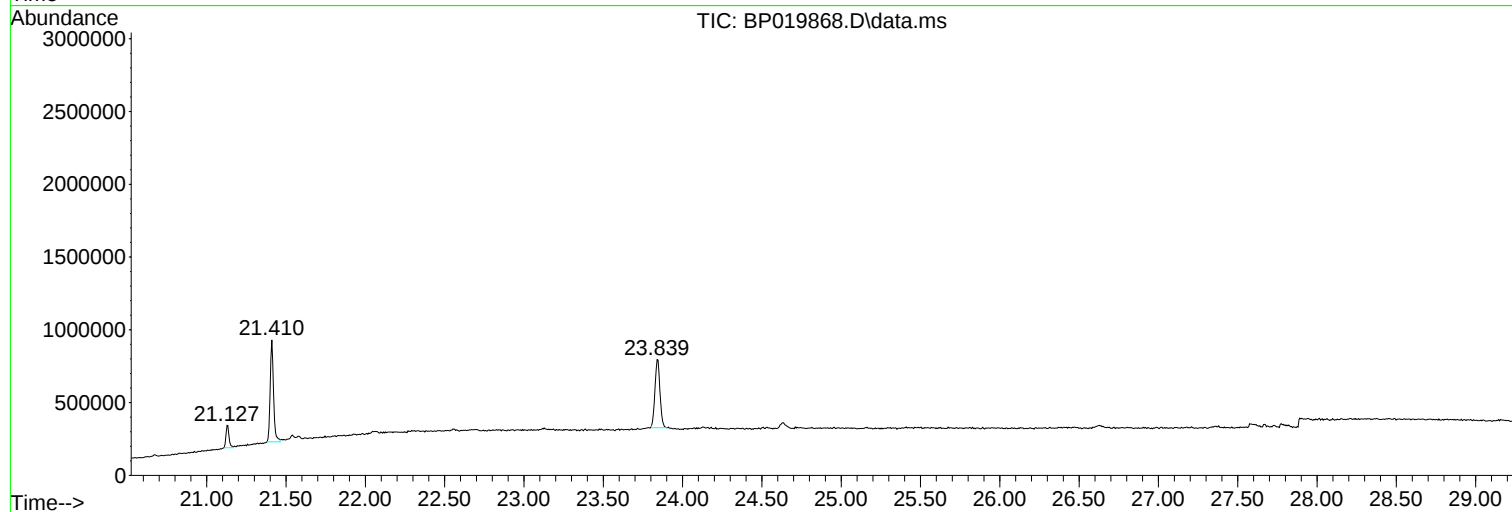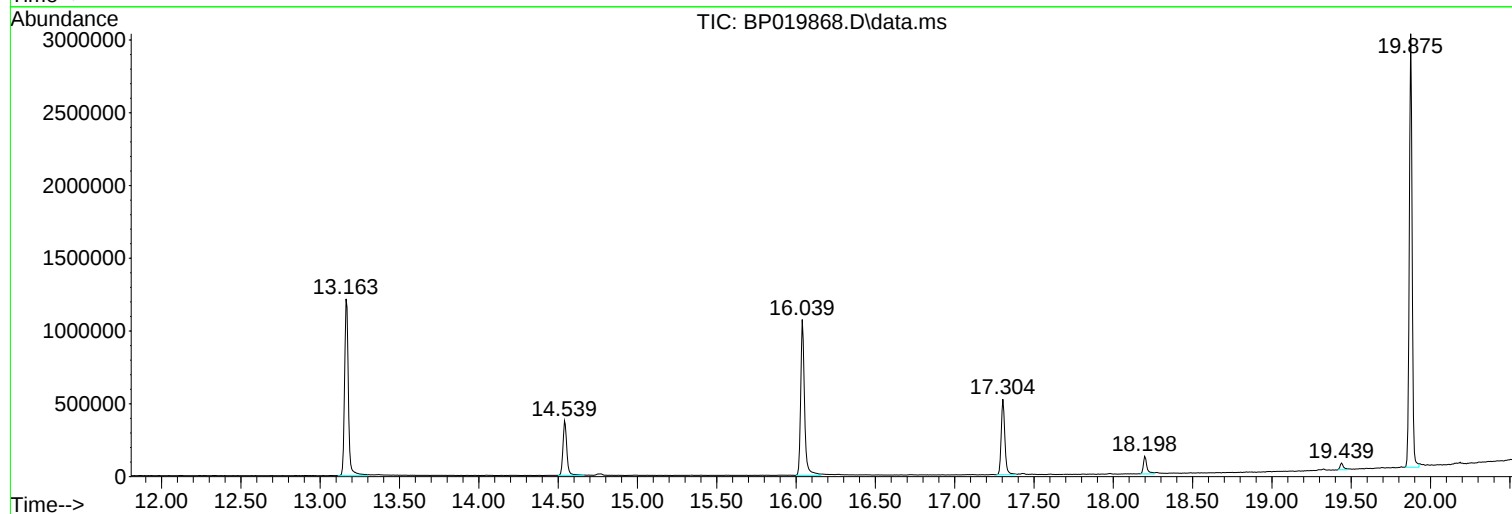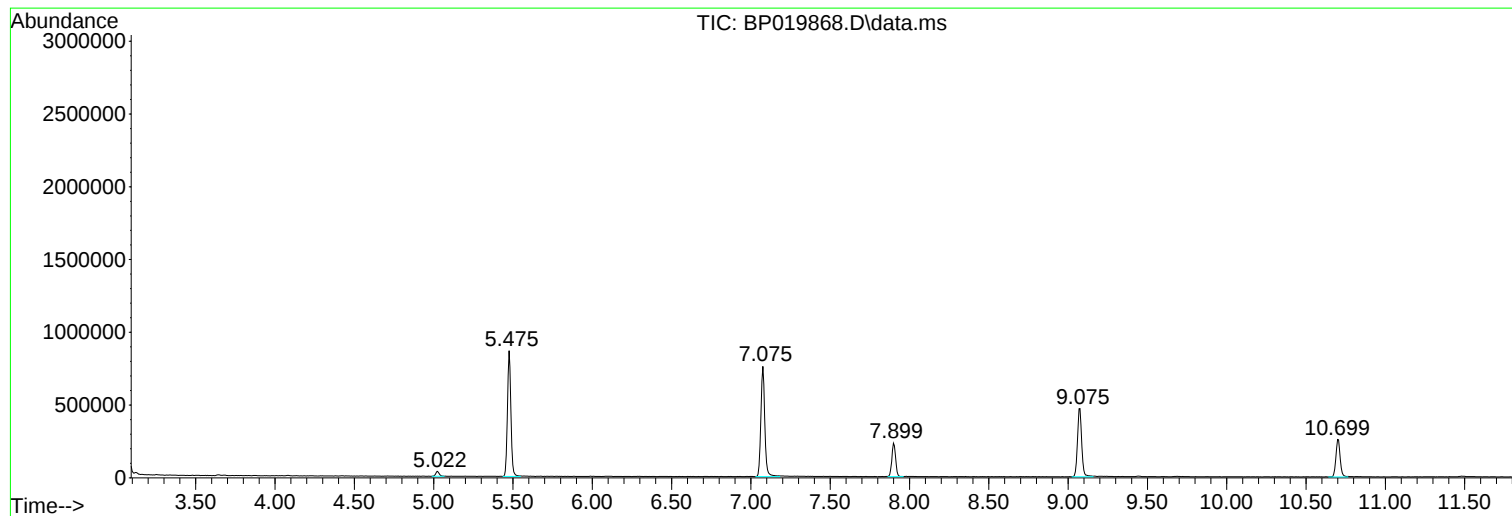

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019868.D
Acq On : 24 Feb 2024 18:40
Operator : MA/JU
Sample : P1564-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019868.D
Acq On : 24 Feb 2024 18:40
Operator : MA/JU
Sample : P1564-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------