

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
 Data File : BP019869.D
 Acq On : 24 Feb 2024 19:14
 Operator : MA/JU
 Sample : P1564-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 LKWD-BACKFILL-15

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP019869.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.022	325	329	337	rVB	20144	31866	1.04%	0.215%
2	5.475	399	406	419	rBV	859495	1294821	42.37%	8.724%
3	7.075	670	678	696	rBV	774150	1331482	43.57%	8.971%
4	7.899	812	818	826	rBV	263293	428448	14.02%	2.887%
5	9.069	1008	1017	1031	rBV	461188	833070	27.26%	5.613%
6	10.698	1286	1294	1306	rBV	280087	515735	16.88%	3.475%
7	13.163	1706	1713	1733	rBV	1070564	1805749	59.09%	12.166%
8	14.539	1940	1947	1965	rBV	372627	636728	20.84%	4.290%
9	16.039	2195	2202	2230	rBV	867912	1534092	50.20%	10.336%
10	17.304	2410	2417	2432	rBV	478465	790463	25.87%	5.326%
11	18.198	2564	2569	2579	rBV	113367	167219	5.47%	1.127%
12	19.439	2776	2780	2784	rBV2	35505	50155	1.64%	0.338%
13	19.874	2848	2854	2866	rBV	2480110	3056000	100.00%	20.589%
14	21.127	3064	3067	3073	rBV2	143188	185741	6.08%	1.251%
15	21.410	3110	3115	3125	rBV	694634	1012890	33.14%	6.824%
16	23.845	3522	3529	3539	rVB	514556	1168295	38.23%	7.871%




Sum of corrected areas: 14842754

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019869.D
Acq On : 24 Feb 2024 19:14
Operator : MA/JU
Sample : P1564-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

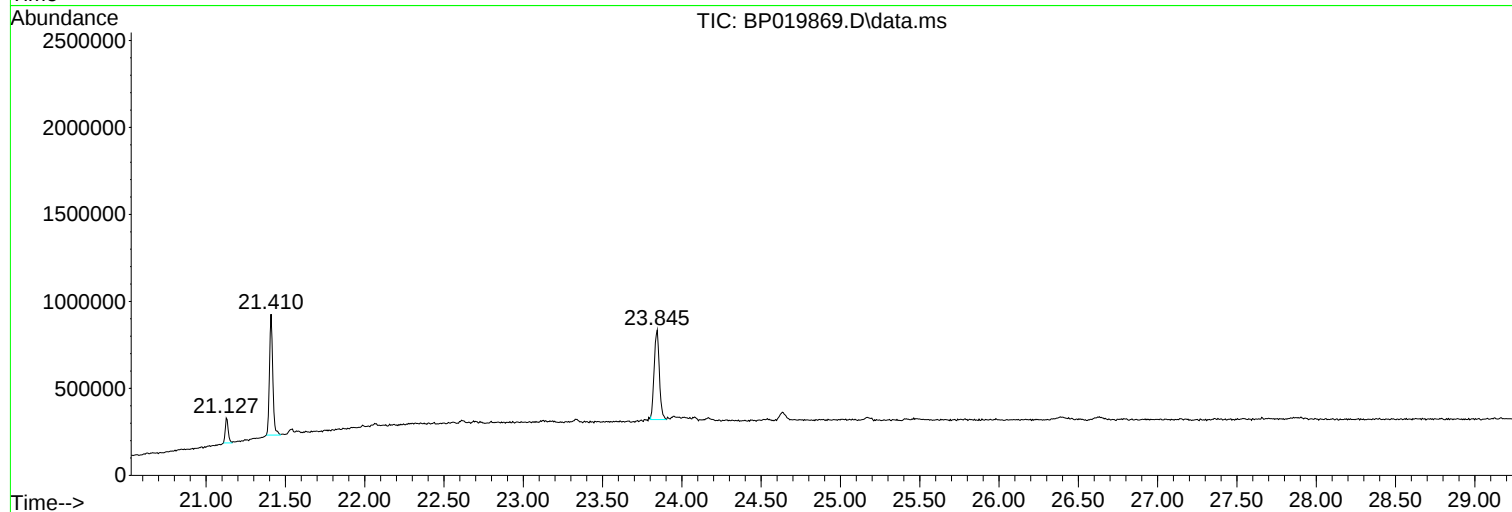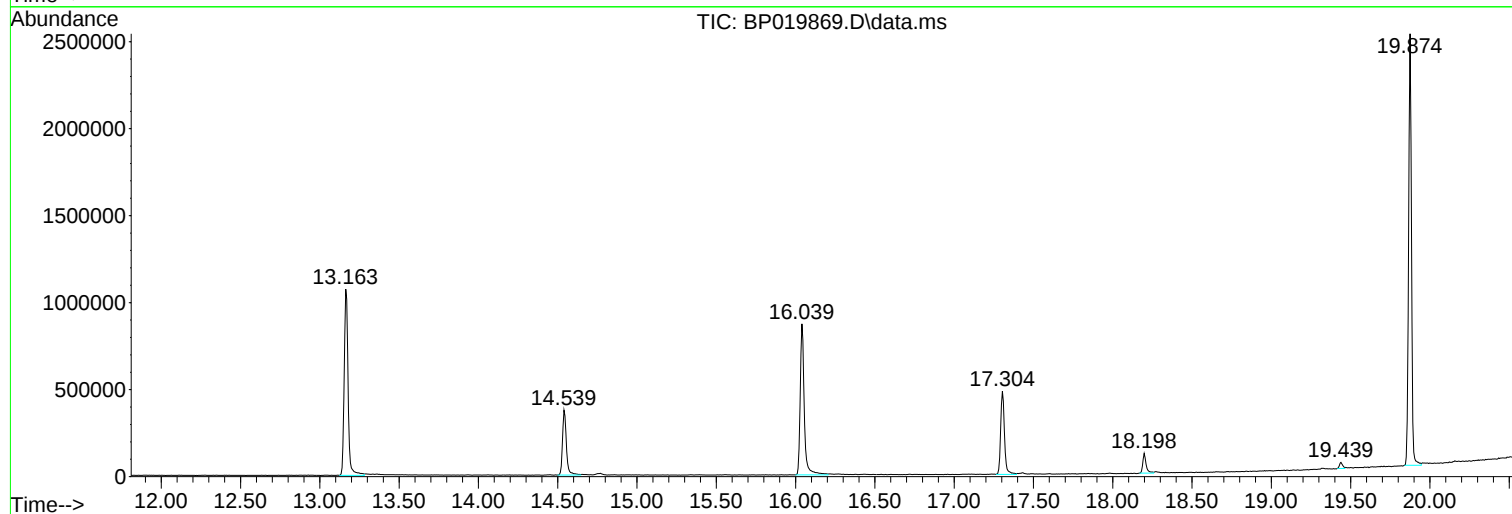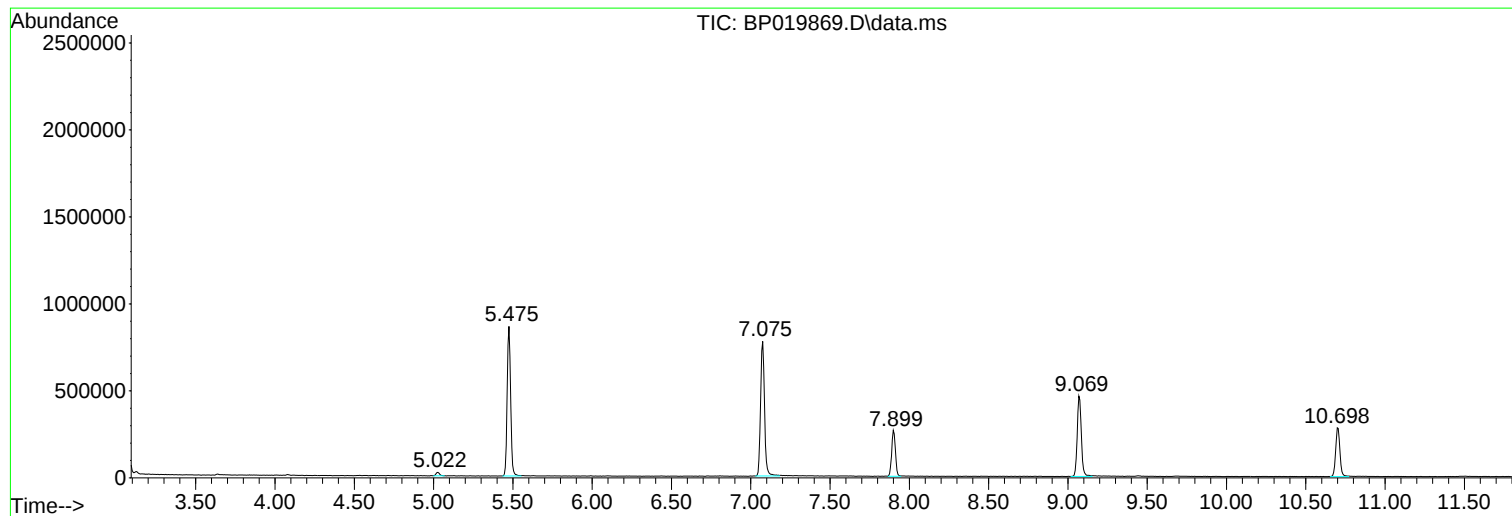

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019869.D
Acq On : 24 Feb 2024 19:14
Operator : MA/JU
Sample : P1564-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019869.D
Acq On : 24 Feb 2024 19:14
Operator : MA/JU
Sample : P1564-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------