

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019870.D
Acq On : 24 Feb 2024 19:47
Operator : MA/JU
Sample : P1564-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-16

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP019870.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.475	399	406	416	rBV	731573	1123595	35.06%	7.160%
2	7.075	671	678	688	rBV	673976	1150689	35.90%	7.333%
3	7.899	809	818	826	rBV	291483	469702	14.65%	2.993%
4	9.069	1009	1017	1031	rBV	474597	877120	27.37%	5.589%
5	10.699	1286	1294	1305	rBV	327303	603367	18.83%	3.845%
6	13.163	1706	1713	1735	rBV	1125642	1936247	60.41%	12.339%
7	14.539	1934	1947	1961	rBV	452613	809134	25.25%	5.156%
8	16.039	2194	2202	2229	rBV	1037679	1848420	57.67%	11.779%
9	17.304	2410	2417	2429	rBV	640696	1040094	32.45%	6.628%
10	18.198	2564	2569	2579	rBV	93195	145525	4.54%	0.927%
11	19.439	2776	2780	2789	rBV5	31243	57368	1.79%	0.366%
12	19.874	2848	2854	2869	rBV	2542719	3205101	100.00%	20.425%
13	21.133	3064	3068	3073	rBV2	117288	160609	5.01%	1.023%
14	21.410	3110	3115	3122	rBV	774179	1112912	34.72%	7.092%
15	23.845	3522	3529	3539	rVB	538894	1152404	35.96%	7.344%




Sum of corrected areas: 15692287

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019870.D
Acq On : 24 Feb 2024 19:47
Operator : MA/JU
Sample : P1564-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-16

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

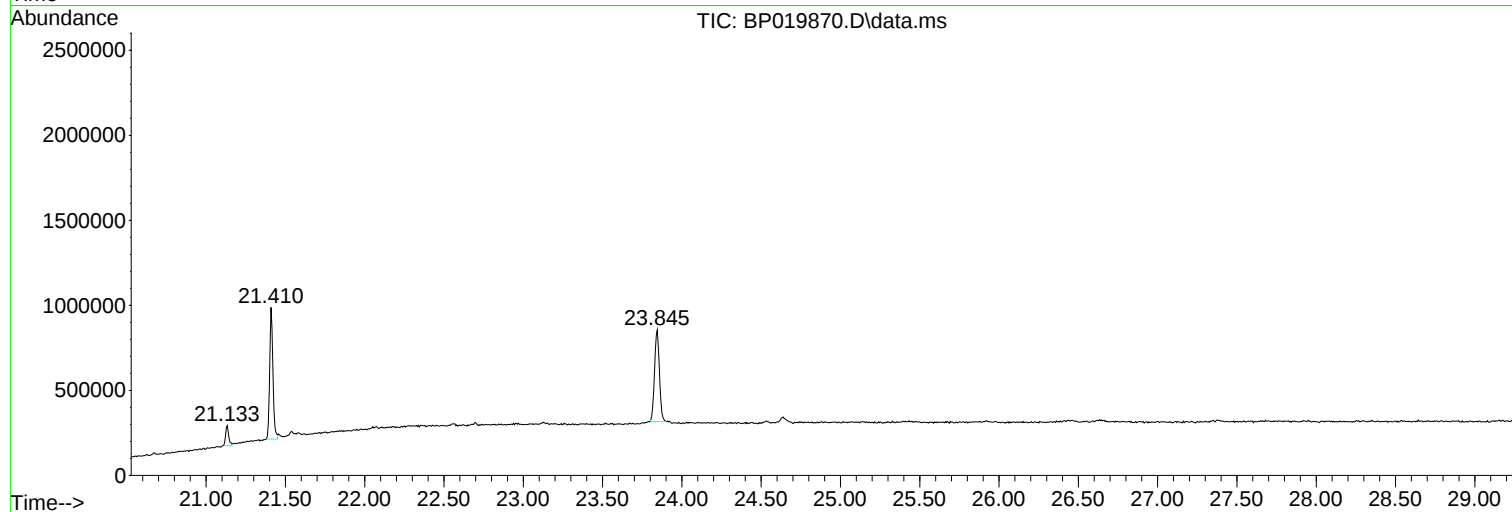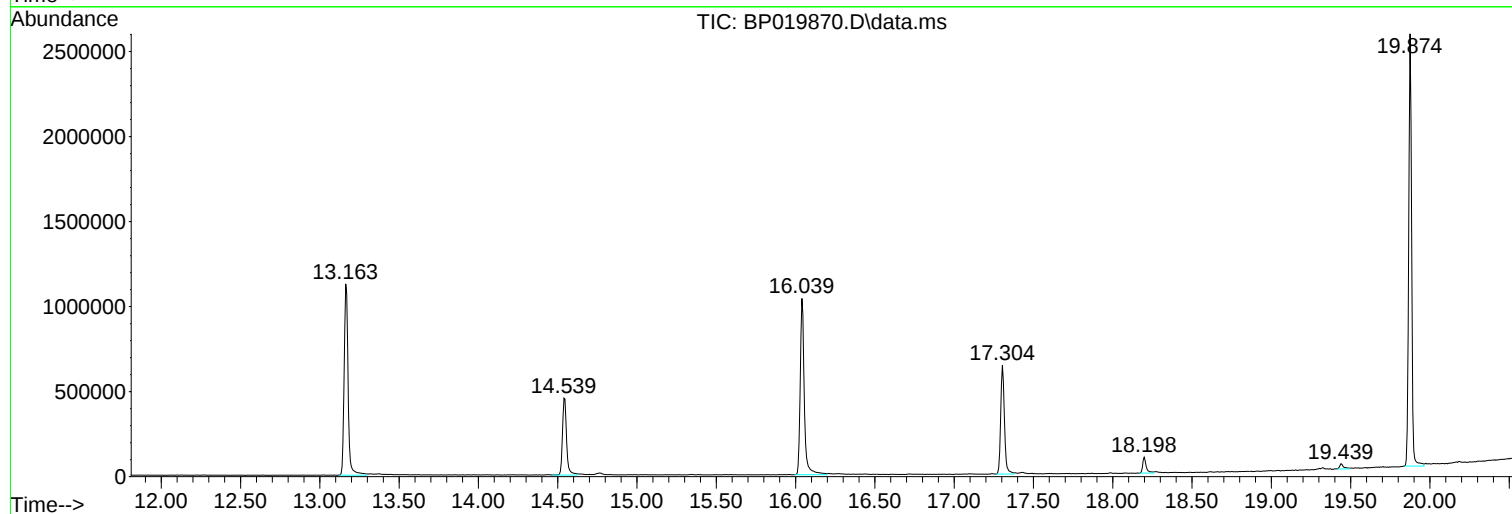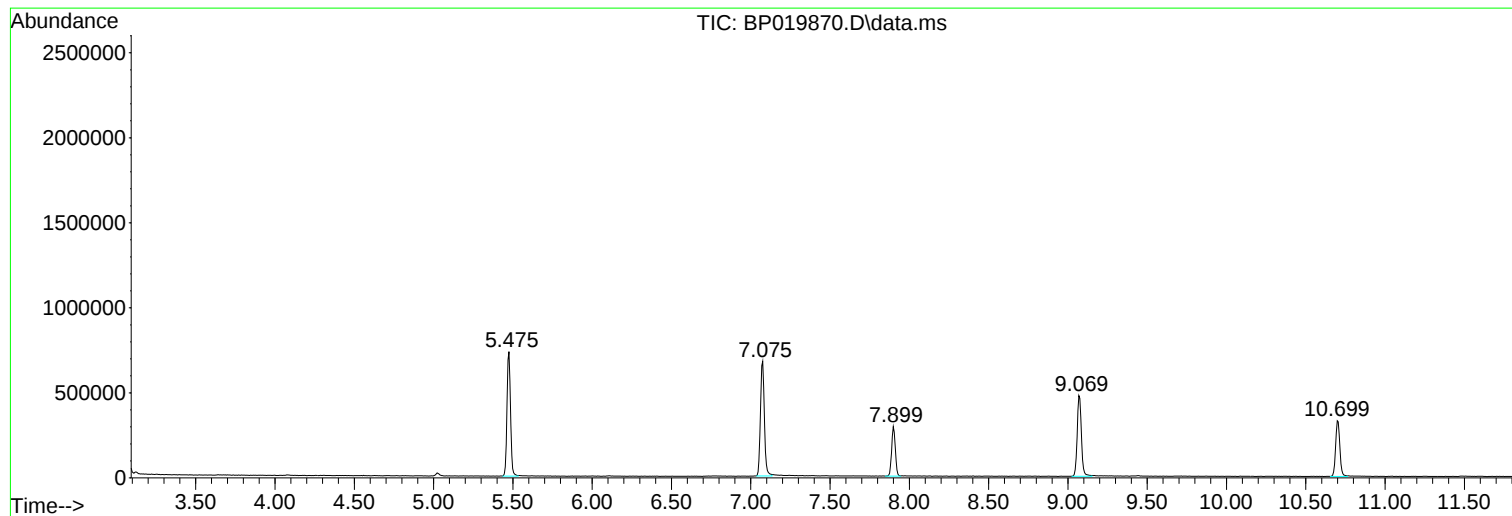

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019870.D
Acq On : 24 Feb 2024 19:47
Operator : MA/JU
Sample : P1564-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-16

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019870.D
Acq On : 24 Feb 2024 19:47
Operator : MA/JU
Sample : P1564-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-16

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------