

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
 Data File : BP019871.D
 Acq On : 24 Feb 2024 20:21
 Operator : MA/JU
 Sample : P1564-17
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 LKWD-BACKFILL-17

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP019871.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.475	399	406	421	rBV	797616	1224446	33.82%	7.712%
2	7.075	670	678	695	rBV	715713	1254758	34.66%	7.903%
3	7.899	811	818	829	rBV	246778	412118	11.38%	2.596%
4	9.069	1010	1017	1031	rBV	463919	845795	23.36%	5.327%
5	10.699	1286	1294	1308	rBV	282008	518044	14.31%	3.263%
6	13.163	1706	1713	1728	rBV	1168273	1961103	54.17%	12.352%
7	14.539	1940	1947	1964	rBV	412531	690380	19.07%	4.348%
8	16.039	2195	2202	2228	rBV	1047555	1796283	49.62%	11.314%
9	17.304	2410	2417	2428	rBV	543604	874421	24.15%	5.508%
10	18.198	2564	2569	2578	rBV2	120831	179657	4.96%	1.132%
11	19.439	2776	2780	2787	rBV3	46014	66750	1.84%	0.420%
12	19.874	2848	2854	2865	rBV	2871627	3620321	100.00%	22.803%
13	21.127	3064	3067	3074	rBV	181261	222514	6.15%	1.401%
14	21.410	3110	3115	3125	rBV	759554	1104867	30.52%	6.959%
15	23.839	3522	3528	3540	rVB	508139	1105398	30.53%	6.962%




Sum of corrected areas: 15876855

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019871.D
Acq On : 24 Feb 2024 20:21
Operator : MA/JU
Sample : P1564-17
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-17

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

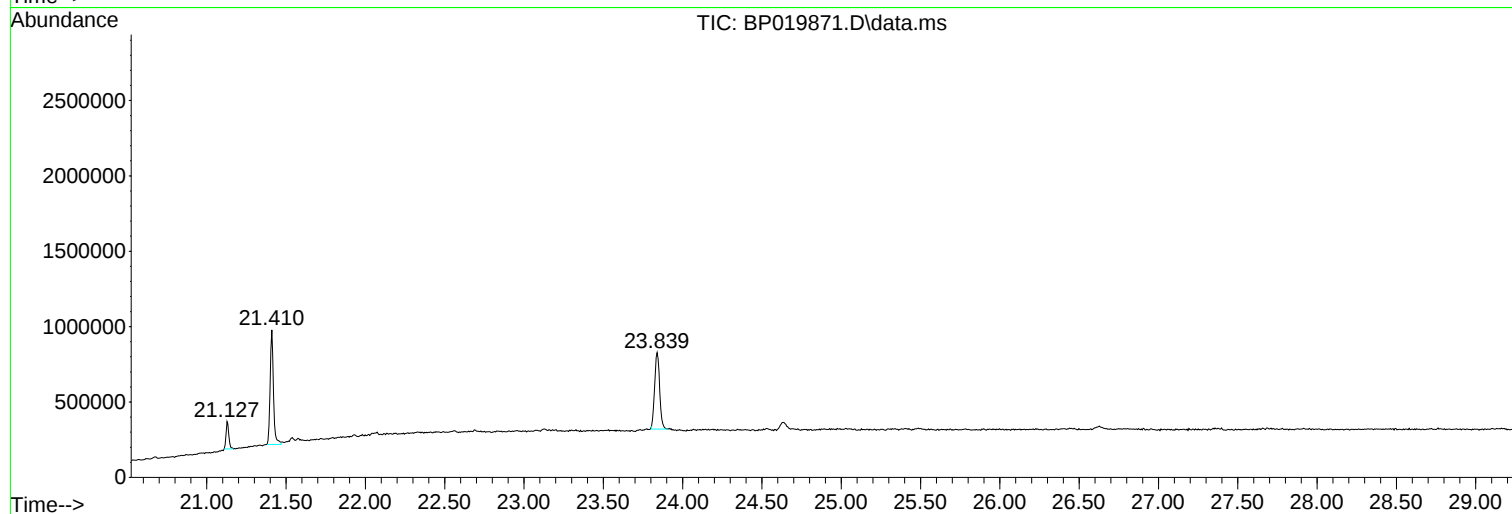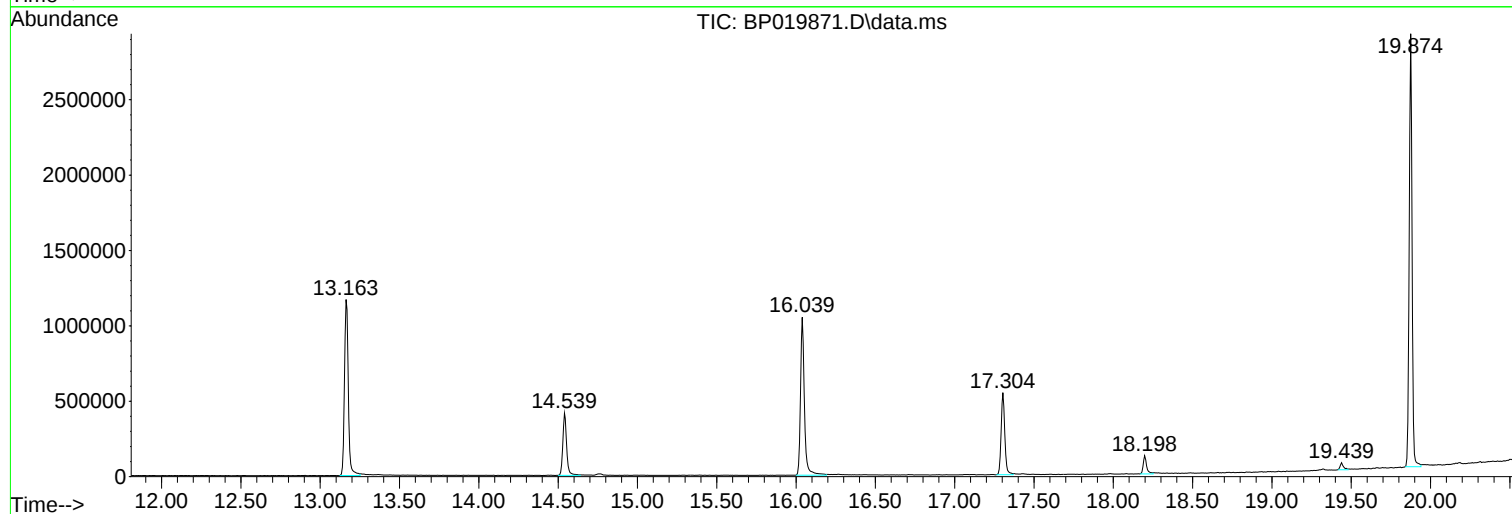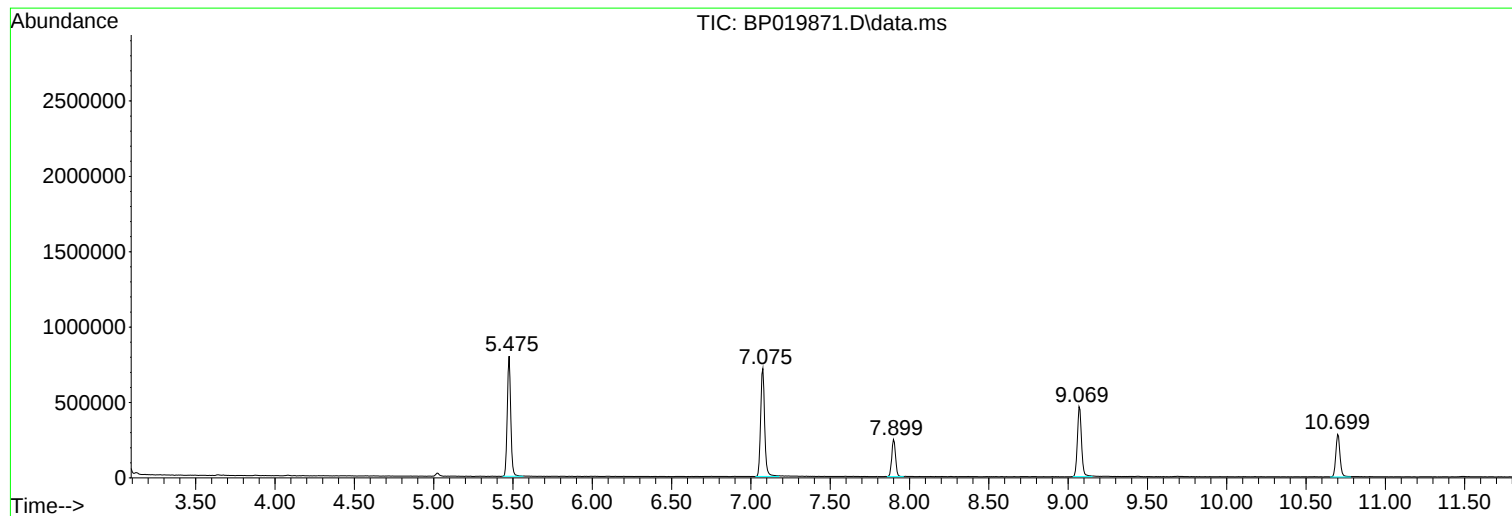

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019871.D
Acq On : 24 Feb 2024 20:21
Operator : MA/JU
Sample : P1564-17
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-17

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019871.D
Acq On : 24 Feb 2024 20:21
Operator : MA/JU
Sample : P1564-17
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-17

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------