

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
 Data File : BP019872.D
 Acq On : 24 Feb 2024 20:55
 Operator : MA/JU
 Sample : P1564-19
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 LKWD-BACKFILL-18

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP019872.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.022	324	329	337	rVB	30740	45531	1.01%	0.246%
2	5.475	399	406	417	rBV	875472	1329585	29.43%	7.173%
3	7.075	670	678	692	rBV	791353	1349173	29.86%	7.278%
4	7.899	811	818	827	rBV	268213	430497	9.53%	2.322%
5	9.069	1010	1017	1035	rBV	524591	932688	20.65%	5.031%
6	10.698	1285	1294	1308	rBV	301878	560832	12.41%	3.025%
7	13.163	1706	1713	1730	rBV	1428313	2284428	50.57%	12.323%
8	14.539	1941	1947	1965	rBV	452260	782502	17.32%	4.221%
9	16.039	2194	2202	2226	rBV	1275333	2152940	47.66%	11.614%
10	17.304	2410	2417	2431	rBV	662038	1064699	23.57%	5.744%
11	18.198	2564	2569	2577	rBV2	122683	176966	3.92%	0.955%
12	19.439	2776	2780	2786	rBV3	41067	59332	1.31%	0.320%
13	19.874	2848	2854	2869	rBV	3568879	4517651	100.00%	24.371%
14	21.127	3063	3067	3077	rBV	266097	365427	8.09%	1.971%
15	21.410	3110	3115	3127	rBV	883977	1265284	28.01%	6.826%
16	23.839	3521	3528	3537	rVB	538469	1219675	27.00%	6.580%




Sum of corrected areas: 18537210

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019872.D
Acq On : 24 Feb 2024 20:55
Operator : MA/JU
Sample : P1564-19
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-18

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

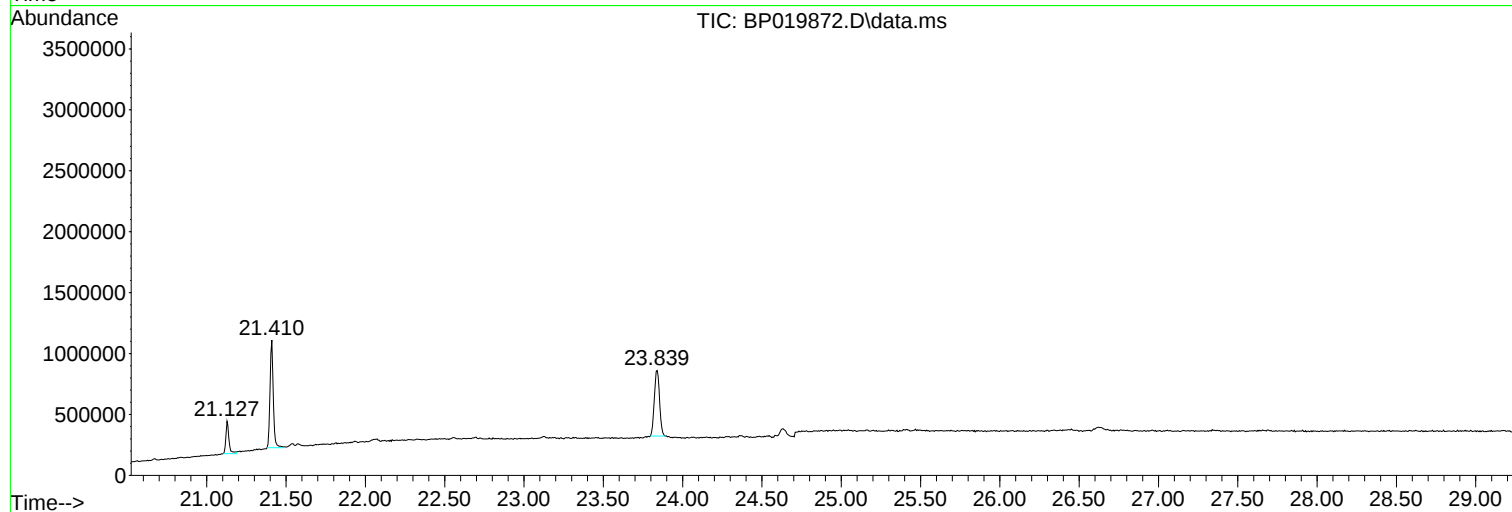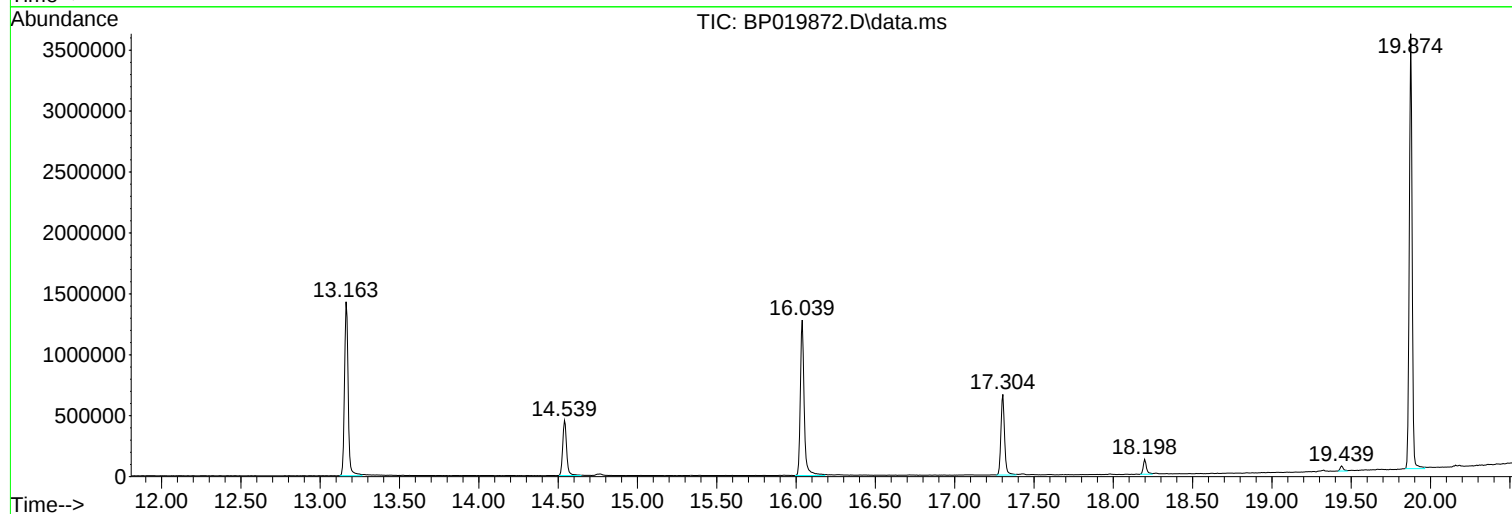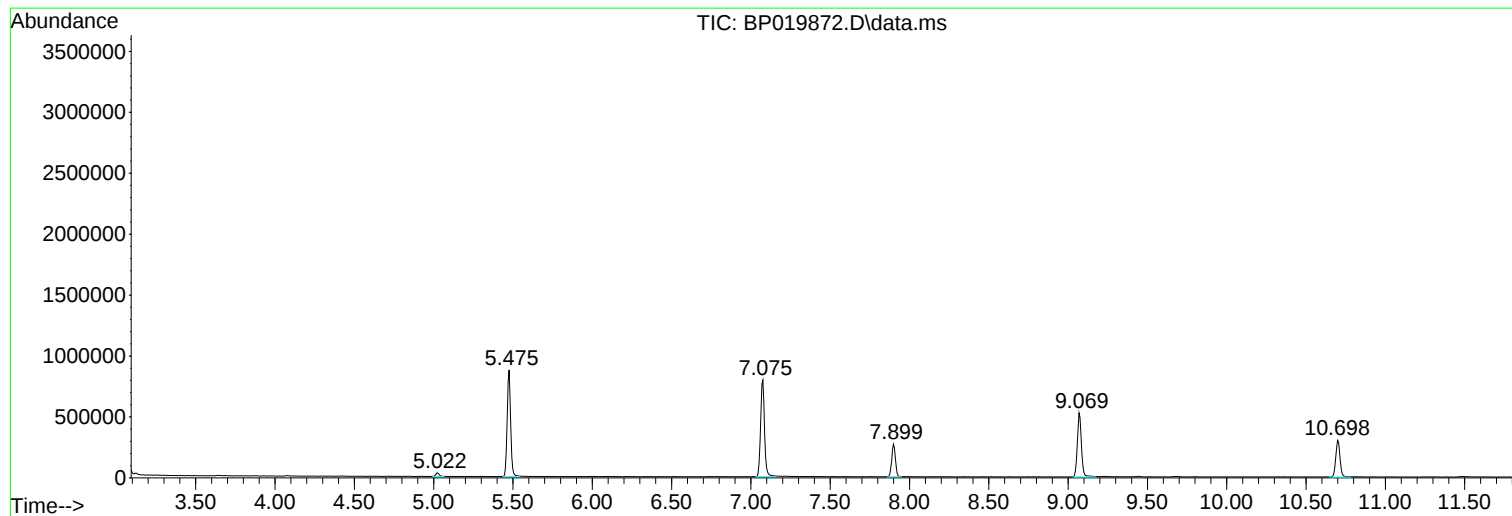

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019872.D
Acq On : 24 Feb 2024 20:55
Operator : MA/JU
Sample : P1564-19
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-18

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019872.D
Acq On : 24 Feb 2024 20:55
Operator : MA/JU
Sample : P1564-19
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
LKWD-BACKFILL-18

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------