


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019854.D
Acq On : 24 Feb 2024 10:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 23 13:10:49 2024

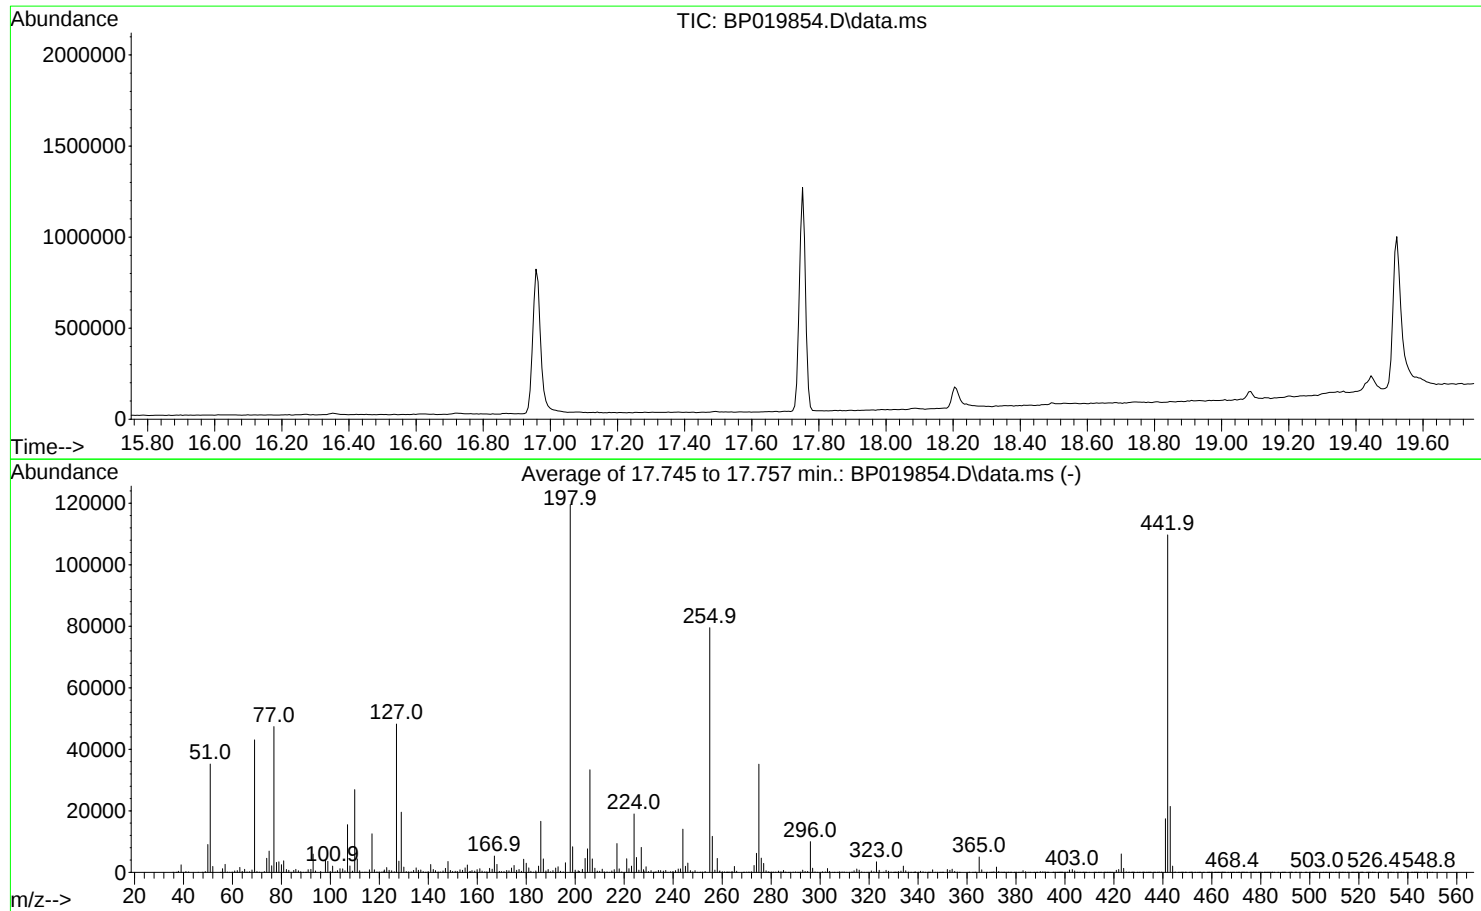




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.5	35240	PASS
68	69	0.00	2	1.8	756	PASS
69	198	0.00	100	36.0	43082	PASS
70	69	0.00	2	0.6	252	PASS
127	198	10	80	40.3	48250	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	119603	PASS
199	198	5	9	7.0	8323	PASS
275	198	10	60	29.4	35155	PASS
365	198	1	100	4.2	4983	PASS
441	198	0.01	100	14.6	17447	PASS
442	442	100	100	100.0	109731	PASS
443	442	15	24	19.6	21460	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019854.D
Acq On : 24 Feb 2024 10:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 26 01:58:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 23 13:10:49 2024
Response via : Initial Calibration

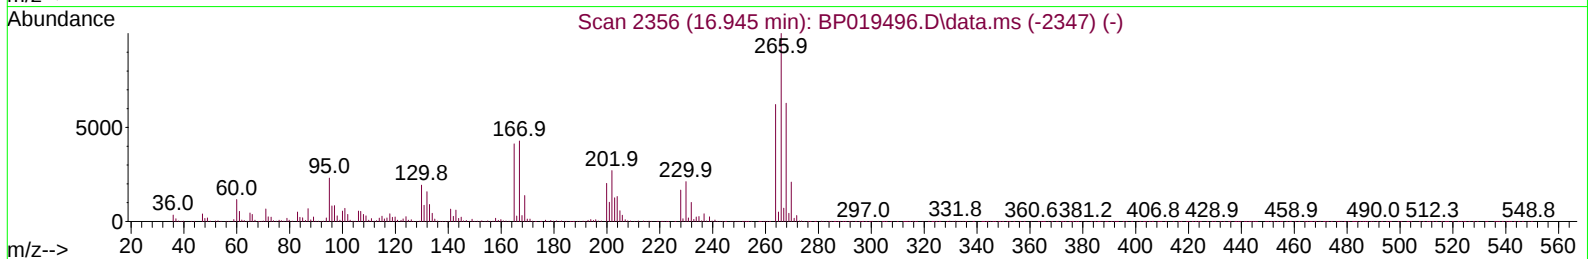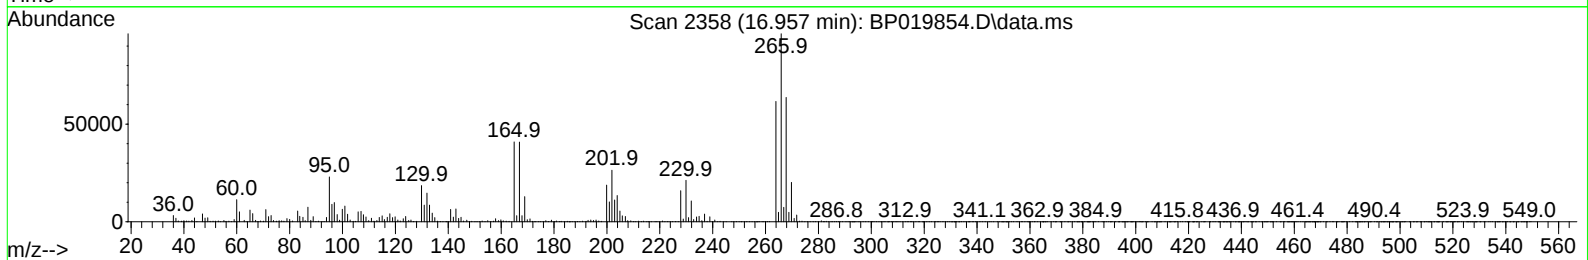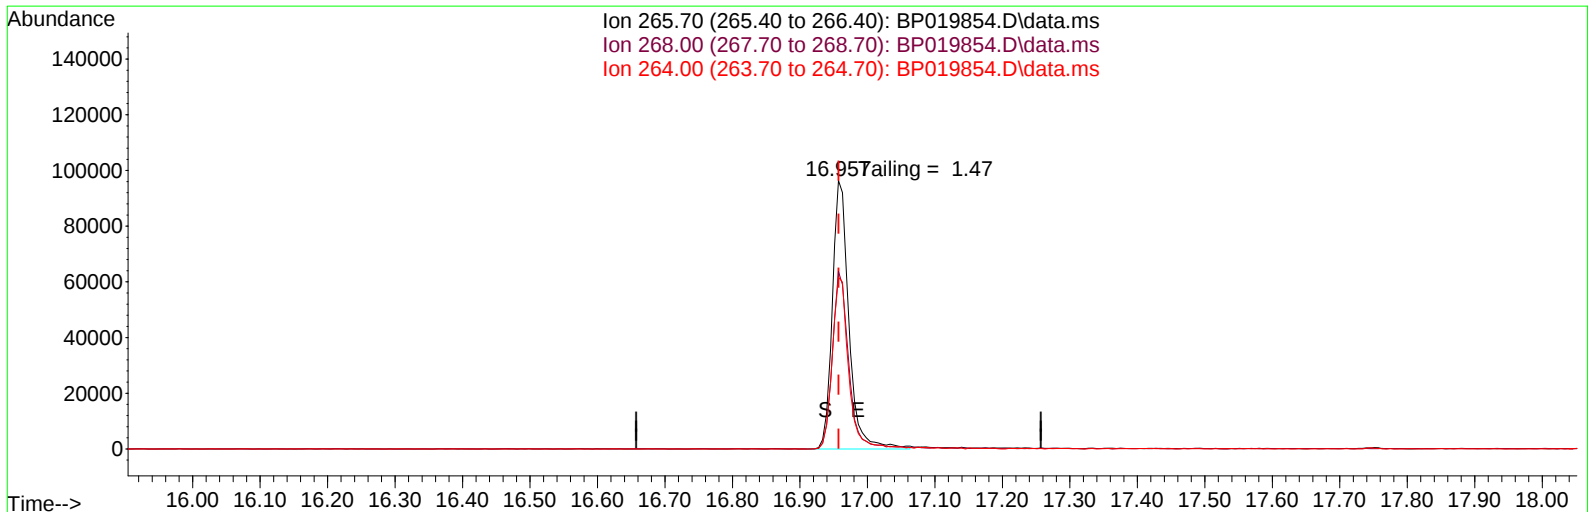

TIC: BP019854.D\data.ms

(70) Pentachlorophenol (C)

16.957min (+ 0.000) 272729.90 ng




response 163643

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	66.11
264.00	62.10	63.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022424\
Data File : BP019854.D
Acq On : 24 Feb 2024 10:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 26 01:58:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 23 13:10:49 2024
Response via : Initial Calibration

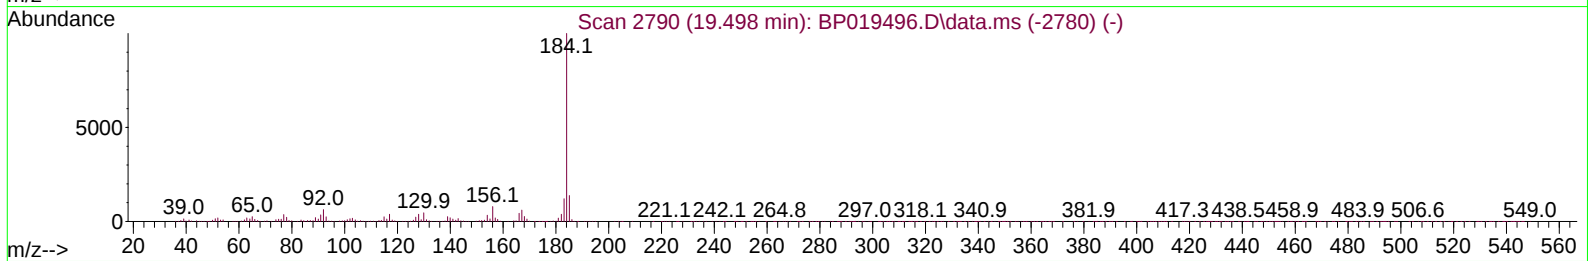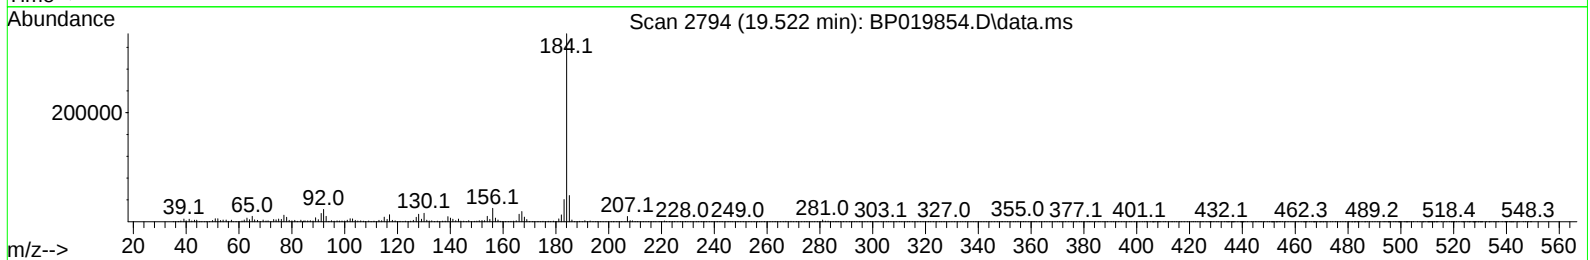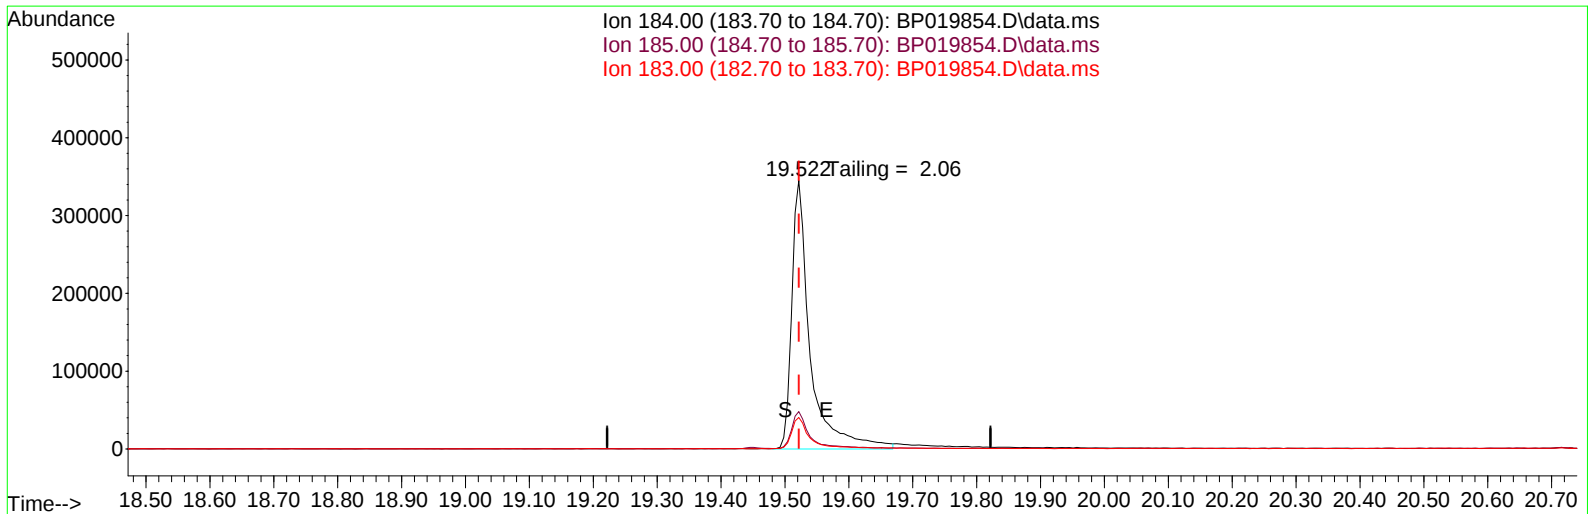

TIC: BP019854.D\data.ms

(77) Benzidine

19.522min (+ 0.000) 118599.99 ng

response 709146

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.92
183.00	12.10	11.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/24/2024	BNA_P	<u>BP019854.D</u>
Compound Name	Response	Retention Time
DDT	417269	20.716
DDD	19110	20.292
DDE	3133	19.786
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22243	439512	5.06

Instrument :
BNA_P
ClientSampleId :
DFTPP