
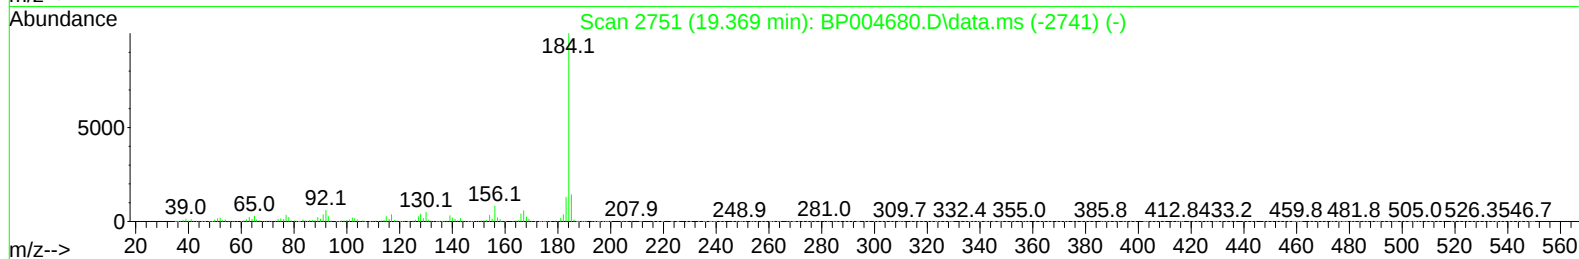
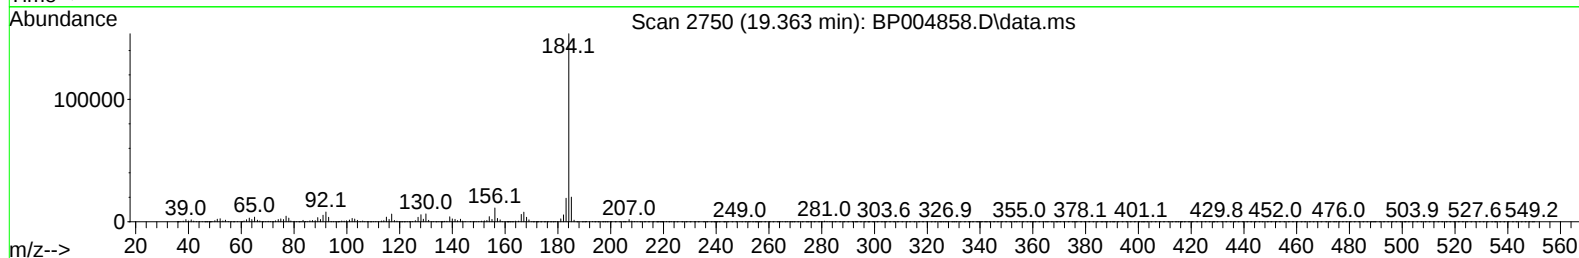


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022621\
 Data File : BP004858.D
 Acq On : 26 Feb 2021 12:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 13:29:19 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 26 13:23:29 2021
 Response via : Initial Calibration

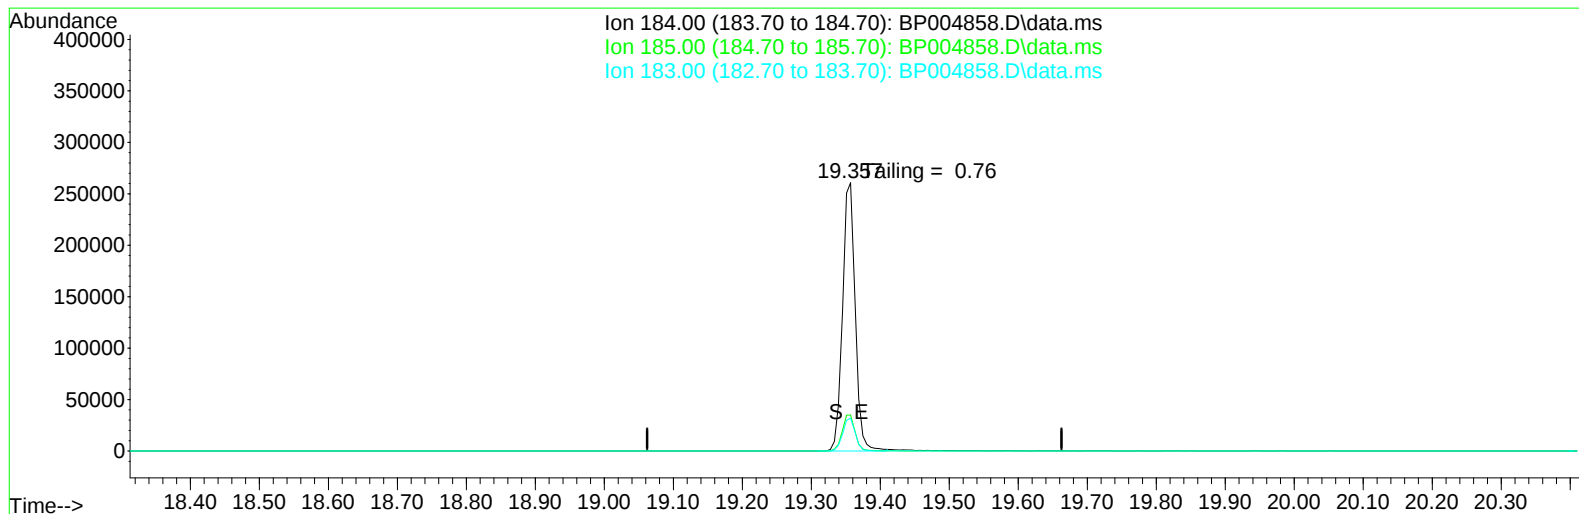

TIC: BP004858.D\data.ms

(77) Benzidine




19.362min (-19.362) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	14.40	0.00#
183.00	12.00	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022621\
 Data File : BP004858.D
 Acq On : 26 Feb 2021 12:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 13:29:19 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 26 13:23:29 2021
 Response via : Initial Calibration

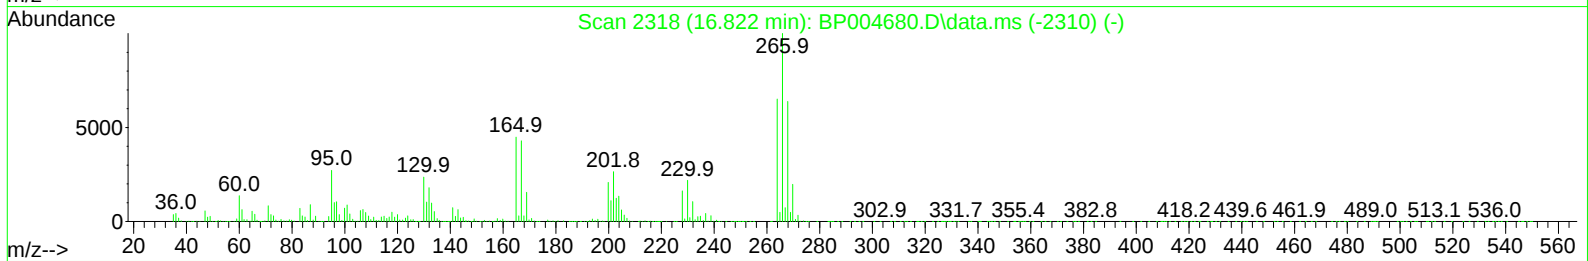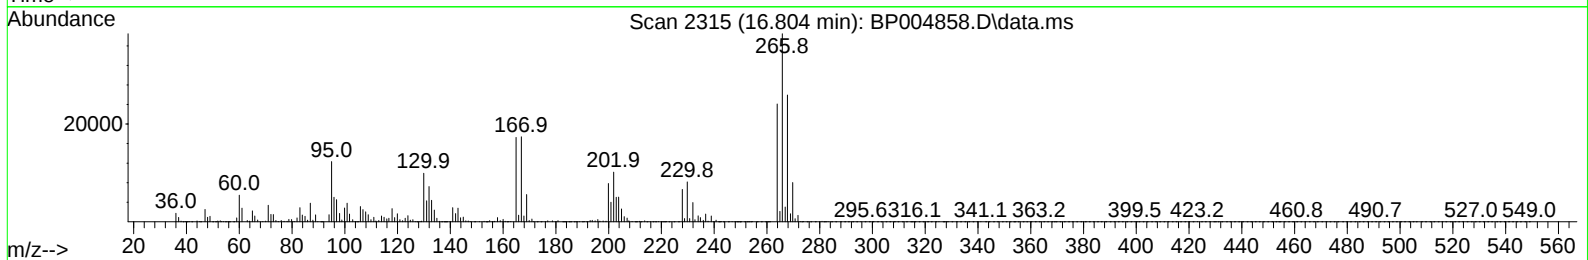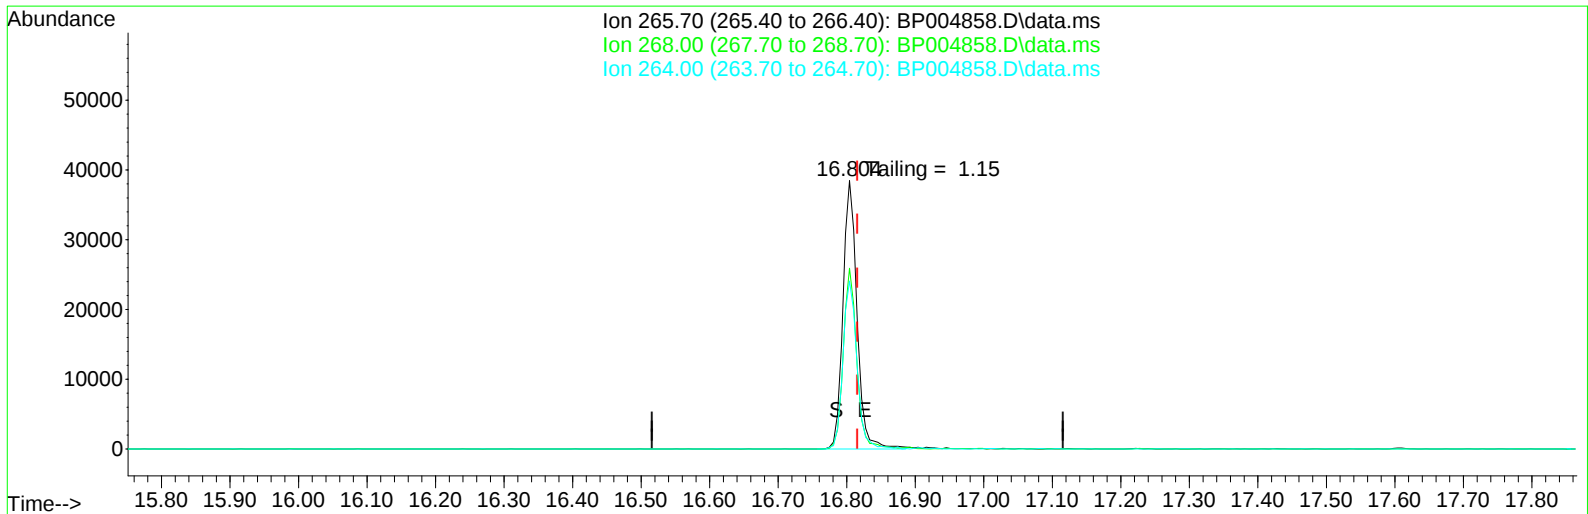

TIC: BP004858.D\data.ms

(70) Pentachlorophenol (C)

16.804min (-0.011) 1095006.19 ng

response 51577

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	67.39
264.00	63.30	62.61
0.00	0.00	0.00