
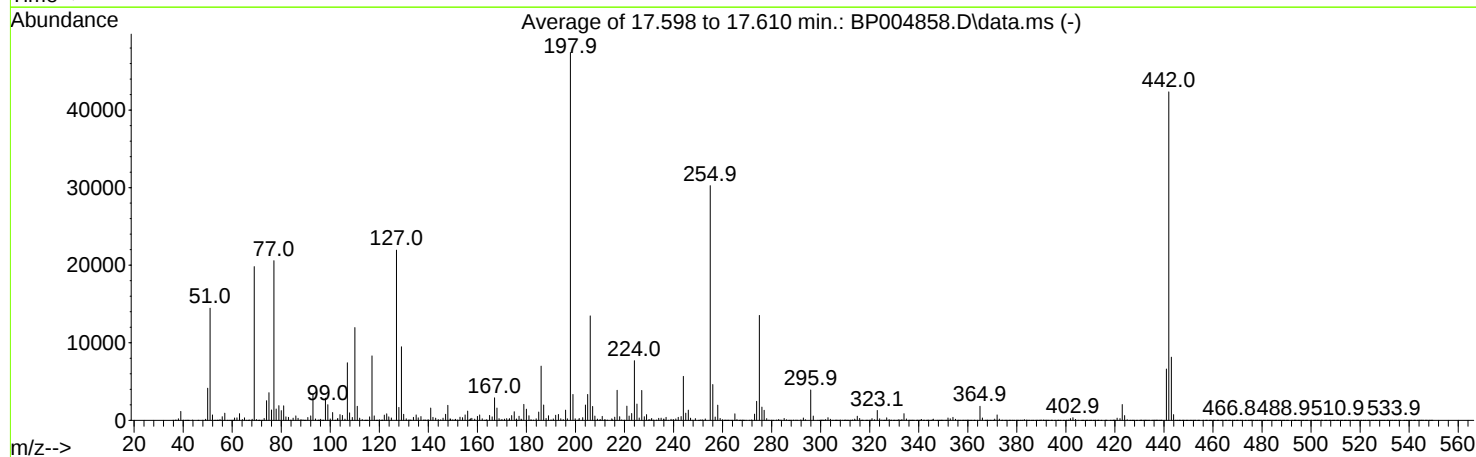


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022621\
 Data File : BP004858.D
 Acq On : 26 Feb 2021 12:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 26 17:41:20 2021

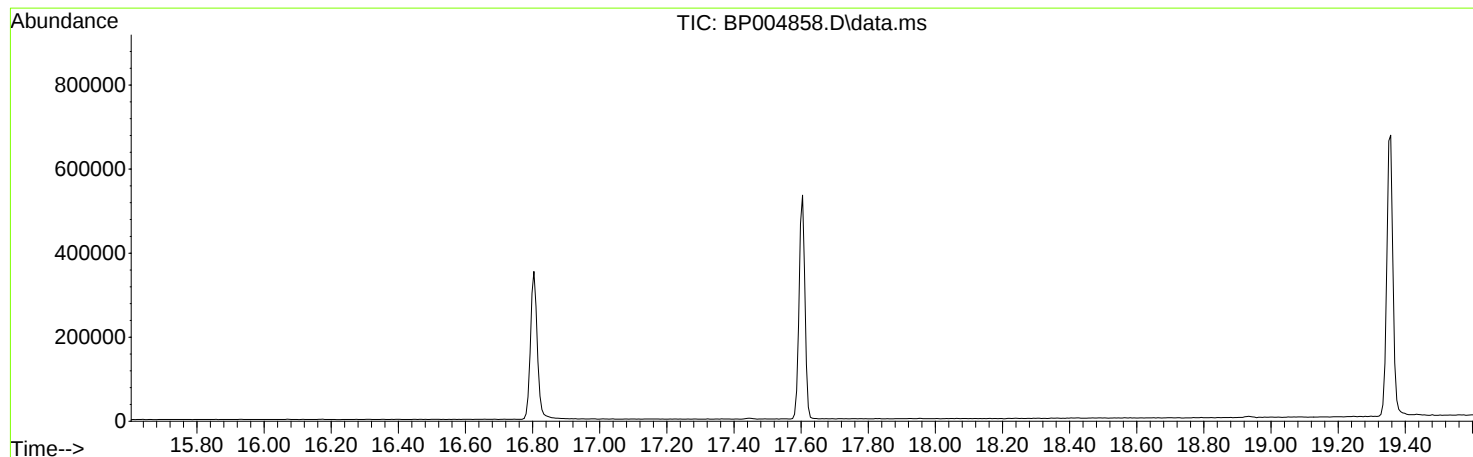

AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	14466	PASS
68	69	0.00	2	0.7	144	PASS
69	198	0.00	100	41.8	19822	PASS
70	69	0.00	2	0.5	107	PASS
127	198	10	80	46.3	21947	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	47419	PASS
199	198	5	9	7.0	3332	PASS
275	198	10	60	28.6	13539	PASS
365	198	1	100	3.8	1821	PASS
441	198	0.01	100	14.0	6627	PASS
442	442	100	100	100.0	42352	PASS
443	442	15	24	19.2	8142	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/26/2021	BNA_P	<u>BP004858.D</u>
Compound Name	Response	Retention Time
DDT	180750	20.55
DDD	831	20.13
DDE	418	19.63
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1249	181999	0.69

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022621\
 Data File : BP004858.D
 Acq On : 26 Feb 2021 12:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Feb 26 13:29:19 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 26 13:23:29 2021
 Response via : Initial Calibration

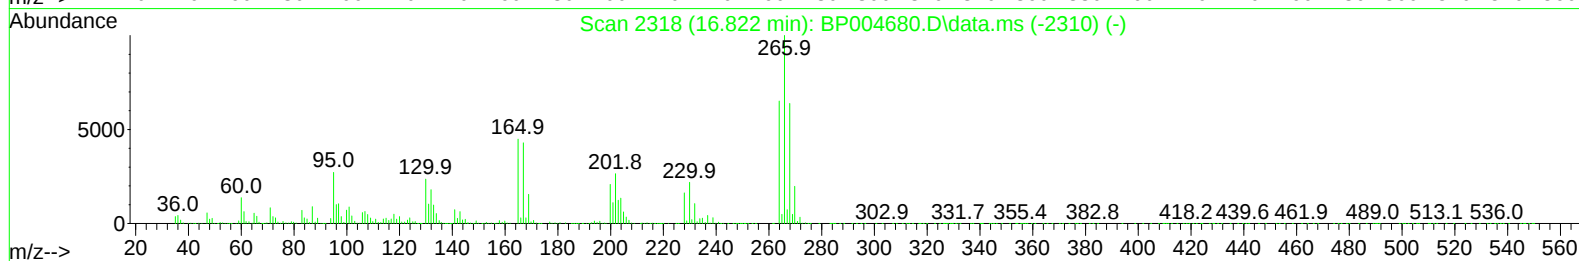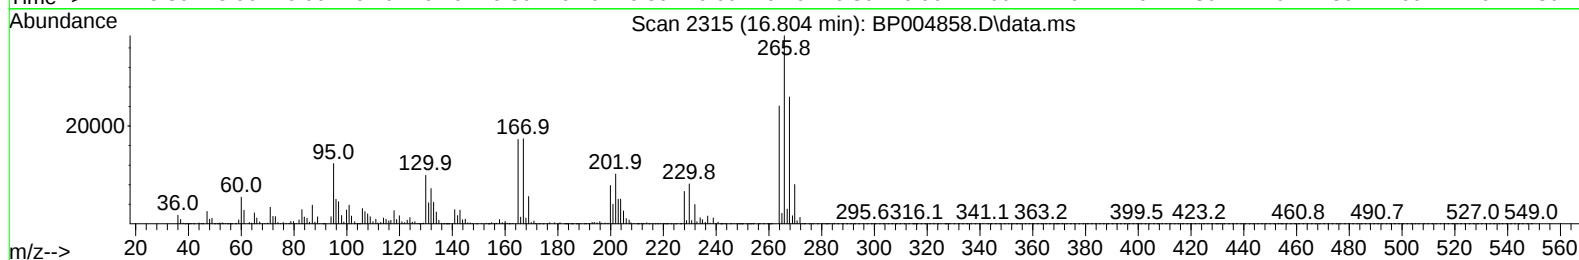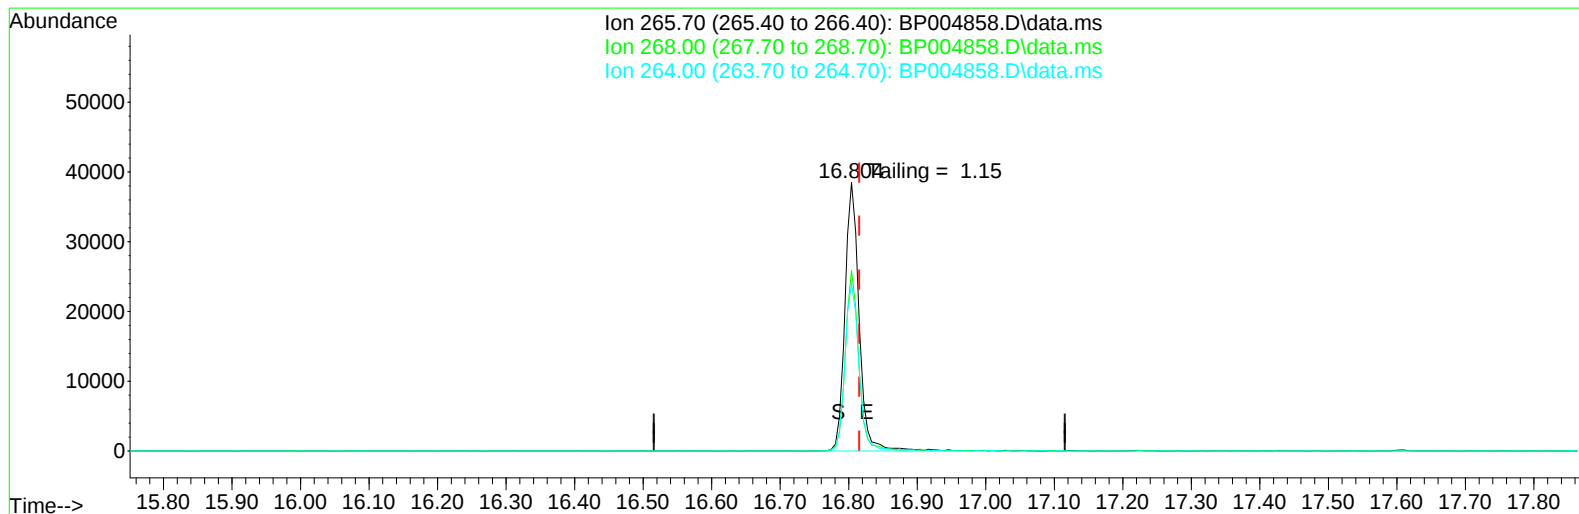

TIC: BP004858.D\data.ms

(70) Pentachlorophenol (C)

16.804min (-0.011) 1095006.19 ng




response 51577

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	67.39
264.00	63.30	62.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022621\
 Data File : BP004858.D
 Acq On : 26 Feb 2021 12:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Feb 26 13:29:19 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 26 13:23:29 2021
 Response via : Initial Calibration

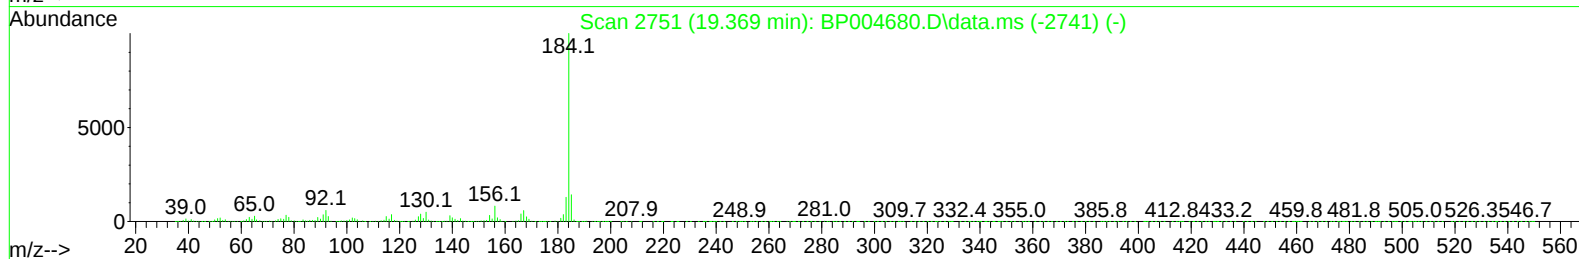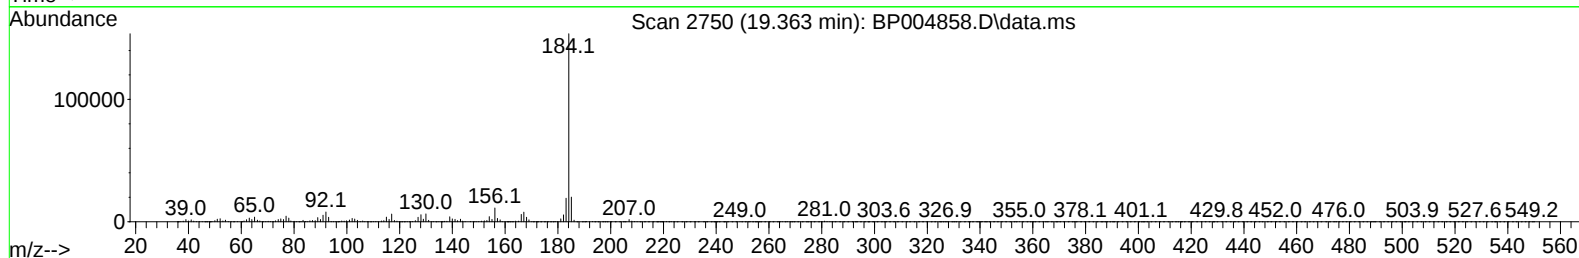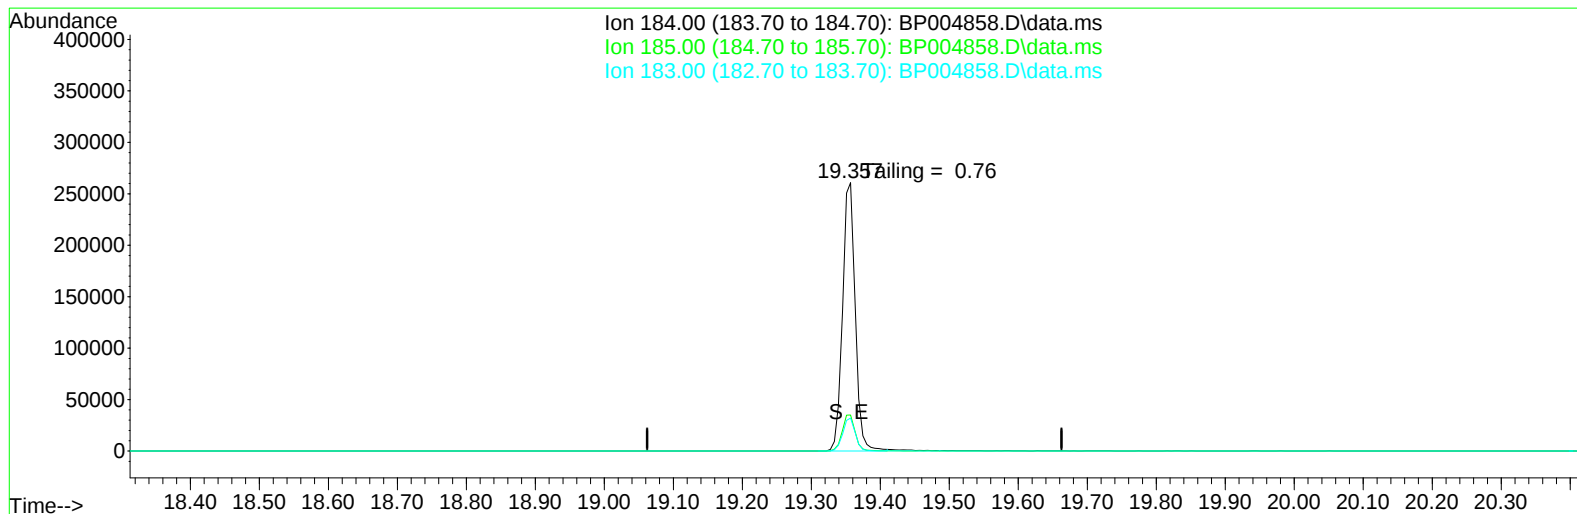

TIC: BP004858.D\data.ms

(77) Benzidine

19.362min (-19.362) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	14.40	0.00#
183.00	12.00	0.00#
0.00	0.00	0.00