
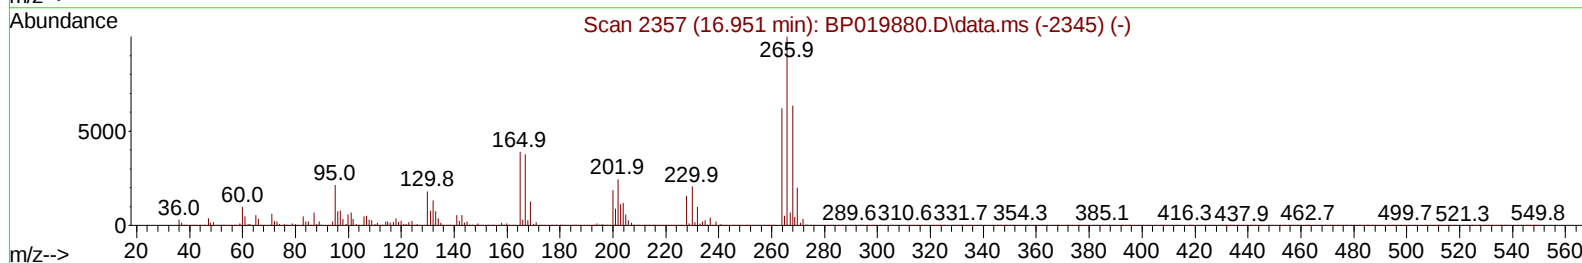
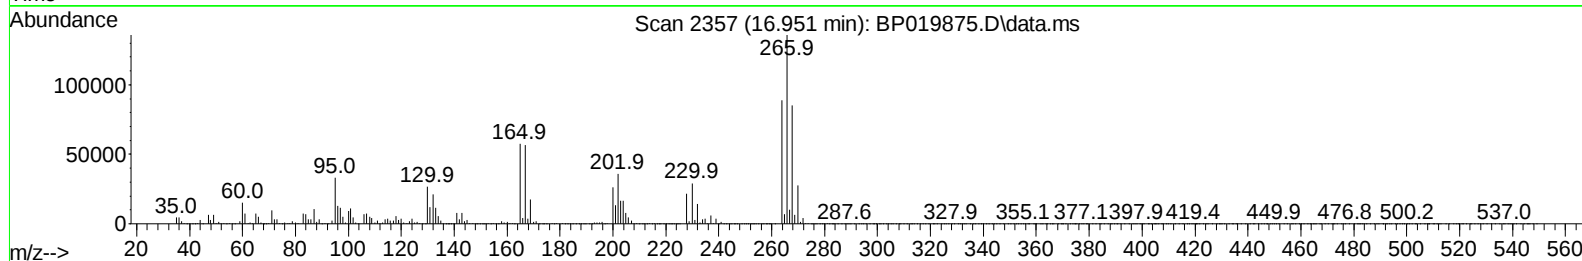


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022624\
Data File : BP019875.D
Acq On : 26 Feb 2024 12:58
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 27 02:10:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 02:05:05 2024
Response via : Initial Calibration

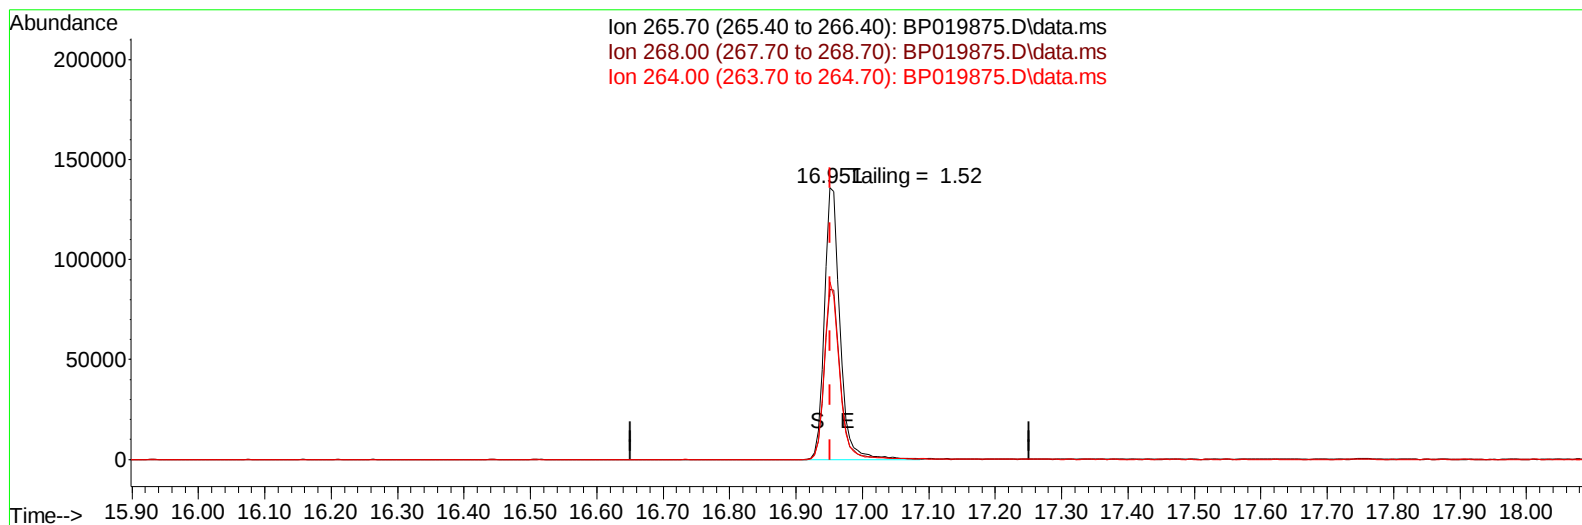

TIC: BP019875.D\data.ms

(70) Pentachlorophenol (C)




16.951min (+ 0.000) 748974.56 ng

response 221468

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	62.58
264.00	62.10	65.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022624\
Data File : BP019875.D
Acq On : 26 Feb 2024 12:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 27 02:10:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP022624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 02:05:05 2024
Response via : Initial Calibration

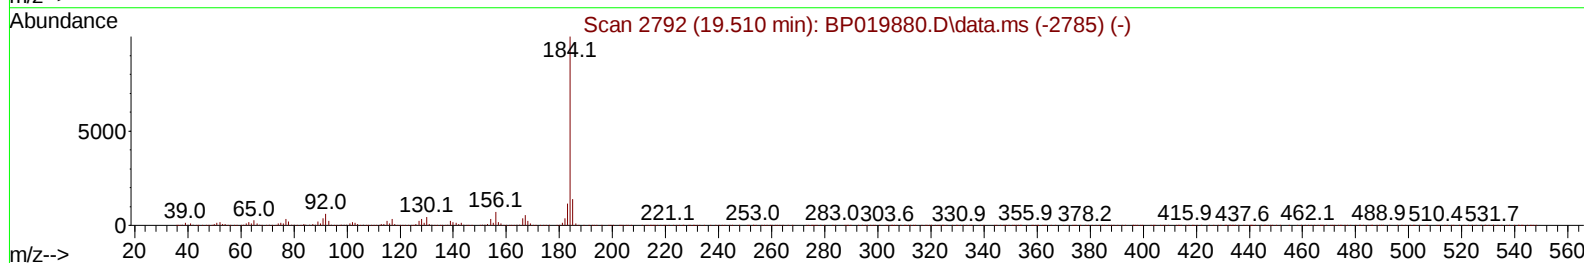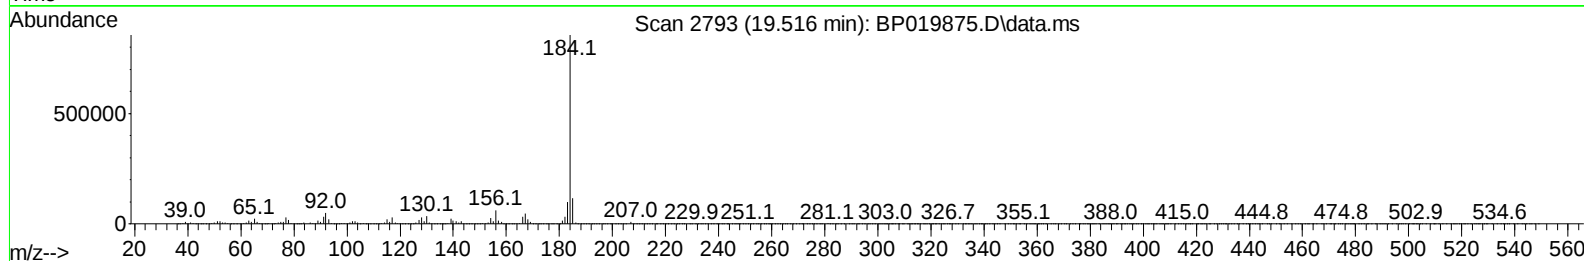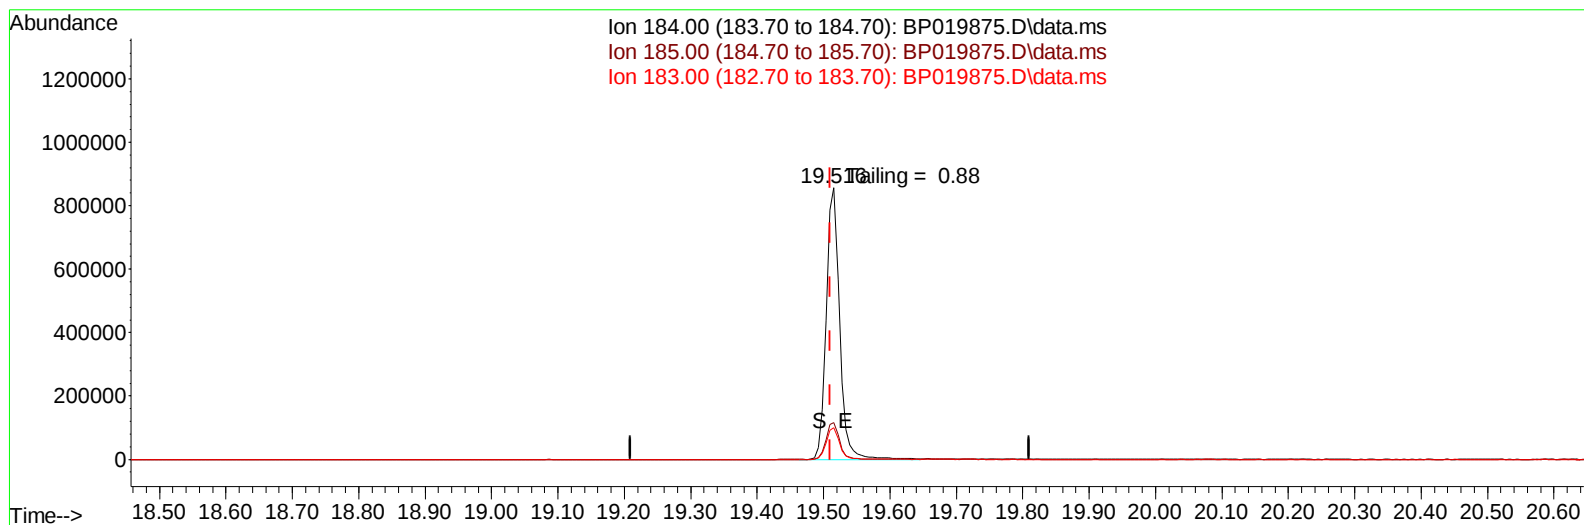

TIC: BP019875.D\data.ms

(77) Benzidine**19.516min (+ 0.006) 572536.29 ng****response 1184118**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.55
183.00	11.60	11.68
0.00	0.00	0.00